

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM111318\
 Data File : BM017642.D
 Acq On : 14 Nov 2018 04:04
 Operator : MJ/SJ
 Sample : PB114777BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB114777BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM111218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.793	302	307	313	rBV	182107	249756	2.84%	0.480%
2	5.240	376	383	395	rBV	2626383	3715830	42.28%	7.144%
3	6.798	642	648	662	rBV	2376841	3862278	43.94%	7.425%
4	7.151	701	708	722	rBV	2569753	3999873	45.51%	7.690%
5	7.616	779	787	798	rBV	724989	1166919	13.28%	2.243%
6	7.928	830	840	849	rBV	2776561	4513006	51.34%	8.677%
7	8.769	975	983	1007	rBV	2079850	3549144	40.38%	6.823%
8	10.386	1251	1258	1277	rBV	778855	1573619	17.90%	3.025%
9	12.874	1673	1681	1701	rBV	5241986	8233383	93.67%	15.829%
10	14.257	1910	1916	1934	rBV2	1150102	2031472	23.11%	3.906%
11	15.757	2165	2171	2191	rBV	2347696	3809261	43.34%	7.324%
12	17.015	2377	2385	2400	rBV	1363135	2335405	26.57%	4.490%
13	19.362	2780	2784	2788	rBV	134780	150676	1.71%	0.290%
14	19.656	2828	2834	2846	rBV	7090772	8789604	100.00%	16.899%
15	20.415	2959	2963	2968	rBV2	100790	116614	1.33%	0.224%
16	21.215	3094	3099	3110	rBV	1535351	2245208	25.54%	4.317%
17	23.409	3466	3472	3486	rVB	787079	1671682	19.02%	3.214%


Sum of corrected areas: 52013730

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM111318\
Data File : BM017642.D
Acq On : 14 Nov 2018 04:04
Operator : MJ/SJ
Sample : PB114777BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB114777BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM111218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

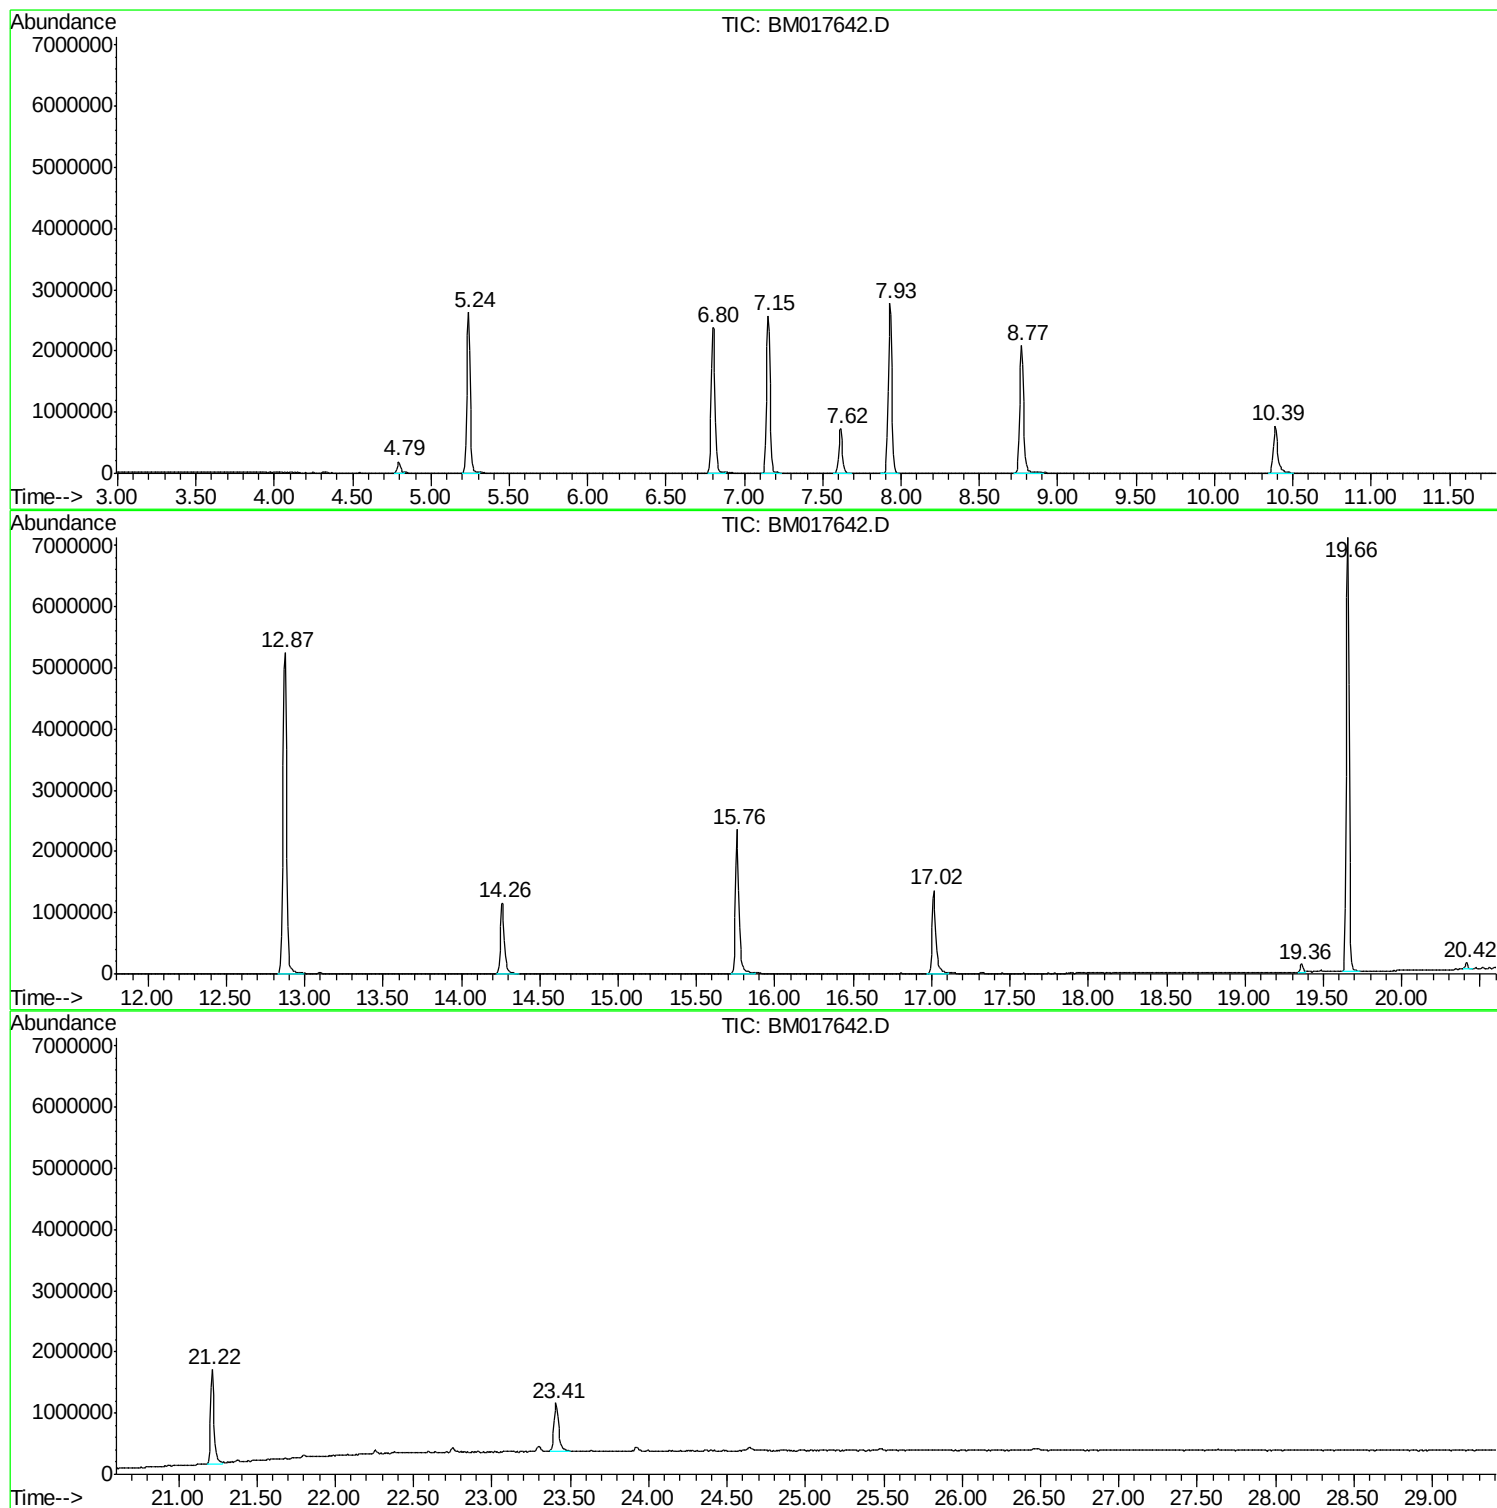

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM111318\
Data File : BM017642.D
Acq On : 14 Nov 2018 04:04
Operator : MJ/SJ
Sample : PB114777BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB114777BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM111218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.79	4.28 ng	249756	1,4-Dichlorobenzene-d4	7.62

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	40
2			2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	35
3			Dimethadione	129	C5H7NO3	000695-53-4	33
4			Butyl aldoxime, 3-methyl-, syn-	101	C5H11NO	005780-40-5	17
5			Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9

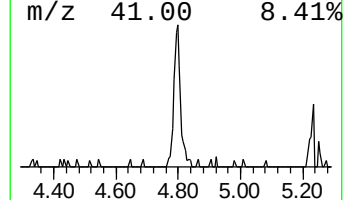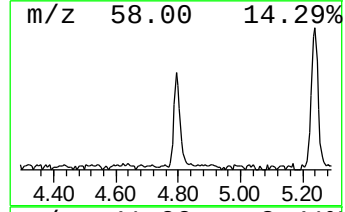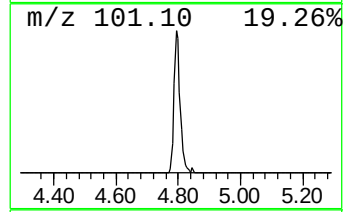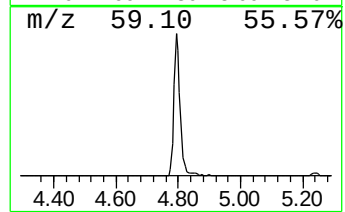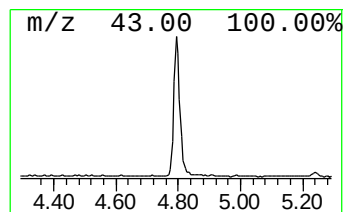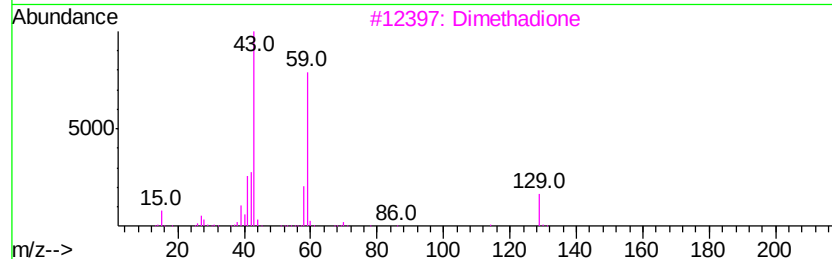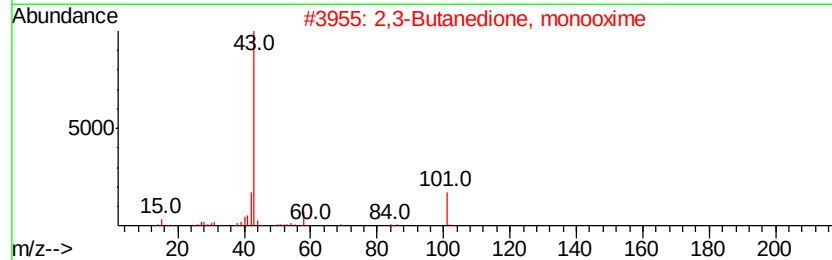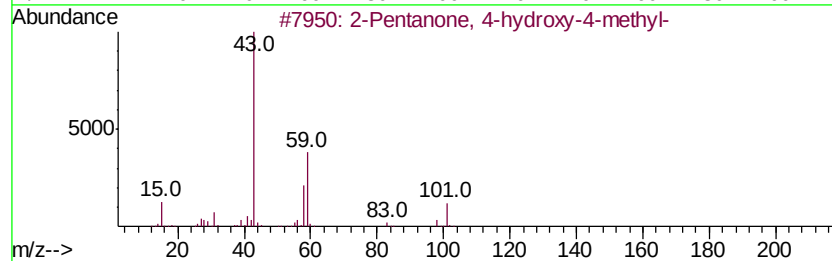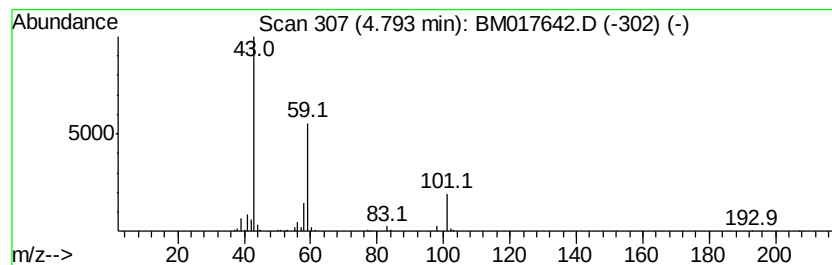

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM111318\
Data File : BM017642.D
Acq On : 14 Nov 2018 04:04
Operator : MJ/SJ
Sample : PB114777BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB114777BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM111218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown7.15 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.15	68.55 ng	3999870	1,4-Dichlorobenzene-d4	7.62

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	12
2		(5-METHYL-2-PYRIDYL)ACETONITRILE	132	C8H8N2	1000241-93-9	10
3		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	9
4		Benzene, 1,3,5-trifluoro-	132	C6H3F3	000372-38-3	9
5		1,2,3-Trifluorobenzene	132	C6H3F3	001489-53-8	9

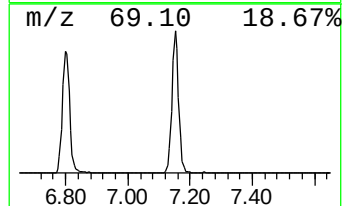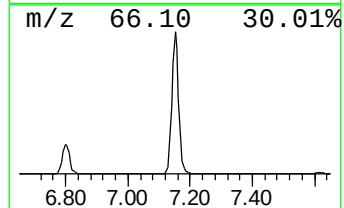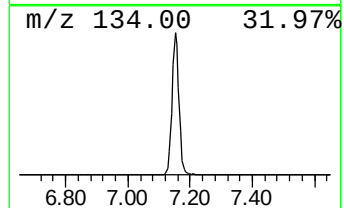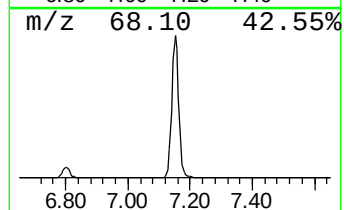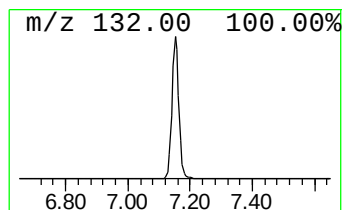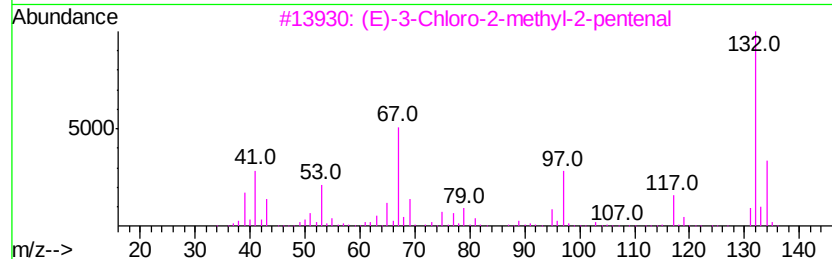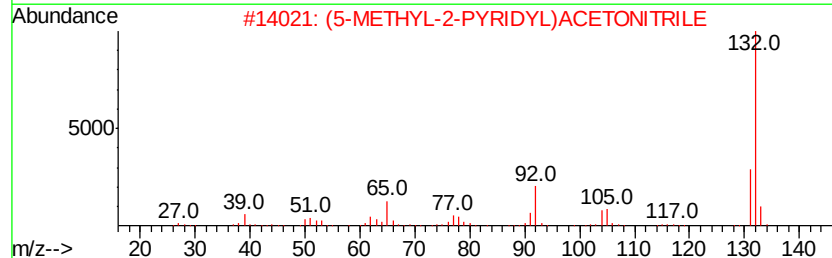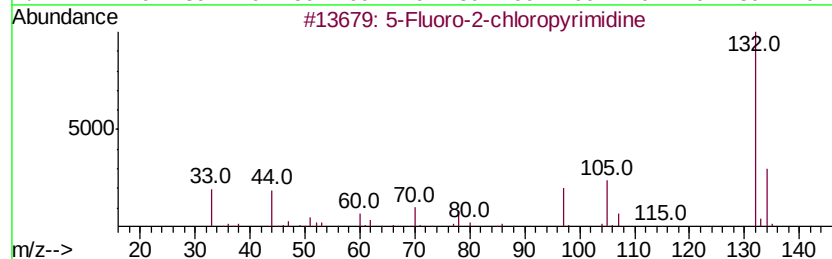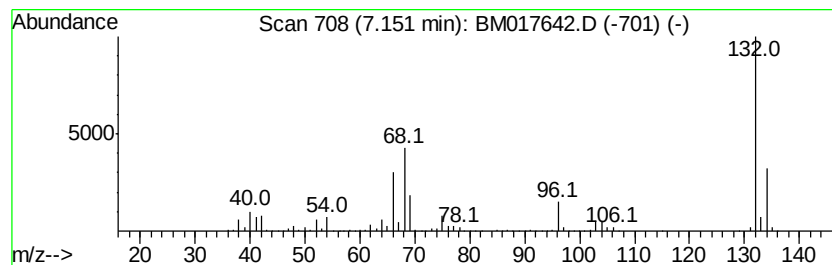

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM111318\
Data File : BM017642.D
Acq On : 14 Nov 2018 04:04
Operator : MJ/SJ
Sample : PB114777BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB114777BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM111218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	4.79	4.3	ng	249756	1	7.62	1166920	20.0
unknown7.15	7.15	68.5	ng	3999870	1	7.62	1166920	20.0