


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM111318\
 Data File : BM017623.D
 Acq On : 13 Nov 2018 16:32
 Operator : MJ/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM111218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Nov 12 18:37:25 2018

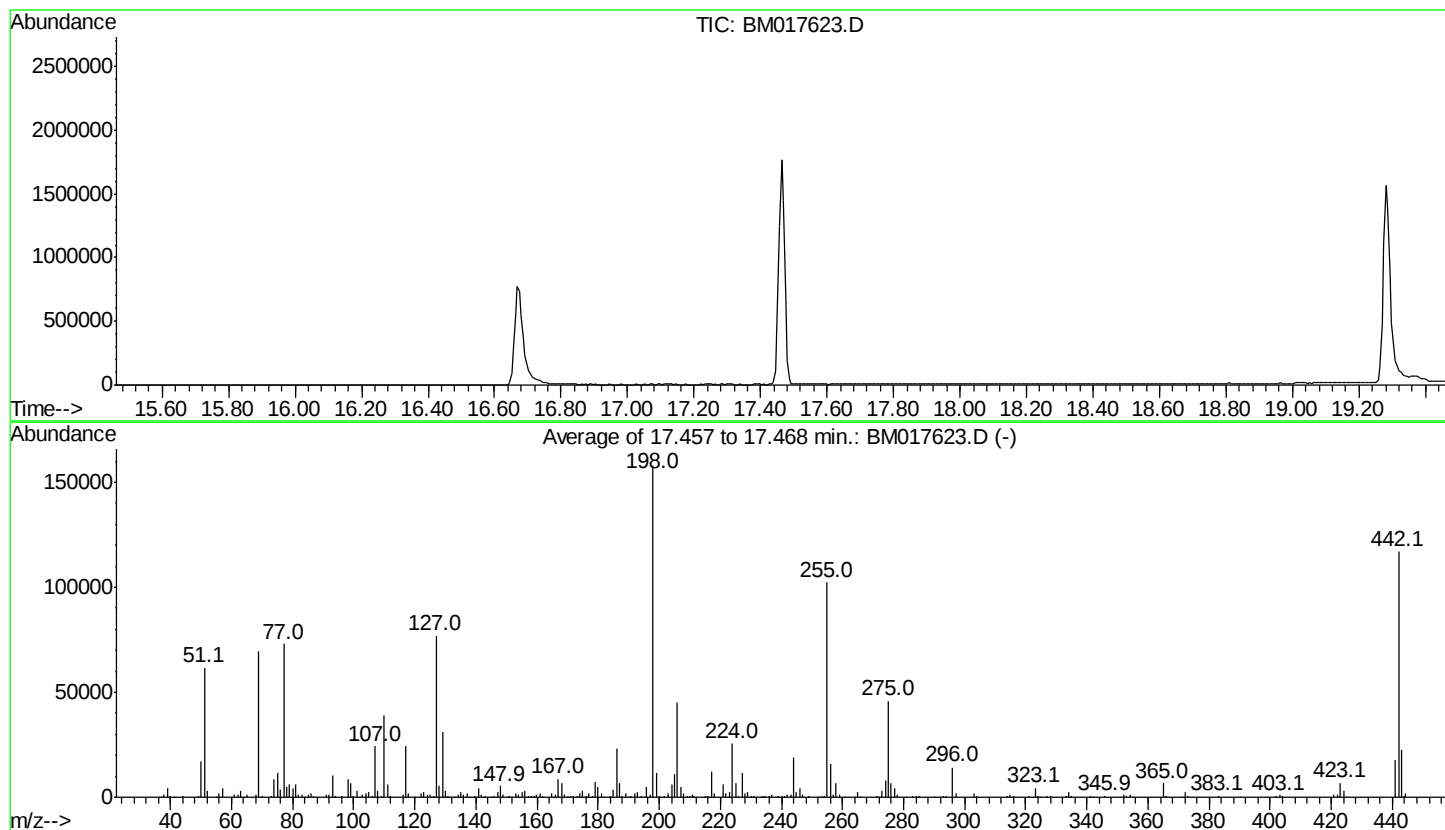

AutoFind: Scans 2460, 2461, 2462; Background Corrected with Scan 2454

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.0	61637	PASS
68	69	0.00	2	1.9	1324	PASS
69	198	0.00	100	43.9	69362	PASS
70	69	0.00	2	0.5	373	PASS
127	198	10	80	48.7	76826	PASS
197	198	0.00	2	0.6	1009	PASS
198	198	100	100	100.0	157898	PASS
199	198	5	9	7.3	11469	PASS
275	198	10	60	29.0	45784	PASS
365	198	1	100	4.2	6579	PASS
441	198	0.01	100	11.3	17904	PASS
442	198	50	100	74.0	116776	PASS
443	442	15	24	19.2	22413	PASS