

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM111319\
 Data File : BM023692.D
 Acq On : 13 Nov 2019 12:19
 Operator : JU
 Sample : K5579-09
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BEJP7

Quant Time: Nov 13 13:54:17 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM11119MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 13 13:51:42 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.54	152	323423	20.00	ng/ul	0.00
18) Naphthalene-d8	10.32	136	1545614	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.20	164	1142532	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.94	188	2589829	20.00	ng/ul	0.00
78) Chrysene-d12	21.14	240	2279274	20.00	ng/ul	0.00
86) Perylene-d12	23.31	264	2041849	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.08	96	47965	6.11	ng/uL	0.00
5) Phenol-d5	6.73	99	281677	9.55	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.89	67	606154	35.78	ng/ul	0.00
9) 2-Chlorophenol-d4	7.08	132	677300	31.71	ng/ul	0.00
13) 4-Methylphenol-d8	8.26	113	527311	22.42	ng/ul	0.00
19) Nitrobenzene-d5	8.69	128	432357	39.08	ng/ul	0.00
22) 2-Nitrophenol-d4	9.41	143	502301	43.20	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.95	165	954360	35.99	ng/ul	0.00
29) 4-Chloroaniline-d4	10.46	131	66638	2.29	ng/ul	0.00
44) Dimethylphthalate-d6	13.62	166	3430443	38.50	ng/ul	0.00
47) Acenaphthylene-d8	13.89	160	3903677	38.39	ng/ul	0.00
52) 4-Nitrophenol-d4	14.42	143	112884	7.42	ng/ul	0.00
58) Fluorene-d10	15.20	176	3047109	38.73	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.33	200	475987	31.77	ng/ul	0.00
71) Anthracene-d10	17.04	188	4985014	40.58	ng/ul	0.00
79) Pyrene-d10	19.35	212	5495479	46.24	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.17	264	4502912	41.91	ng/ul	0.00


Target Compounds					Qvalue
45) Dimethylphthalate	13.66	163	211302	2.420 ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM111319\
Data File : BM023692.D
Acq On : 13 Nov 2019 12:19
Operator : JU
Sample : K5579-09
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BEJP7

Quant Time: Nov 13 13:54:17 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM11119MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 13 13:51:42 2019
Response via : Initial Calibration

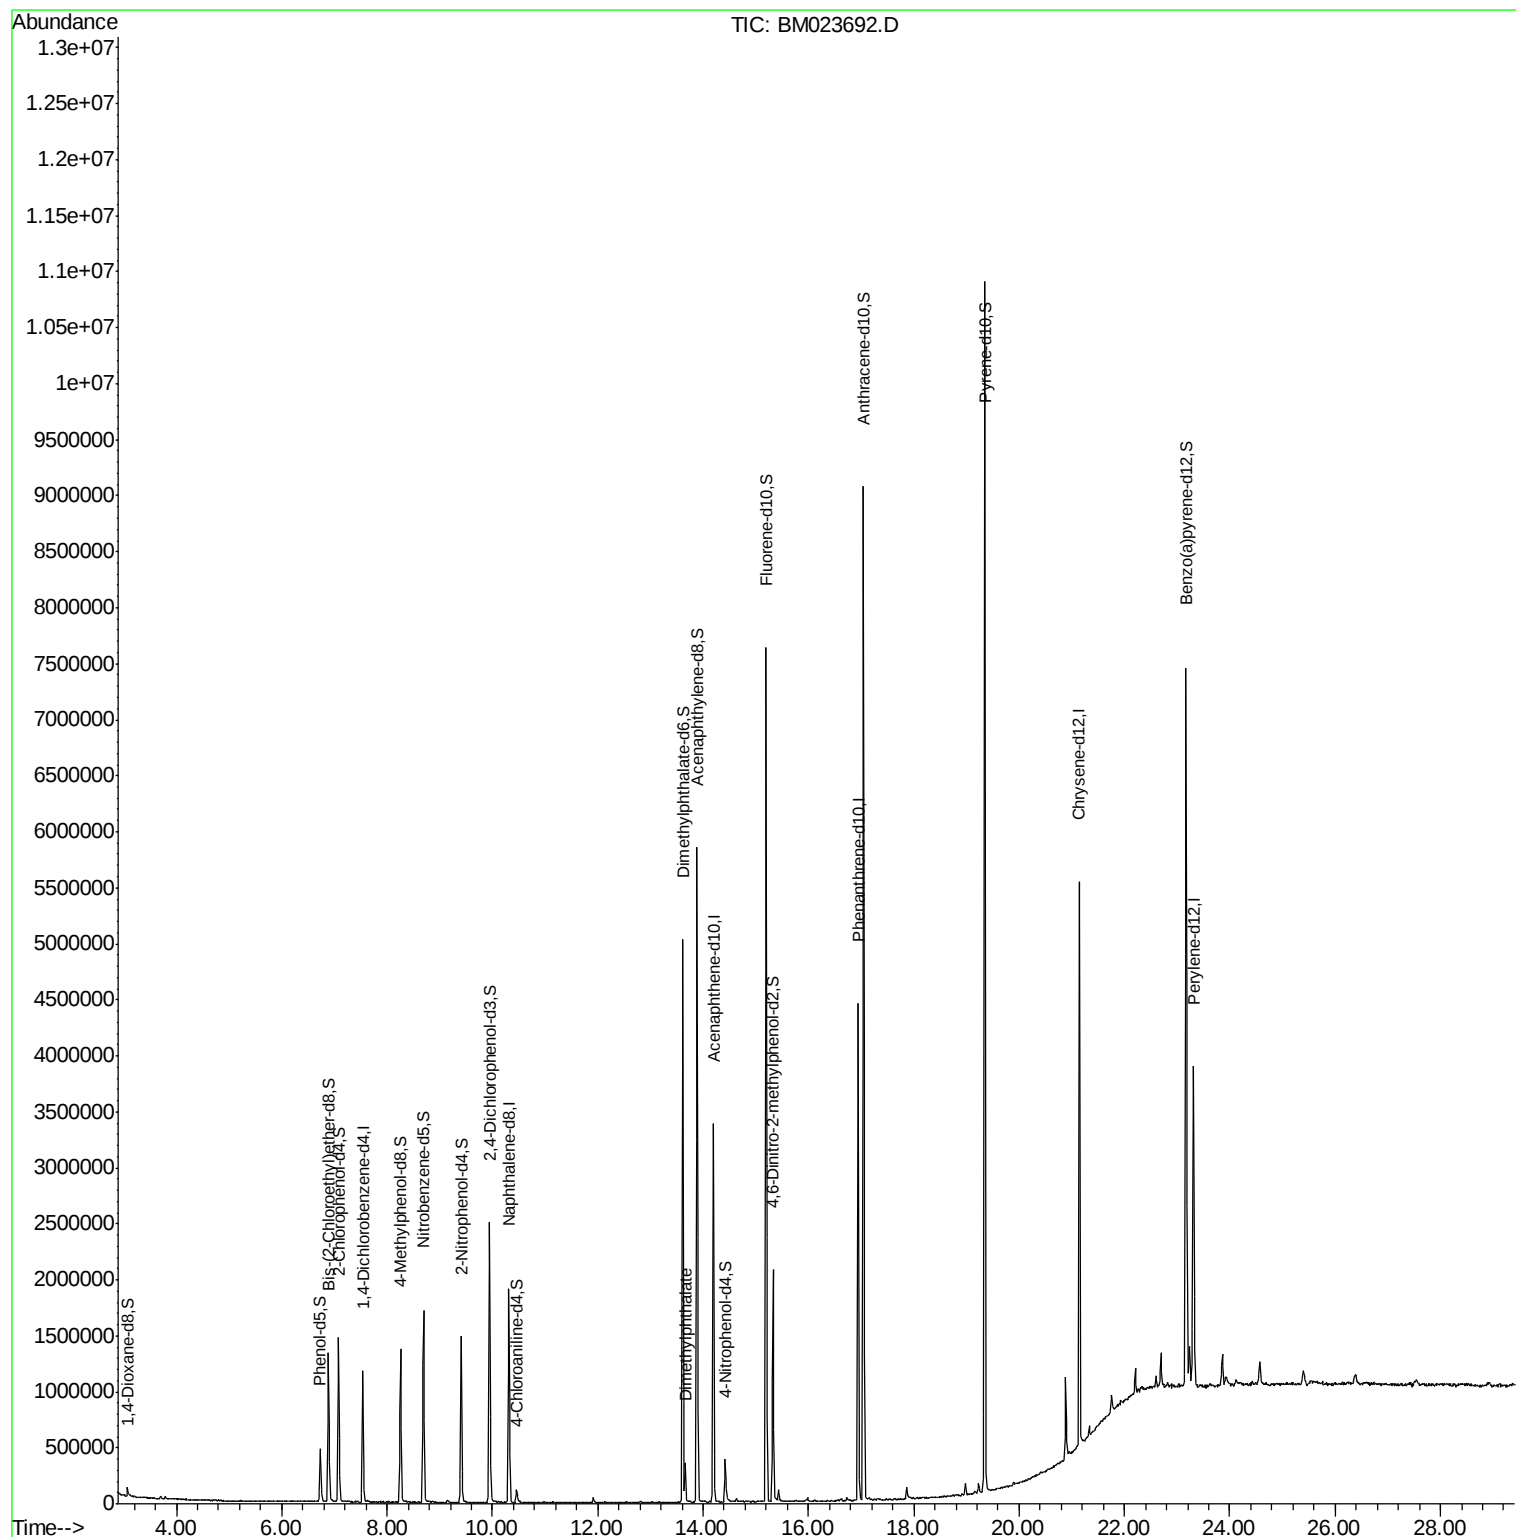

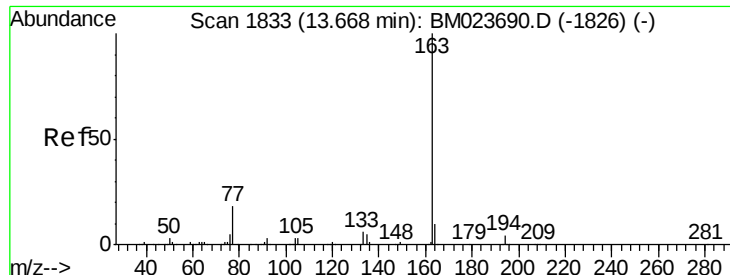

#45

Dimethylphthalate

Concen: 2.420 ng/ul

RT: 13.66 min Scan# 1832

Delta R.T. -0.01 min

Lab File: BM023692.D

Acq: 13 Nov 2019 12:19

Instrument :

BNA_M

ClientSampleId :

BEJP7



Tgt Ion:163 Resp: 211302

Ion Ratio Lower Upper

163 100

194 4.7 3.4 5.2

164 9.4 8.0 12.0

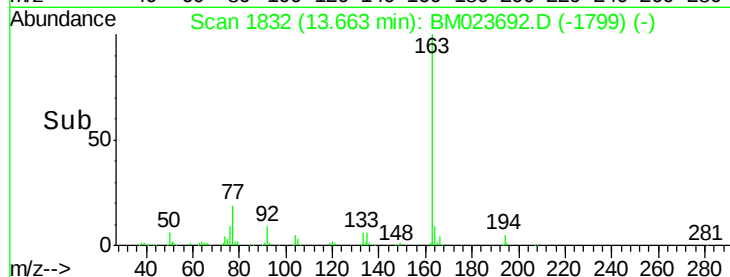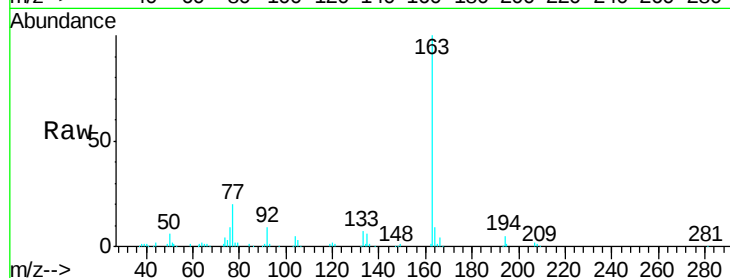

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

