

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM111319\
 Data File : BM023696.D
 Acq On : 13 Nov 2019 14:43
 Operator : JU
 Sample : K5579-11
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BEJP9

Quant Time: Nov 13 15:21:07 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM11119MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 13 13:51:42 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.54	152	362908	20.00	ng/ul	0.00
18) Naphthalene-d8	10.32	136	1715775	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.20	164	1257277	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.94	188	2875951	20.00	ng/ul	0.00
78) Chrysene-d12	21.14	240	2570004	20.00	ng/ul	0.00
86) Perylene-d12	23.31	264	2289355	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.07	96	49319	5.60	ng/uL	0.00
5) Phenol-d5	6.73	99	216284	6.54	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.89	67	511368	26.90	ng/ul	0.00
9) 2-Chlorophenol-d4	7.08	132	565792	23.61	ng/ul	0.00
13) 4-Methylphenol-d8	8.26	113	416470	15.78	ng/ul	0.00
19) Nitrobenzene-d5	8.69	128	368686	30.02	ng/ul	0.00
22) 2-Nitrophenol-d4	9.41	143	426314	33.03	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.95	165	813266	27.63	ng/ul	0.00
29) 4-Chloroaniline-d4	10.46	131	54003	1.67	ng/ul	0.00
44) Dimethylphthalate-d6	13.62	166	2927602	29.86	ng/ul	0.00
47) Acenaphthylene-d8	13.89	160	3328253	29.75	ng/ul	0.00
52) 4-Nitrophenol-d4	14.42	143	98170	5.87	ng/ul	0.00
58) Fluorene-d10	15.20	176	2684737	31.01	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.33	200	445965	26.81	ng/ul	0.00
71) Anthracene-d10	17.04	188	4959140	36.35	ng/ul	0.00
79) Pyrene-d10	19.35	212	5505369	41.09	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.17	264	4529127	37.60	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.66	163	161024	1.676	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM111319\
Data File : BM023696.D
Acq On : 13 Nov 2019 14:43
Operator : JU
Sample : K5579-11
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BEJP9

Quant Time: Nov 13 15:21:07 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM11119MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 13 13:51:42 2019
Response via : Initial Calibration

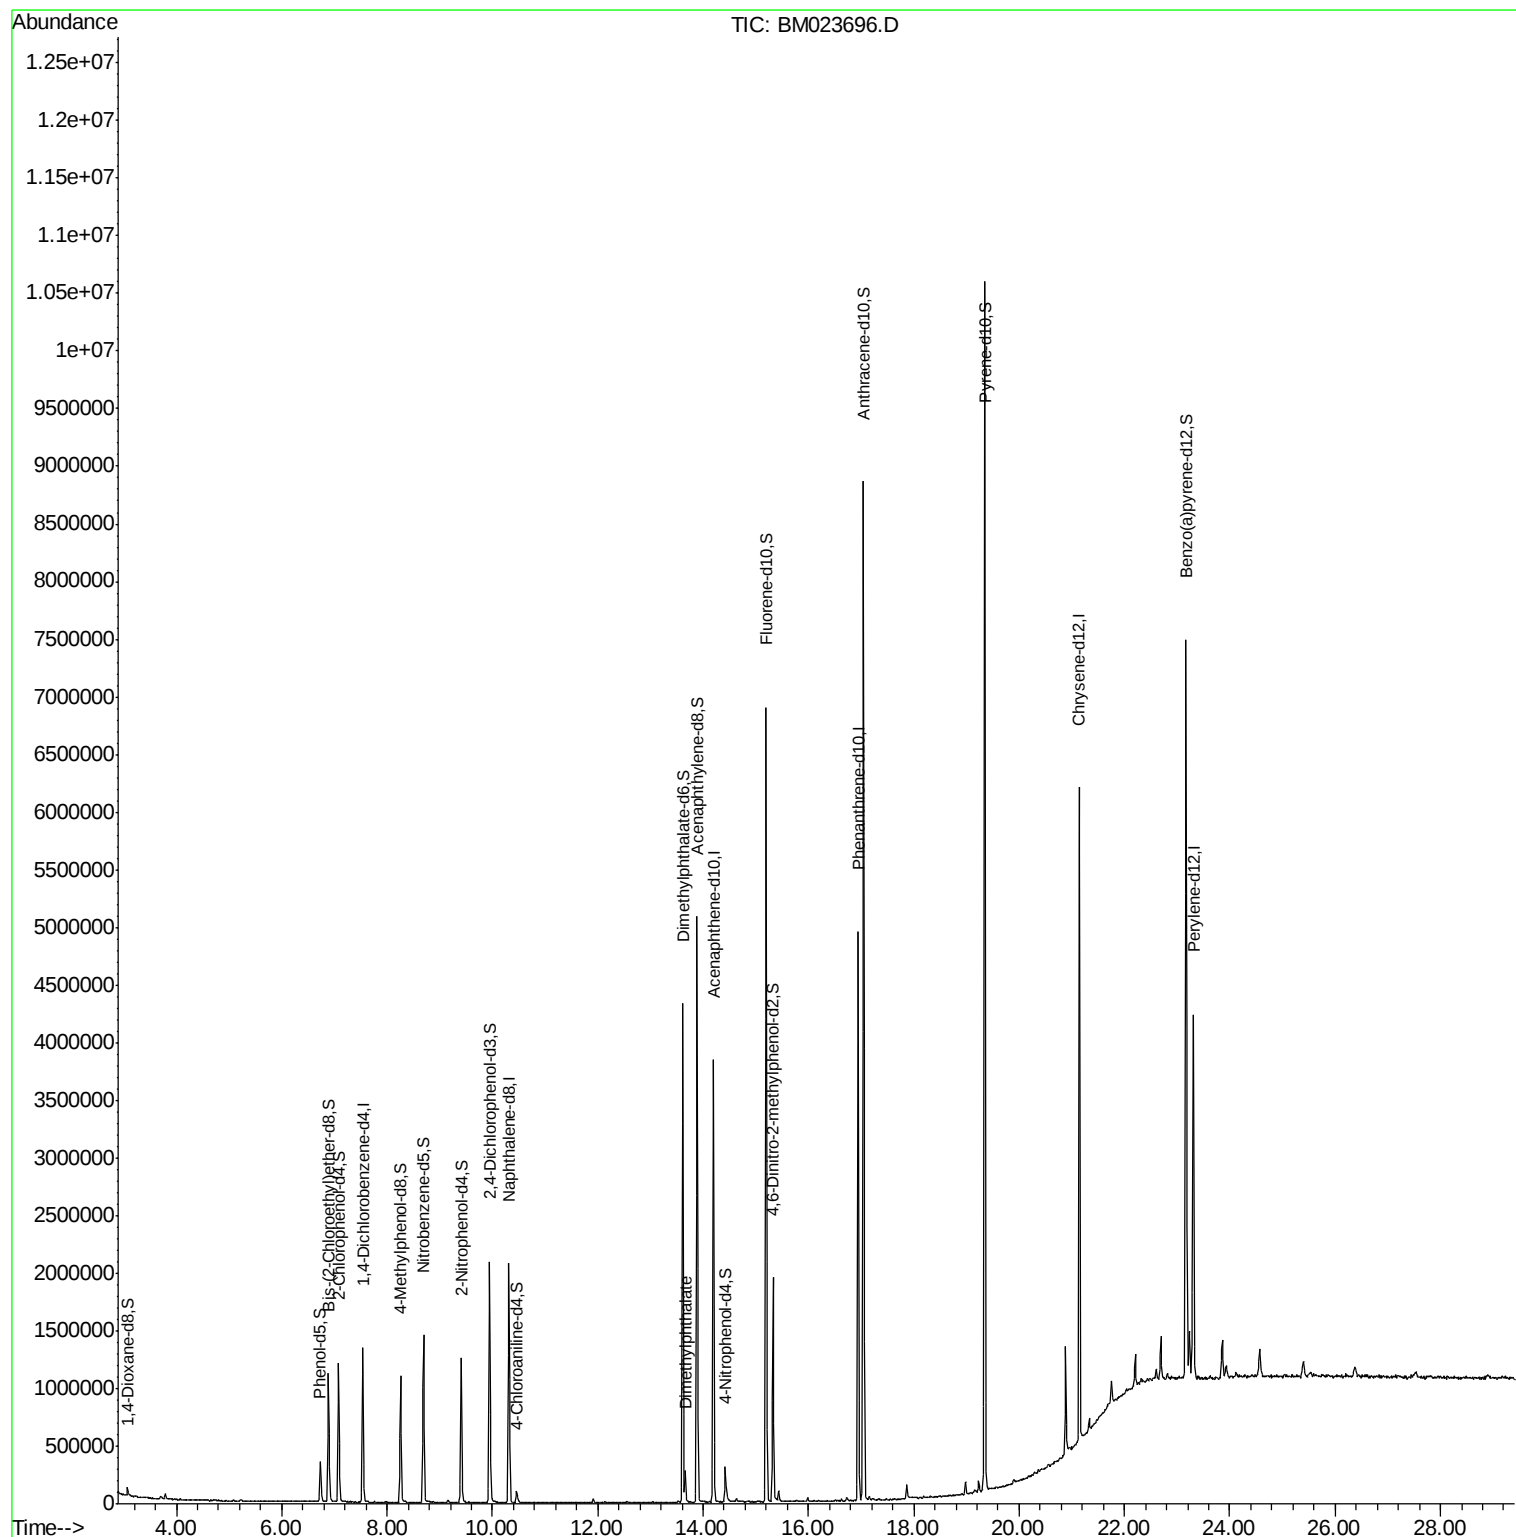

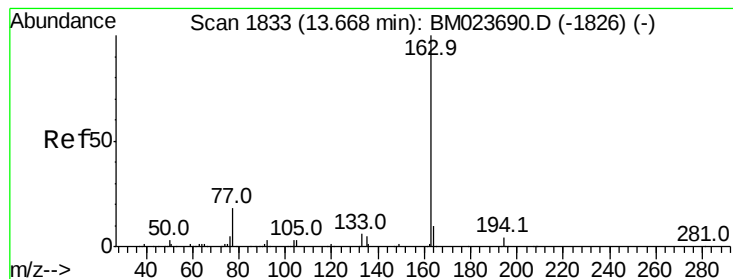

#45

Dimethylphthalate

Concen: 1.676 ng/ul

RT: 13.66 min Scan# 1832

Delta R.T. -0.01 min

Lab File: BM023696.D

Acq: 13 Nov 2019 14:43

Instrument :

BNA_M

ClientSampleId :

BEJP9

Tot Ion:163 Resp: 161024

Ion Ratio Lower Upper

163 100

194 4.3 3.4 5.2

164 10.7 8.0 12.0

