

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM111319\
 Data File : BM023705.D
 Acq On : 13 Nov 2019 20:07
 Operator : JU
 Sample : K5678-06
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JLM73

Quant Time: Nov 14 01:17:37 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM11119MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Nov 14 01:13:45 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.54	152	432655	20.00	ng/ul	0.00
18) Naphthalene-d8	10.32	136	2034284	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.19	164	1407804	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.94	188	2945744	20.00	ng/ul	0.00
78) Chrysene-d12	21.14	240	2033135	20.00	ng/ul	0.00
86) Perylene-d12	23.31	264	2039479	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.08	96	10931	1.04	ng/uL	0.00
5) Phenol-d5	6.73	99	362984	9.20	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.89	67	235598	10.40	ng/ul	0.00
9) 2-Chlorophenol-d4	7.07	132	312609	10.94	ng/ul	0.00
13) 4-Methylphenol-d8	8.26	113	343079	10.90	ng/ul	0.00
19) Nitrobenzene-d5	8.69	128	165287	11.35	ng/ul	0.00
22) 2-Nitrophenol-d4	9.41	143	188177	12.30	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.95	165	390741	11.20	ng/ul	0.00
29) 4-Chloroaniline-d4	10.46	131	83655	2.18	ng/ul	0.00
44) Dimethylphthalate-d6	13.62	166	1281241	11.67	ng/ul	0.00
47) Acenaphthylene-d8	13.88	160	1480657	11.82	ng/ul	0.00
52) 4-Nitrophenol-d4	14.43	143	47292	2.52	ng/ul	0.00
58) Fluorene-d10	15.19	176	1127681	11.63	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.33	200	105692	6.20	ng/ul	0.00
71) Anthracene-d10	17.04	188	1667828	11.94	ng/ul	0.00
79) Pyrene-d10	19.34	212	1657391	15.63	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.17	264	1270394	11.84	ng/ul	0.00


Target Compounds				Ovalue		
4) Benzaldehyde	6.69	77	31951	1.381	ng/ul	98
6) Phenol	6.76	94	49621	1.221	ng/ul	97
14) Acetophenone	8.36	105	55430	1.130	ng/ul	99
45) Dimethylphthalate	13.66	163	224386	2.086	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM111319\
Data File : BM023705.D
Acq On : 13 Nov 2019 20:07
Operator : JU
Sample : K5678-06
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JLM73

Quant Time: Nov 14 01:17:37 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM11119MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Nov 14 01:13:45 2019
Response via : Initial Calibration

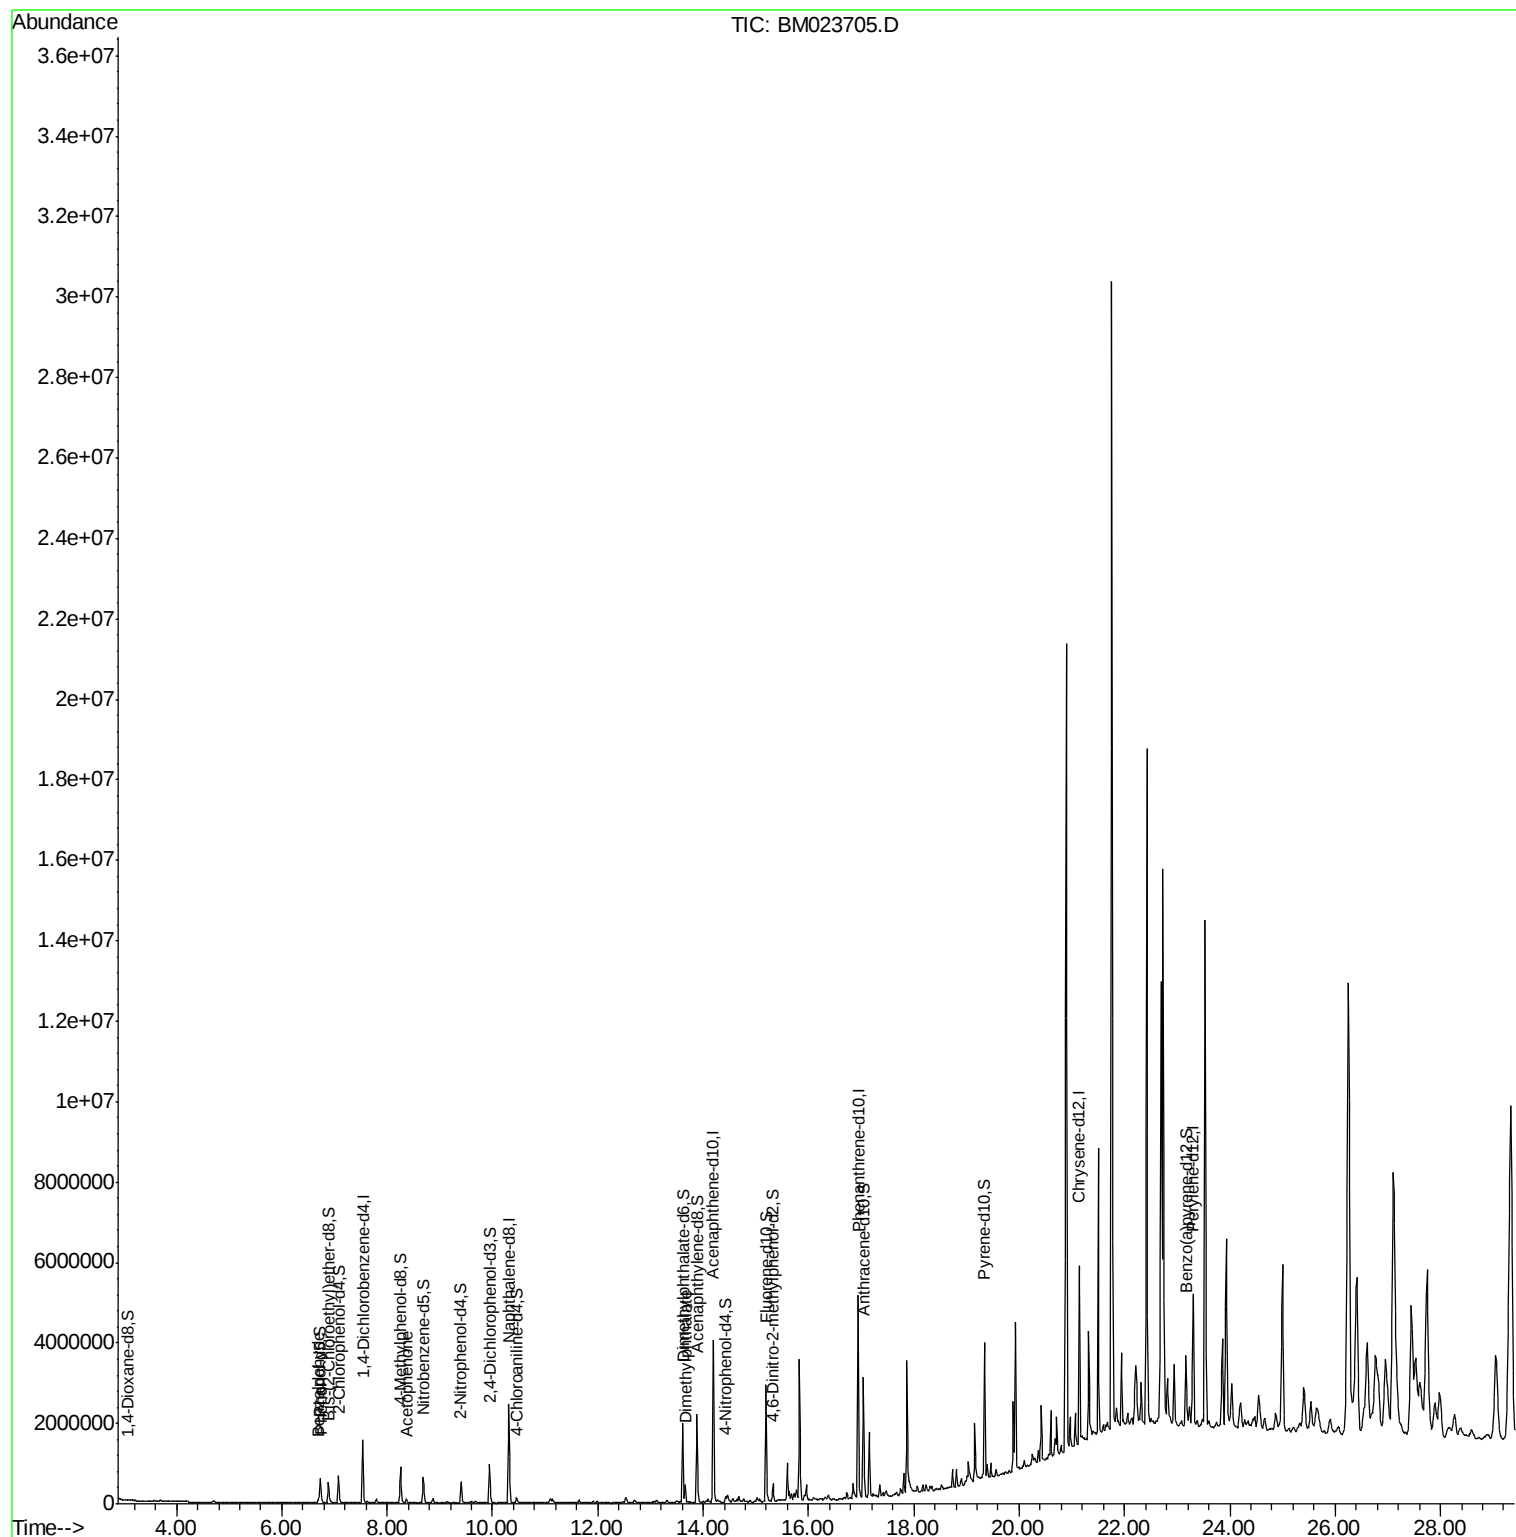

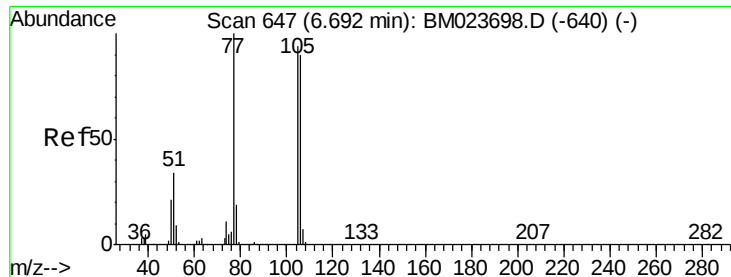

#4

Benzaldehyde

Concen: 1.381 ng/ul

RT: 6.69 min Scan# 647

Delta R.T. -0.00 min

Lab File: BM023705.D

Acq: 13 Nov 2019 20:07

Instrument :

BNA_M

ClientSampleId :

JLM73


Tot Ion: 77 Resp: 31951

Ion Ratio Lower Upper

77 100

105 92.7 75.9 113.9




106 89.9 70.2 105.4

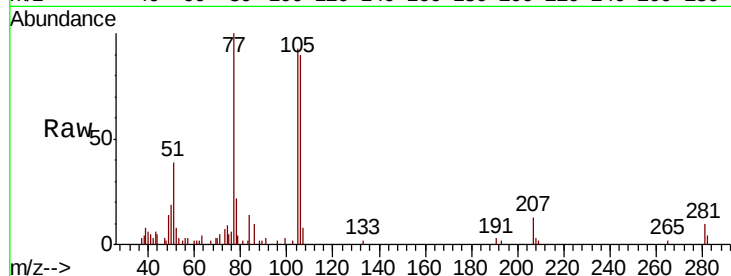

Abundance Ion 77.00 (76.70 to 77.70): BM023705.D (-613) (-)

Ion 105.00 (104.70 to 105.70): BM023705.D (-613) (-)

Ion 106.00 (105.70 to 106.70): BM023705.D (-613) (-)

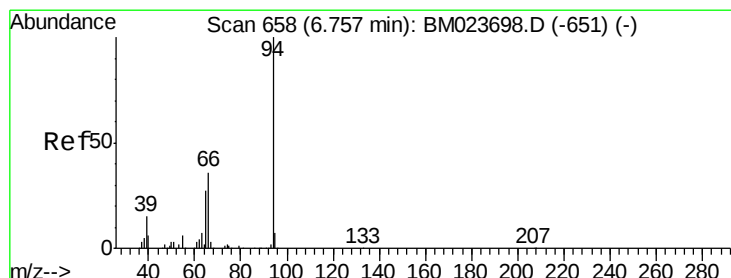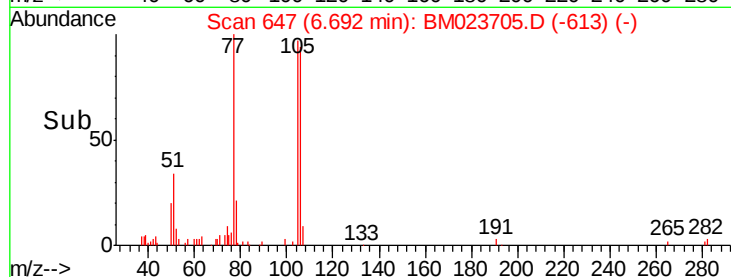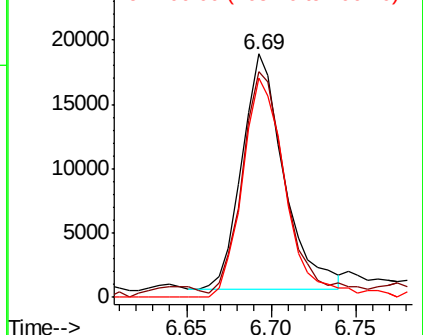

#6

Phenol

Concen: 1.221 ng/ul

RT: 6.76 min Scan# 658

Delta R.T. -0.00 min

Lab File: BM023705.D

Acq: 13 Nov 2019 20:07


Tgt Ion: 94 Resp: 49621

Ion Ratio Lower Upper

94 100

65 27.9 21.4 32.2



66 36.3 30.7 46.1

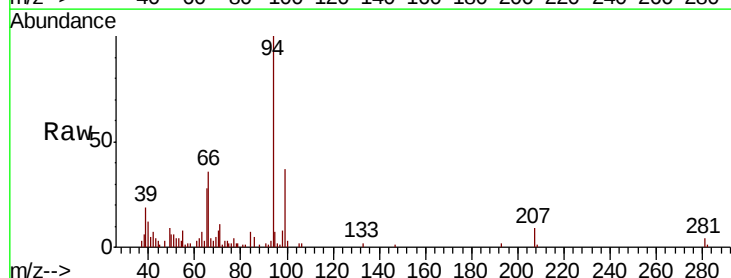


Abundance Ion 94.00 (93.70 to 94.70): BM023705.D (-624) (-)

Ion 65.00 (64.70 to 65.70): BM023705.D (-624) (-)

Ion 66.00 (65.70 to 66.70): BM023705.D (-624) (-)



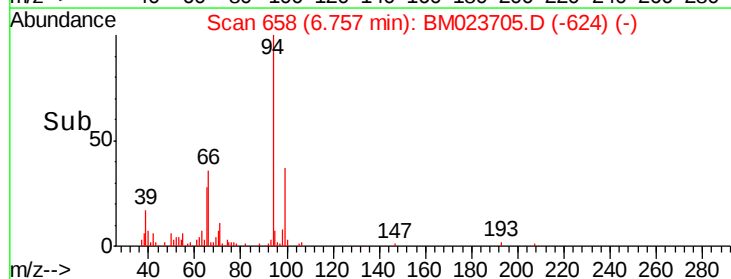
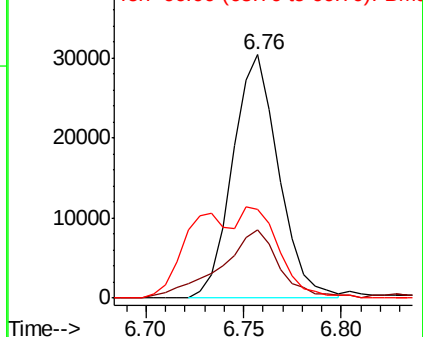


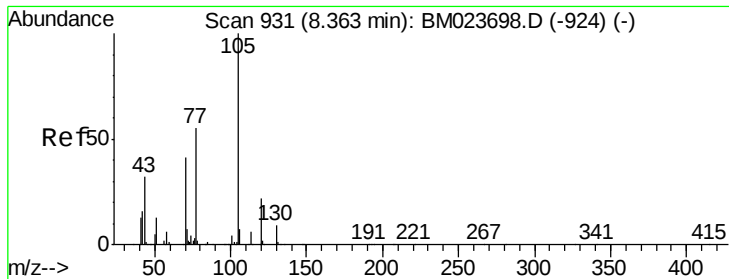

#14
Acetophenone
Concen: 1.130 ng/ul
RT: 8.36 min Scan# 931
Delta R.T. -0.00 min
Lab File: BM023705.D
Acq: 13 Nov 2019 20:07

Instrument :
BNA_M
ClientSampleId :
JLM73

Tot Ion	Ratio	Lower	Upper
105	100		
77	80.5	63.8	95.6
51	20.8	16.3	24.5

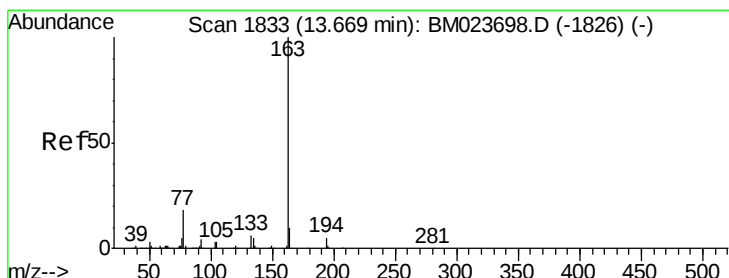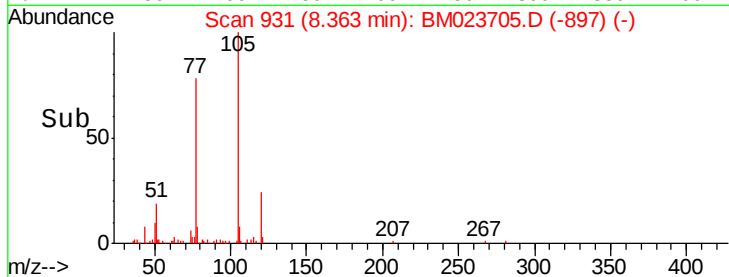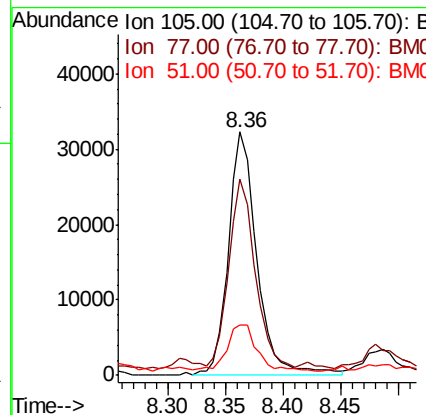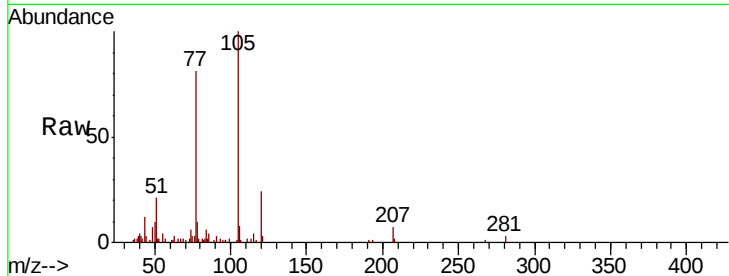

#45
Dimethylphthalate
Concen: 2.086 ng/ul
RT: 13.66 min Scan# 1832
Delta R.T. -0.01 min
Lab File: BM023705.D
Acq: 13 Nov 2019 20:07

Tgt Ion	Ratio	Lower	Upper
163	100		
194	4.6	3.4	5.2
164	10.1	8.0	12.0

