

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM111319\
 Data File : BM023714.D
 Acq On : 14 Nov 2019 01:31
 Operator : JU
 Sample : K5678-21
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JLMM1

Quant Time: Nov 14 03:48:05 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM11119MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Nov 14 03:45:07 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.54	152	402437	20.00	ng/ul	0.00
18) Naphthalene-d8	10.32	136	1939316	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.20	164	1402039	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.94	188	3015234	20.00	ng/ul	0.00
78) Chrysene-d12	21.14	240	2173541	20.00	ng/ul	0.00
86) Perylene-d12	23.31	264	2163315	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.07	96	63290	6.48	ng/uL	0.00
5) Phenol-d5	6.73	99	1650794	45.00	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.89	67	894331	42.43	ng/ul	0.00
9) 2-Chlorophenol-d4	7.08	132	1238990	46.62	ng/ul	0.00
13) 4-Methylphenol-d8	8.26	113	1455312	49.73	ng/ul	0.00
19) Nitrobenzene-d5	8.69	128	697144	50.22	ng/ul	0.00
22) 2-Nitrophenol-d4	9.41	143	841689	57.69	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.95	165	1591674	47.84	ng/ul	0.00
29) 4-Chloroaniline-d4	10.46	131	2080343	56.95	ng/ul	0.00
44) Dimethylphthalate-d6	13.62	166	5097486	46.62	ng/ul	0.00
47) Acenaphthylene-d8	13.89	160	5959609	47.76	ng/ul	0.00
52) 4-Nitrophenol-d4	14.43	143	840781	45.05	ng/ul	0.00
58) Fluorene-d10	15.20	176	4386262	45.43	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.33	200	764247	43.82	ng/ul	0.00
71) Anthracene-d10	17.04	188	6755439	47.23	ng/ul	0.00
79) Pyrene-d10	19.35	212	6596223	58.20	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.17	264	5409865	47.52	ng/ul	0.00


Target Compounds					Ovalue
45) Dimethylphthalate	13.66	163	536920	5.011	ng/ul 100




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM111319\
Data File : BM023714.D
Acq On : 14 Nov 2019 01:31
Operator : JU
Sample : K5678-21
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JLMM1

Quant Time: Nov 14 03:48:05 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM11119MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Nov 14 03:45:07 2019
Response via : Initial Calibration

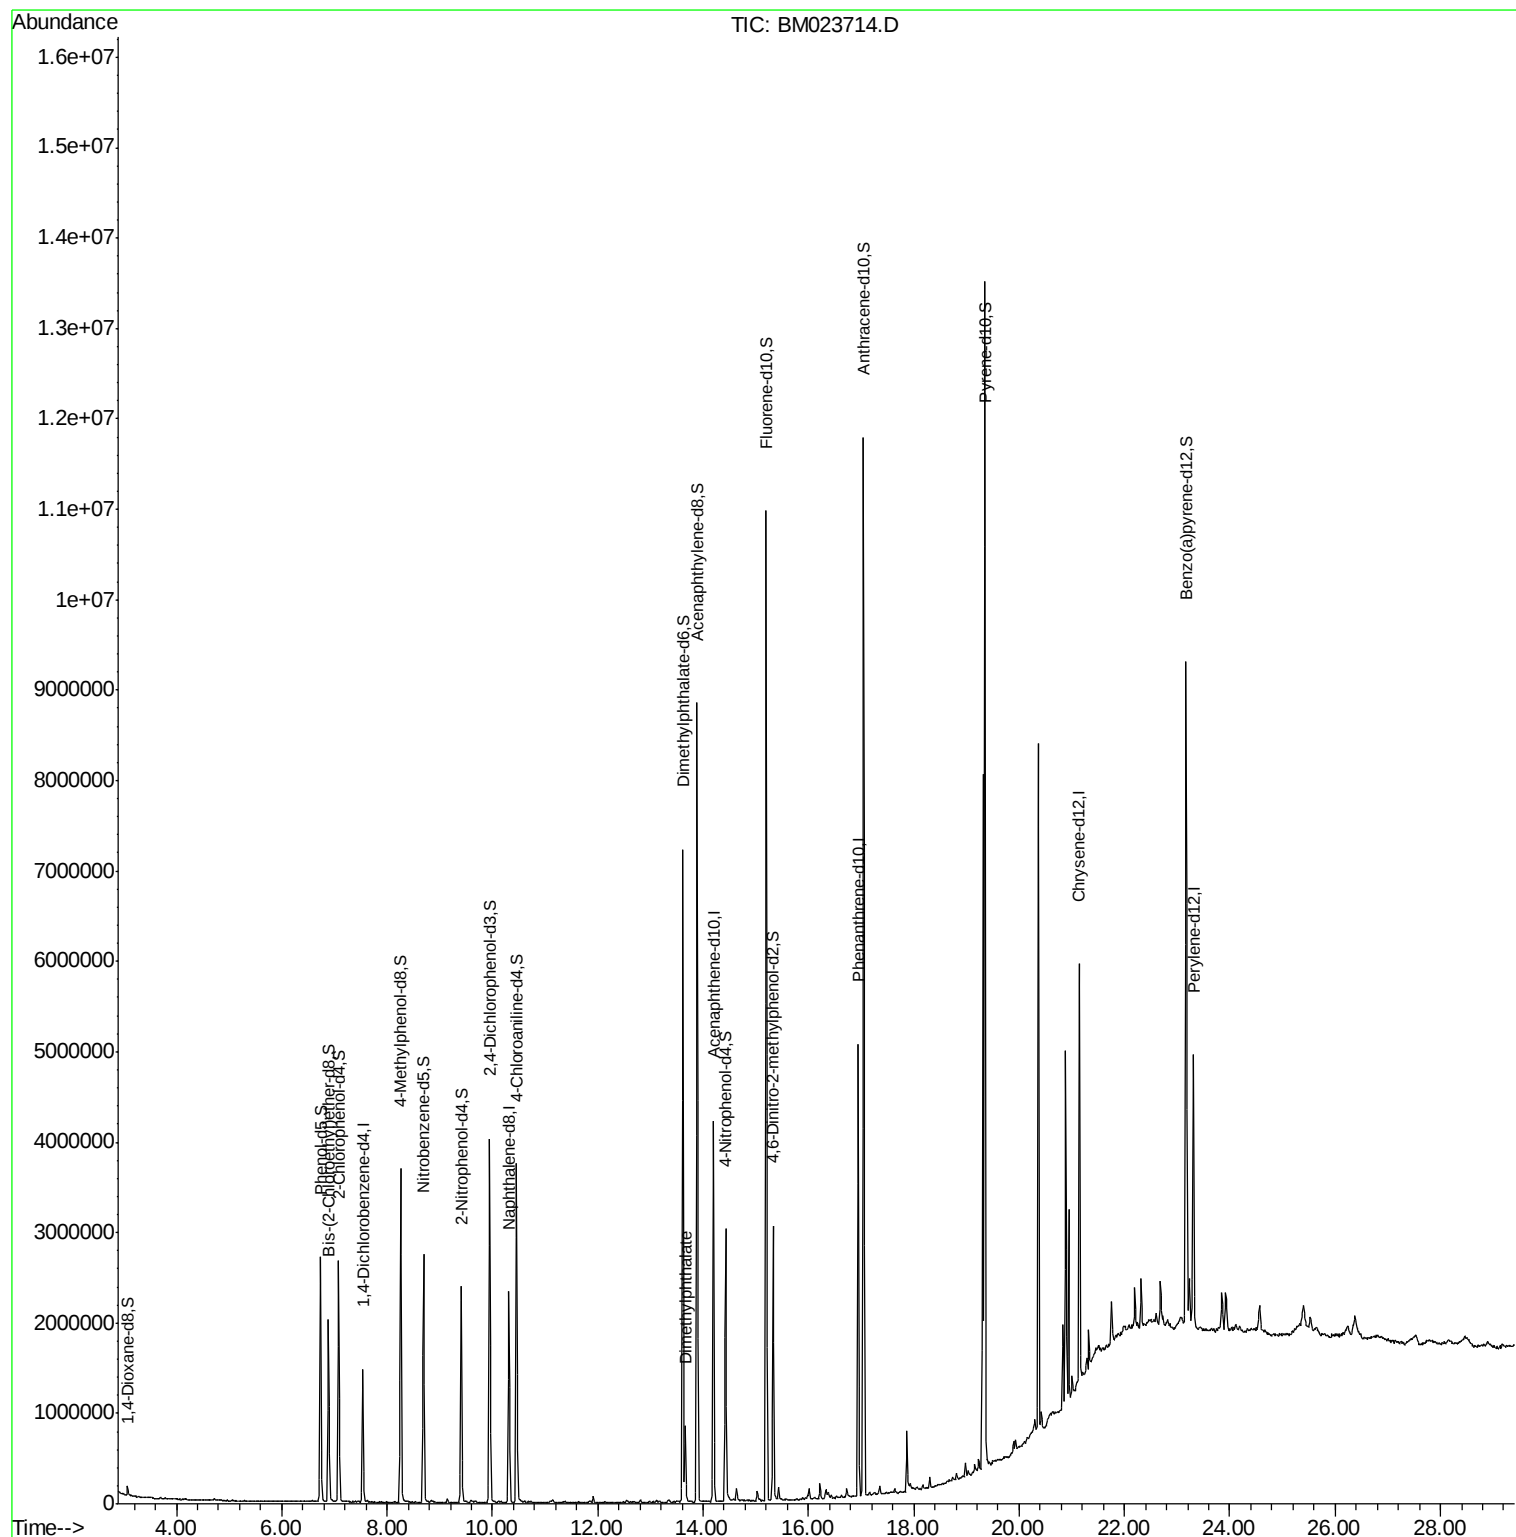

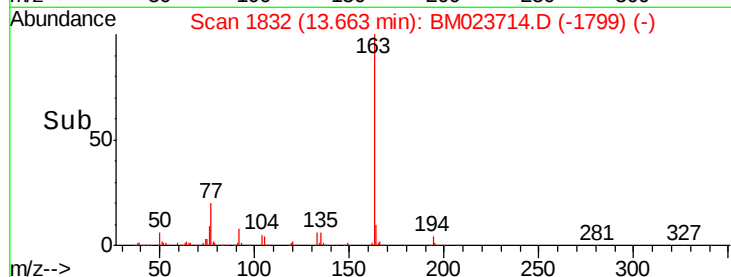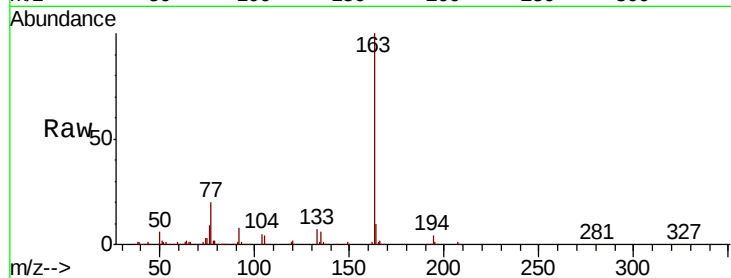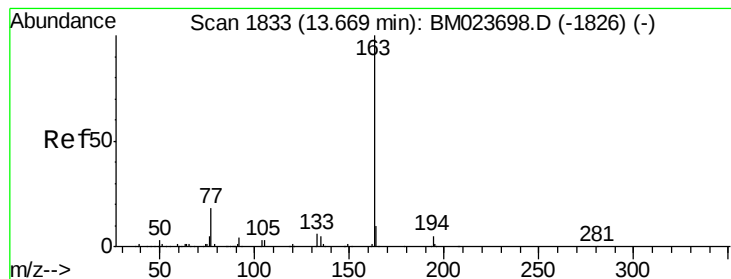

#45

Dimethylphthalate

Concen: 5.011 ng/ul

RT: 13.66 min Scan# 1832

Delta R.T. -0.01 min

Lab File: BM023714.D

Acq: 14 Nov 2019 01:31

Instrument :

BNA_M

ClientSampleId :

JLMM1

Tot Ion:163 Resp: 536920

Ion Ratio Lower Upper

163 100

194 4.4 3.4 5.2

164 10.0 8.0 12.0

