




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
 Data File : BM042718.D
 Acq On : 14 Nov 2023 01:00
 Operator : MA/JU
 Sample : 05016-02MS
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A49A1MS

Manual IntegrationsAPPROVED

Quant Time: Nov 14 15:50:49 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 14 00:02:28 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/15/2023
 Supervised By :mohammad ahmed 11/19/2023

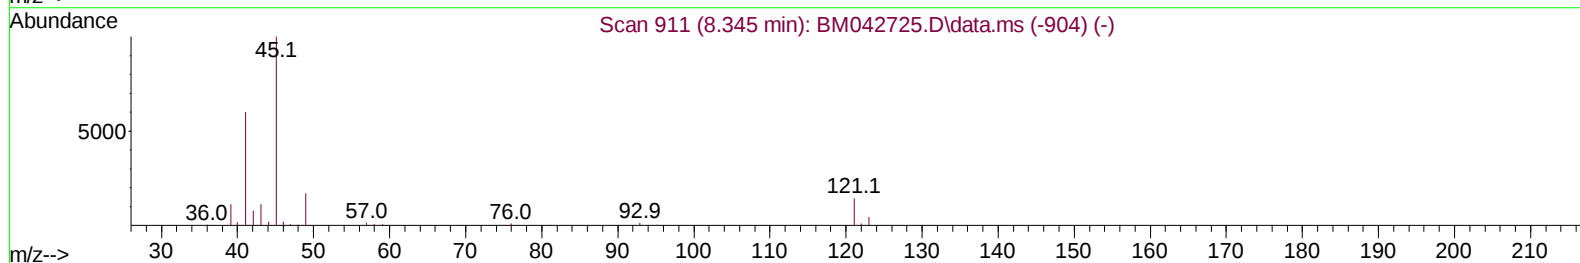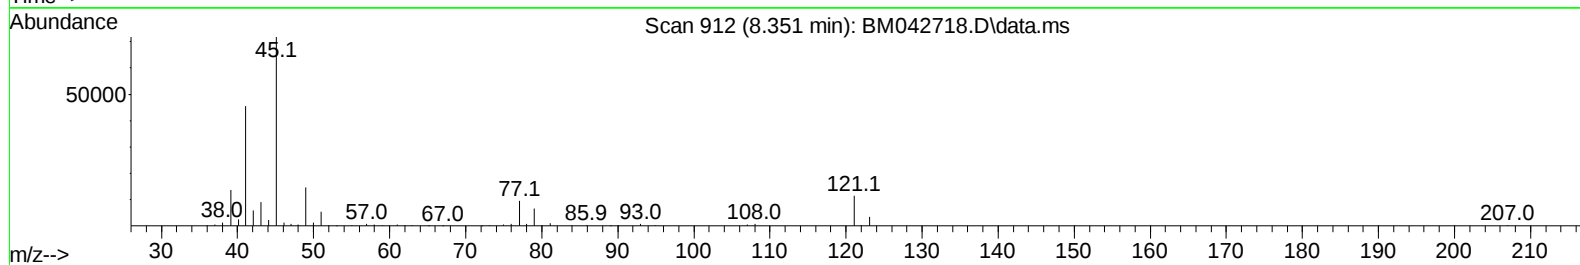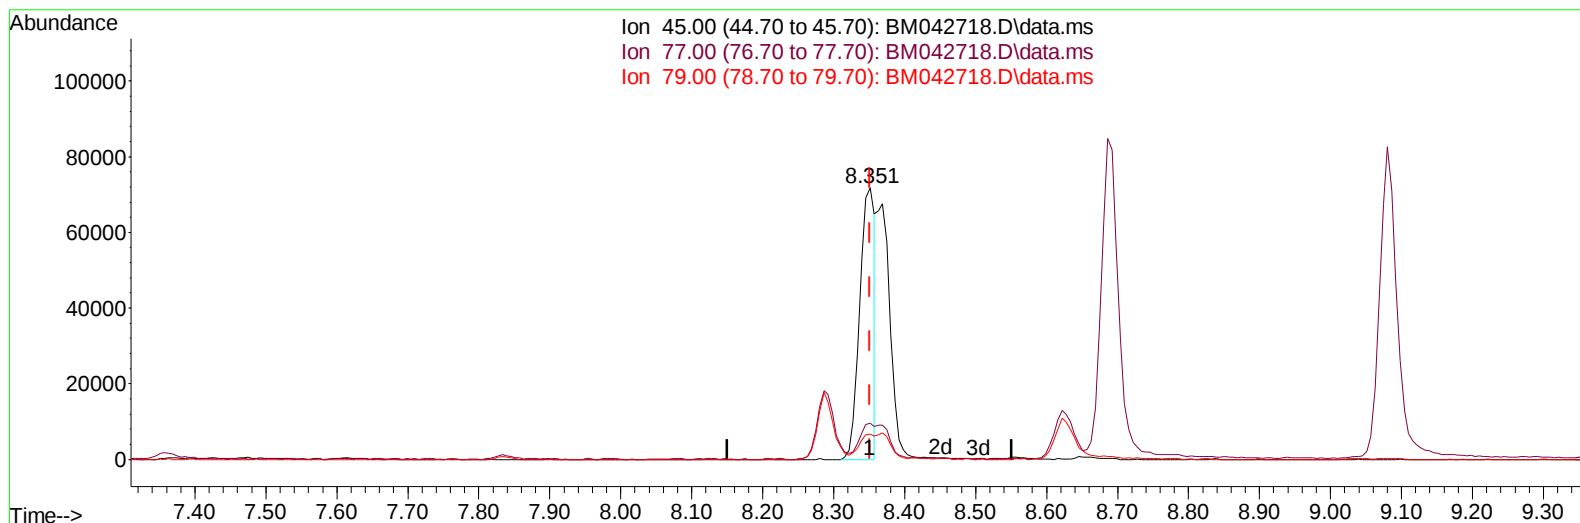

TIC: BM042718.D\data.ms

(14) 2,2'-oxybis(1-Chloropropane)

8.351min (-0.000) 26.31 ng/u1

response 105800

Ion	Exp%	Act%
45.00	100.00	100.00
77.00	15.20	13.38
79.00	10.20	9.34
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
 Data File : BM042718.D
 Acq On : 14 Nov 2023 01:00
 Operator : MA/JU
 Sample : 05016-02MS
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A49A1MS

Manual IntegrationsAPPROVED

Quant Time: Nov 14 15:50:49 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 14 00:02:28 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/15/2023
 Supervised By :mohammad ahmed 11/19/2023

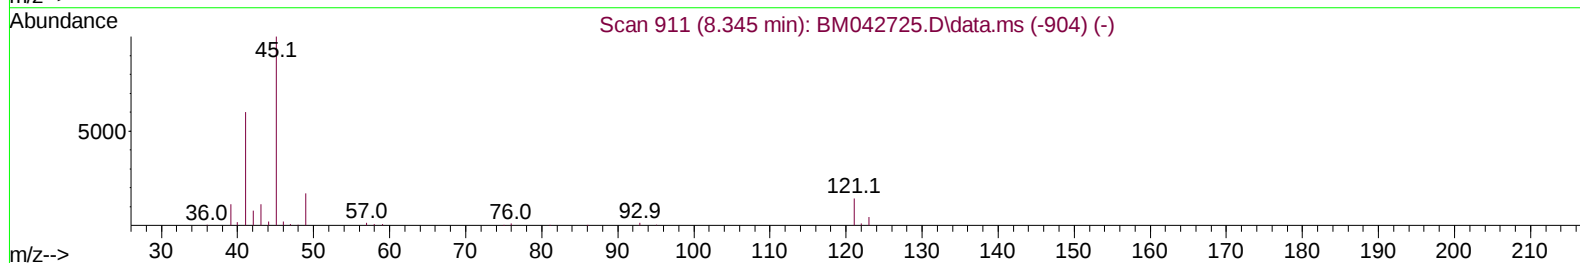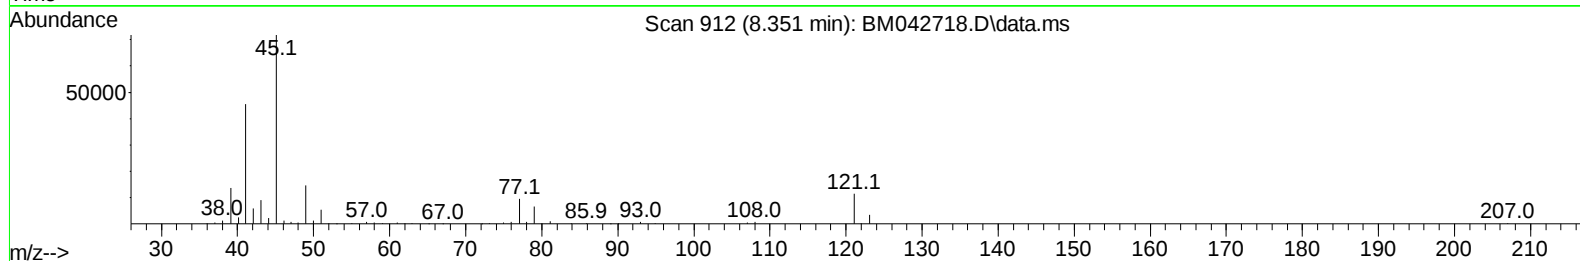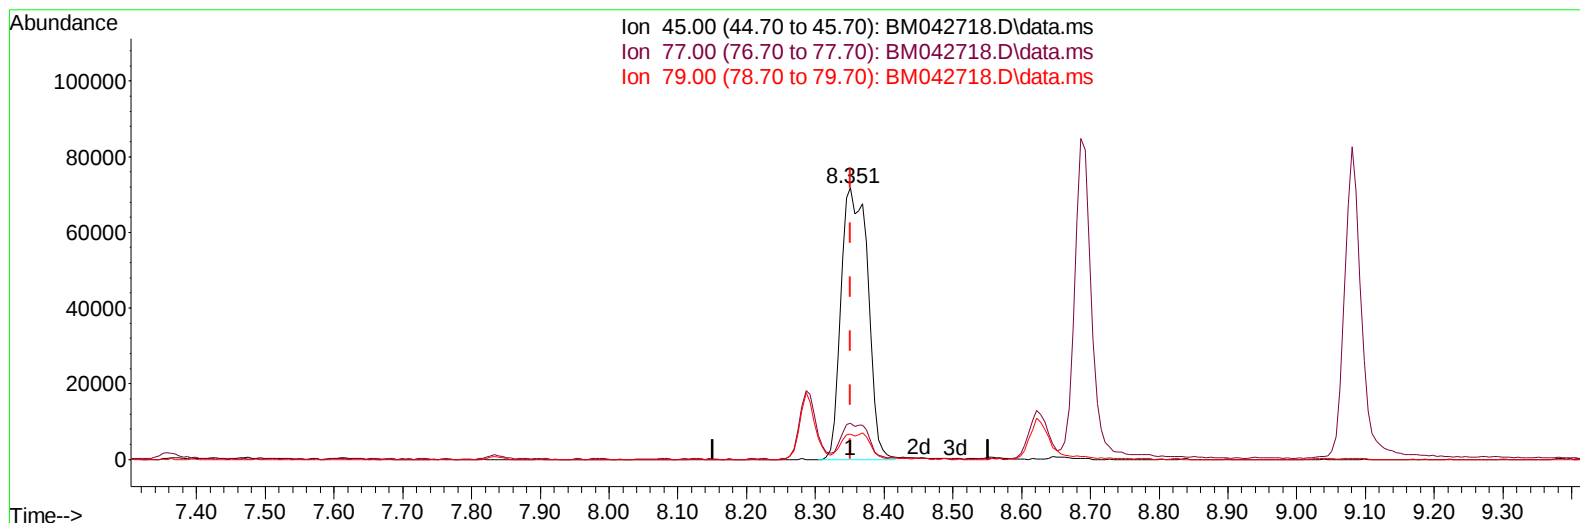

TIC: BM042718.D\data.ms

(14) 2,2'-oxybis(1-Chloropropane)

8.351min (-0.000) 48.19 ng/ul m

response 193789

Ion	Exp%	Act%
45.00	100.00	100.00
77.00	15.20	13.38
79.00	10.20	9.34
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
 Data File : BM042718.D
 Acq On : 14 Nov 2023 01:00
 Operator : MA/JU
 Sample : 05016-02MS
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A49A1MS

Manual IntegrationsAPPROVED

Quant Time: Nov 14 15:50:49 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 14 00:02:28 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/15/2023
 Supervised By :mohammad ahmed 11/19/2023

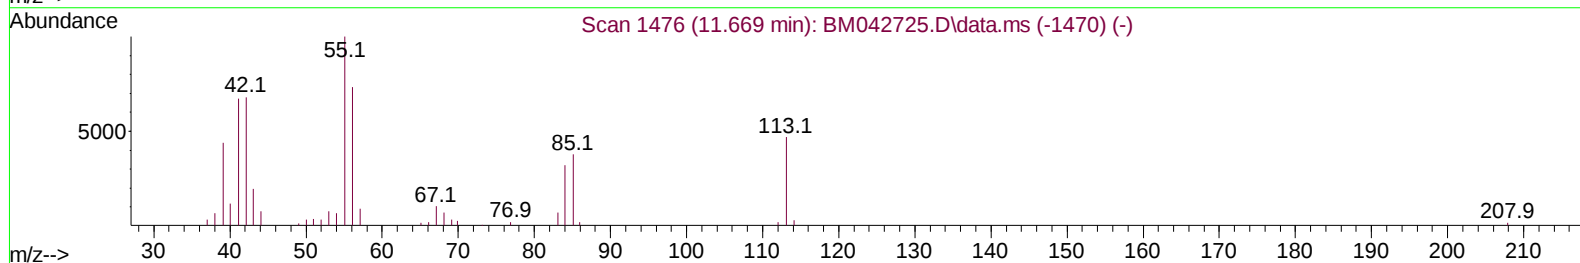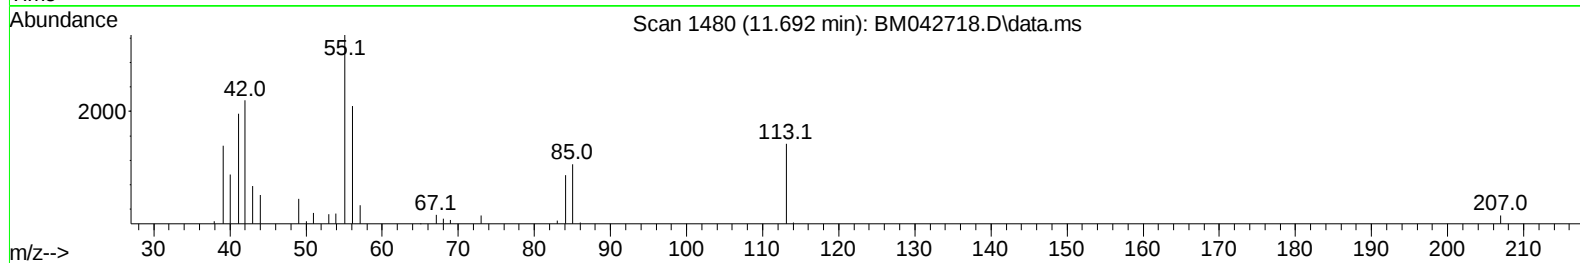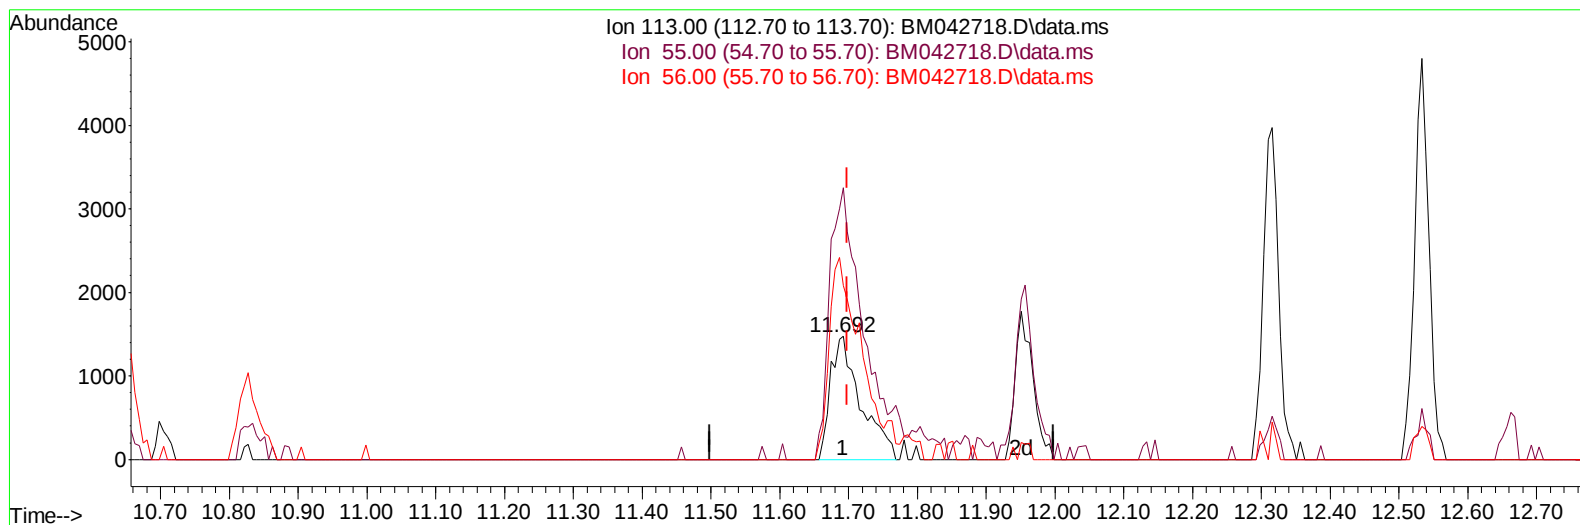

TIC: BM042718.D\data.ms

(34) Caprolactam

11.692min (-0.006) 7.22 ng/u1

response 4524

Ion	Exp%	Act%
113.00	100.00	100.00
55.00	230.20	220.79
56.00	167.90	141.51
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
 Data File : BM042718.D
 Acq On : 14 Nov 2023 01:00
 Operator : MA/JU
 Sample : 05016-02MS
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A49A1MS

Manual IntegrationsAPPROVED

Quant Time: Nov 14 15:50:49 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 14 00:02:28 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/15/2023
 Supervised By :mohammad ahmed 11/19/2023

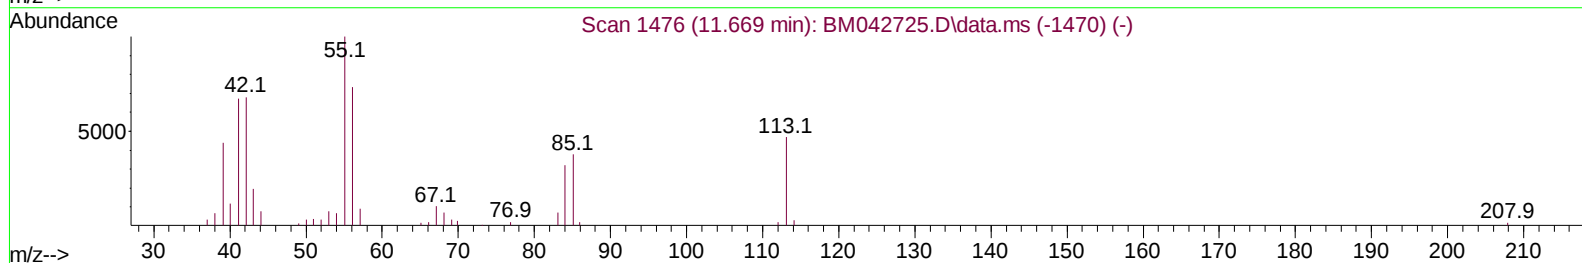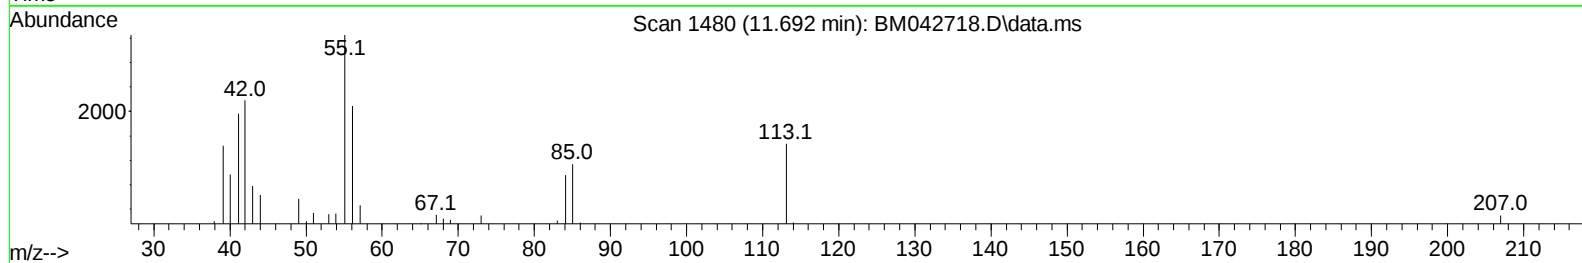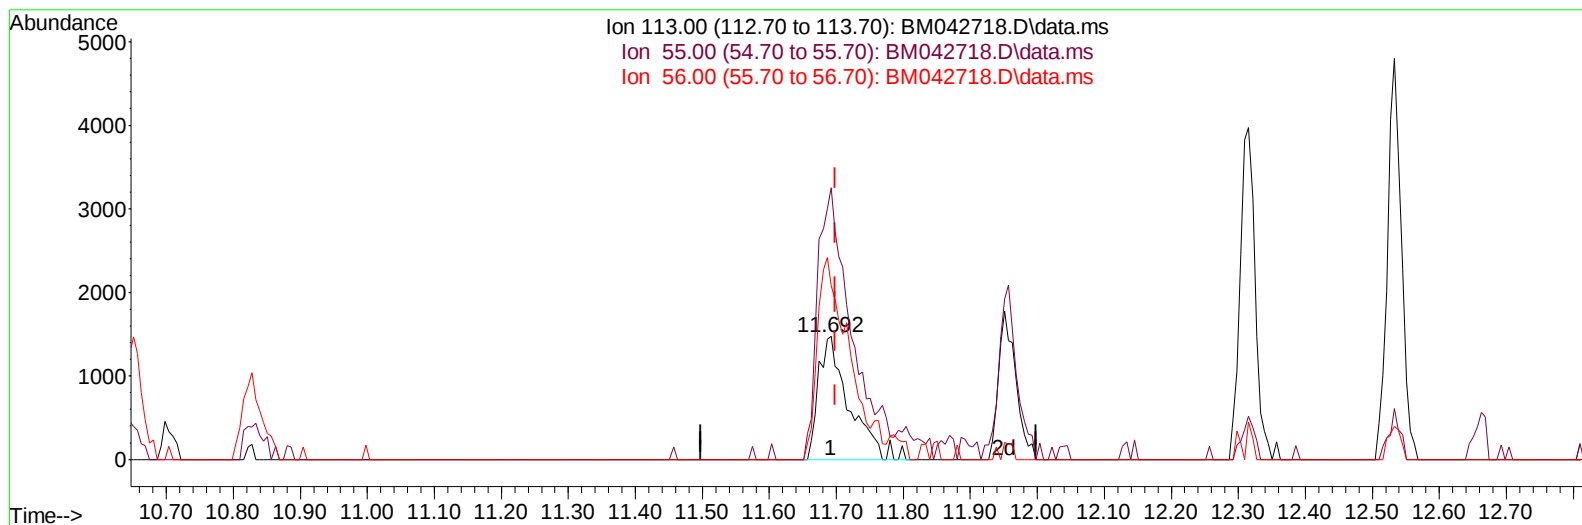

TIC: BM042718.D\data.ms

(34) Caprolactam

11.692min (-0.006) 7.44 ng/ul m

response 4665

Ion	Exp%	Act%
113.00	100.00	100.00
55.00	230.20	220.79
56.00	167.90	141.51
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
 Data File : BM042718.D
 Acq On : 14 Nov 2023 01:00
 Operator : MA/JU
 Sample : 05016-02MS
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A49A1MS

Manual IntegrationsAPPROVED

Quant Time: Nov 14 15:52:57 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 14 00:02:28 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/15/2023
 Supervised By :mohammad ahmed 11/19/2023

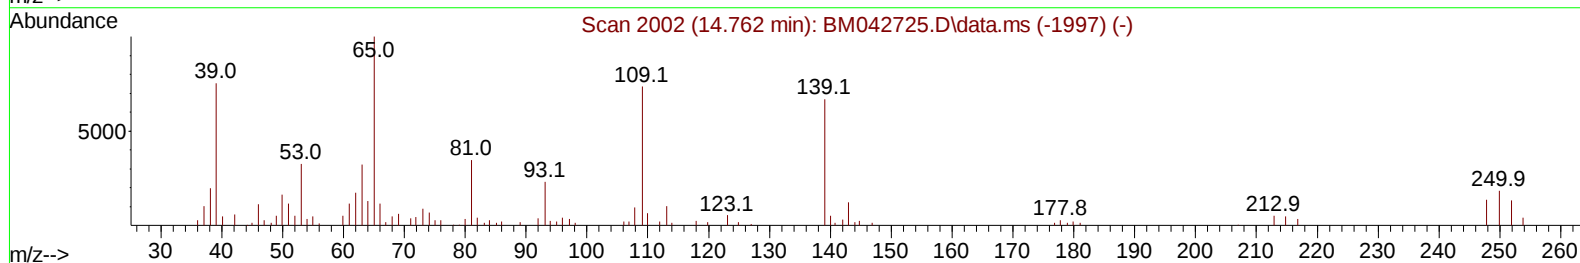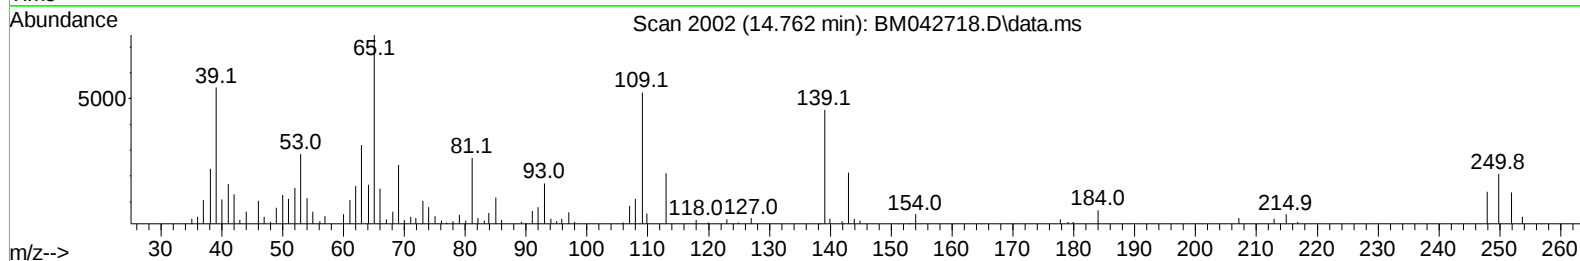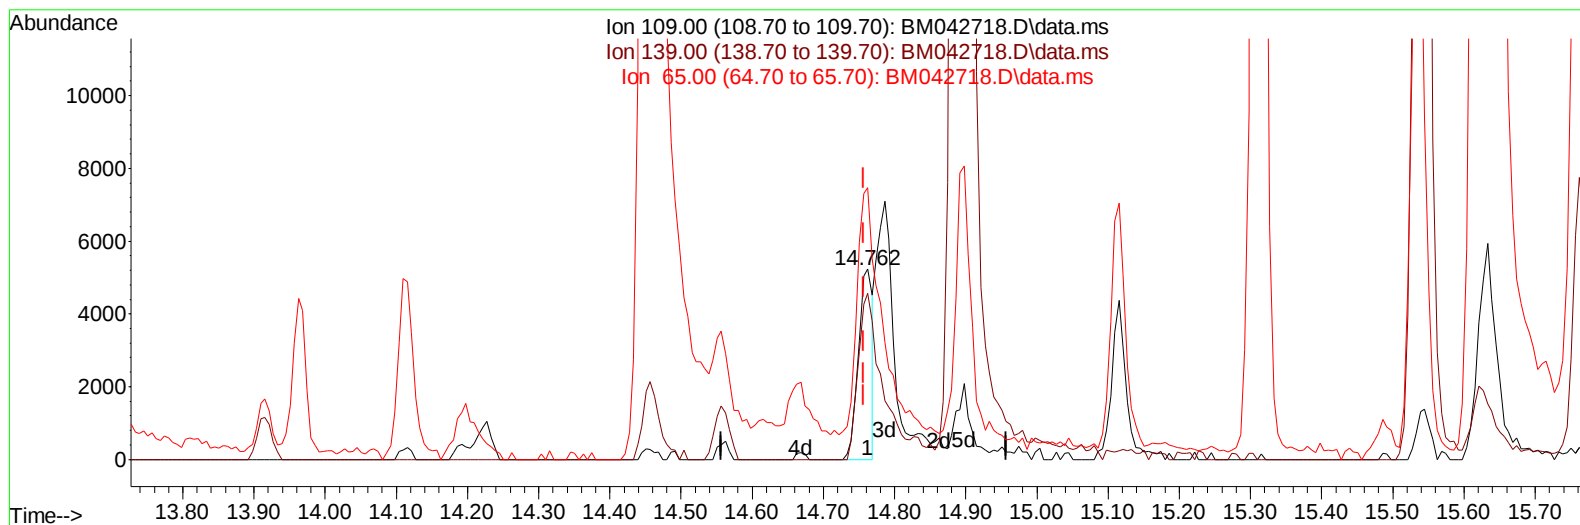

TIC: BM042718.D\data.ms

(55) 4-Nitrophenol

14.762min (+ 0.006) 5.68 ng/u1

response 7251

Ion	Exp%	Act%
109.00	100.00	100.00
139.00	83.90	87.16
65.00	133.90	142.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
 Data File : BM042718.D
 Acq On : 14 Nov 2023 01:00
 Operator : MA/JU
 Sample : 05016-02MS
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A49A1MS

Manual IntegrationsAPPROVED

Quant Time: Nov 15 02:56:21 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 14 00:02:28 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/15/2023
 Supervised By :mohammad ahmed 11/19/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.833	152		27626	20.000	ng/ul	0.00
20) Naphthalene-d8	10.651	136		117107	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.492	164		75860	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.245	188		169252	20.000	ng/ul	0.00
79) Chrysene-d12	21.427	240		186967	20.000	ng/ul	# 0.00
88) Perylene-d12	23.797	264		198107	20.000	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.181	96		4191	4.760	ng/uL	0.00
4) Pyridine-d5	3.628	84		28603	13.061	ng/ul	0.00
7) Phenol-d5	7.004	99		25547	9.502	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.181	67		84683	44.823	ng/ul	0.00
11) 2-Chlorophenol-d4	7.357	132		67619	32.593	ng/ul	0.00
15) 4-Methylphenol-d8	8.563	113		43790	20.685	ng/ul	0.00
21) Nitrobenzene-d5	9.039	128		40837	39.774	ng/ul	0.00
24) 2-Nitrophenol-d4	9.751	143		43260	36.017	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.275	165		81189	36.354	ng/ul	0.00
31) 4-Chloroaniline-d4	10.827	131		81738	28.826	ng/ul	0.00
46) Dimethylphthalate-d6	13.915	166		309705	43.137	ng/ul	0.00
49) Acenaphthylene-d8	14.192	160		310175	40.377	ng/ul	0.00
54) 4-Nitrophenol-d4	14.745	143		6761	8.335	ng/ul	0.00
60) Fluorene-d10	15.486	176		251162	42.245	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.633	200		61107	47.664	ng/ul	0.00
73) Anthracene-d10	17.345	188		425833	44.894	ng/ul	0.00
81) Pyrene-d10	19.644	212		605954	49.493	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.644	264		603245	50.907	ng/ul	0.00
Target Compounds							
						Qvalue	
2) 1,4-Dioxane	3.222	88		6672	7.116	ng/uL	94
5) Pyridine	3.646	79		36715	15.417	ng/ul	99
6) Benzaldehyde	6.998	77		69599	45.117	ng/ul	96
8) Phenol	7.028	94		29883	11.174	ng/ul	100
10) Bis(2-Chloroethyl)ether	7.281	93		100558	45.519	ng/ul	96
12) 2-Chlorophenol	7.392	128		73086	35.398	ng/ul	89
13) 2-Methylphenol	8.286	108		53143	26.647	ng/ul	95
14) 2,2'-oxybis(1-Chloropr...	8.351	45		193789m	48.187	ng/ul	
16) Acetophenone	8.686	105		153159	43.025	ng/ul	95
17) N-Nitroso-di-n-propyla...	8.657	70		99647	45.984	ng/ul	95
18) 4-Methylphenol	8.622	108		52298	24.120	ng/ul	98
19) Hexachloroethane	8.892	117		42170	36.645	ng/ul	86
22) Nitrobenzene	9.080	77		141779	45.688	ng/ul	98
23) Isophorone	9.586	82		276763	44.780	ng/ul	97
25) 2-Nitrophenol	9.780	139		49275	40.379	ng/ul	94
26) 2,4-Dimethylphenol	9.822	107		63058	24.151	ng/ul	97
27) Bis(2-Chloroethoxy)met...	10.075	93		140671	45.041	ng/ul	98
29) 2,4-Dichlorophenol	10.304	162		82305	38.925	ng/ul	97
30) Naphthalene	10.704	128		290659	39.618	ng/ul	98
32) 4-Chloroaniline	10.851	127		82340	30.268	ng/ul	95
33) Hexachlorobutadiene	10.922	225		64868	34.730	ng/ul	96
34) Caprolactam	11.692	113		4665m	7.441	ng/ul	
35) 4-Chloro-3-methylphenol	11.957	107		85518	37.744	ng/ul	98

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
 Data File : BM042718.D
 Acq On : 14 Nov 2023 01:00
 Operator : MA/JU
 Sample : 05016-02MS
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A49A1MS

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/15/2023
 Supervised By :mohammad ahmed 11/19/2023

Quant Time: Nov 15 02:56:21 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 14 00:02:28 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
36) 2-Methylnaphthalene	12.316	142	204081	41.504	ng/ul	97
37) 1-Methylnaphthalene	12.533	142	208401	40.311	ng/ul	95
39) 1,2,4,5-Tetrachloroben...	12.668	216	129186	43.422	ng/ul	99
40) Hexachlorocyclopentadiene	12.604	237	39376	27.956	ng/ul	98
41) 2,4,6-Trichlorophenol	12.927	196	79160	43.560	ng/ul	93
42) 2,4,5-Trichlorophenol	12.998	196	79758	45.452	ng/ul	98
43) 1,1'-Biphenyl	13.327	154	284244	44.929	ng/ul	98
44) 2-Chloronaphthalene	13.374	162	224337	44.079	ng/ul	97
45) 2-Nitroaniline	13.621	65	90450	54.494	ng/ul	93
47) Dimethylphthalate	13.963	163	336449	48.113	ng/ul	100
48) 2,6-Dinitrotoluene	14.115	165	65161	49.599	ng/ul	95
50) Acenaphthylene	14.221	152	388166	45.096	ng/ul	99
51) 3-Nitroaniline	14.457	138	50848	47.332	ng/ul	99
52) Acenaphthene	14.557	153	263945	45.340	ng/ul	97
53) 2,4-Dinitrophenol	14.662	184	32091	49.126	ng/ul	87
55) 4-Nitrophenol	14.786	109	18644m	14.606	ng/ul	
56) Dibenzofuran	14.898	168	375434	46.465	ng/ul	98
57) 2,4-Dinitrotoluene	14.898	165	106766	55.355	ng/ul	99
58) 2,3,4,6-Tetrachlorophenol	15.115	232	86449	47.460	ng/ul#	98
59) Diethylphthalate	15.315	149	374989	51.138	ng/ul	98
61) Fluorene	15.545	166	338038	49.277	ng/ul	100
62) 4-Chlorophenyl-phenyle...	15.539	204	178624	48.316	ng/ul	98
63) 4-Nitroaniline	15.627	138	52538	53.643	ng/ul	94
66) 4,6-Dinitro-2-methylph...	15.651	198	68360	52.375	ng/ul	97
67) N-Nitrosodiphenylamine	15.762	169	268970	50.669	ng/ul	99
68) 4-Bromophenyl-phenylether	16.433	248	109922	48.792	ng/ul	91
69) Hexachlorobenzene	16.515	284	140355	50.962	ng/ul	96
70) Atrazine	16.715	200	99342	48.584	ng/ul	99
71) Pentachlorophenol	16.880	266	80725	50.901	ng/ul	98
72) Phenanthrene	17.292	178	561849	53.137	ng/ul	99
74) Anthracene	17.380	178	547216	51.452	ng/ul	100
75) 1,2,3,4-Tetrachloroben...	13.280	216	131588	43.968	ng/uL	98
76) Pentachlorobenzene	14.786	250	133753	42.594	ng/uL	99
77) Carbazole	17.674	167	491664	55.986	ng/ul	99
78) Di-n-butylphthalate	18.192	149	730535	56.887	ng/ul	99
80) Fluoranthene	19.303	202	758263	54.317	ng/ul#	97
82) Pyrene	19.674	202	808786	54.641	ng/ul	99
83) Butylbenzylphthalate	20.550	149	342347	54.150	ng/ul	92
84) 3,3'-Dichlorobenzidine	21.356	252	169946	35.515	ng/ul	98
85) Benzo(a)anthracene	21.415	228	805463	54.880	ng/ul	100
86) Bis(2-ethylhexyl)phtha...	21.297	149	523885	54.616	ng/ul	99
87) Chrysene	21.468	228	783696	55.058	ng/ul	99
89) Di-n-octyl phthalate	22.209	149	909093	56.809	ng/ul	100
90) Benzo(b)fluoranthene	23.068	252	782794	57.900	ng/ul#	98
91) Benzo(k)fluoranthene	23.115	252	823646	57.230	ng/ul	99
93) Benzo(a)pyrene	23.697	252	754570	57.277	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	26.273	276	952254	58.161	ng/ul	98
95) Dibenzo(a,h)anthracene	26.291	278	800617	58.982	ng/ul	98
96) Benzo(g,h,i)perylene	27.044	276	734951	56.529	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Instrument :

BNA_M

ClientSampleId :

A49A1MS

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/15/2023

Supervised By :mohammad ahmed 11/19/2023

