




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042820.D
Acq On : 16 Nov 2023 23:57
Operator : MA/JU
Sample : 05268-11
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCKD3

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/17/2023
Supervised By :mohammad ahmed 11/19/2023

Quant Time: Nov 17 00:47:31 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 15 22:28:07 2023
Response via : Initial Calibration

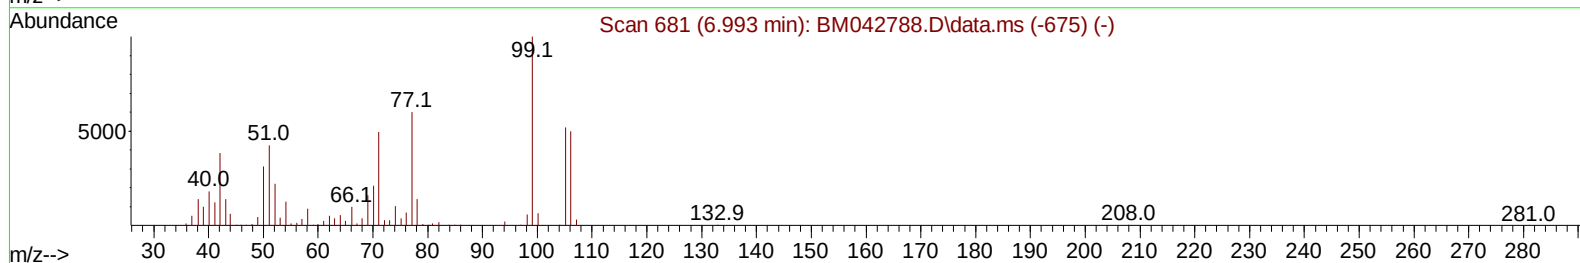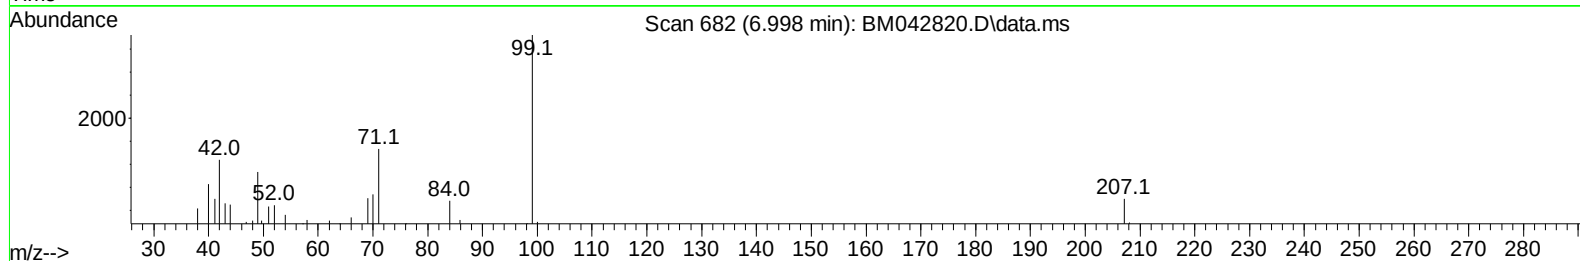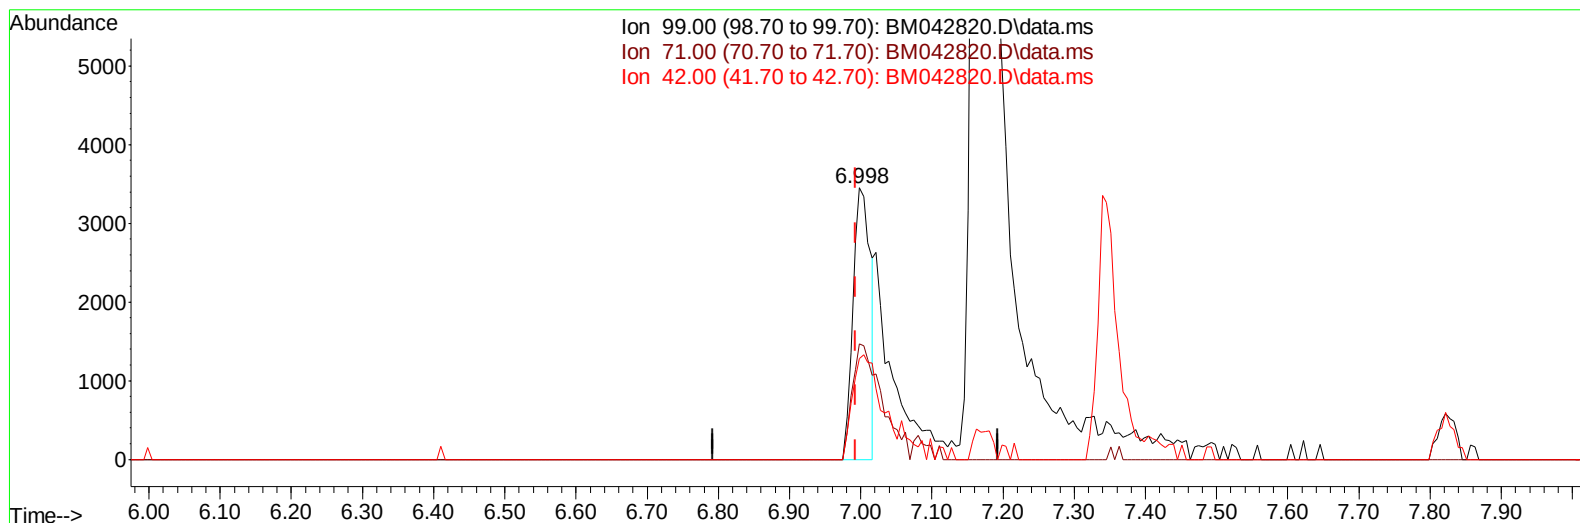

TIC: BM042820.D\data.ms

(7) Phenol-d5 (S)

6.998min (+ 0.006) 2.81 ng/uL

response 5917

Ion	Exp%	Act%
99.00	100.00	100.00
71.00	43.50	42.64
42.00	32.20	37.07
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042820.D
Acq On : 16 Nov 2023 23:57
Operator : MA/JU
Sample : 05268-11
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCKD3

Manual IntegrationsAPPROVED

Quant Time: Nov 17 00:47:31 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 15 22:28:07 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/17/2023
Supervised By :mohammad ahmed 11/19/2023

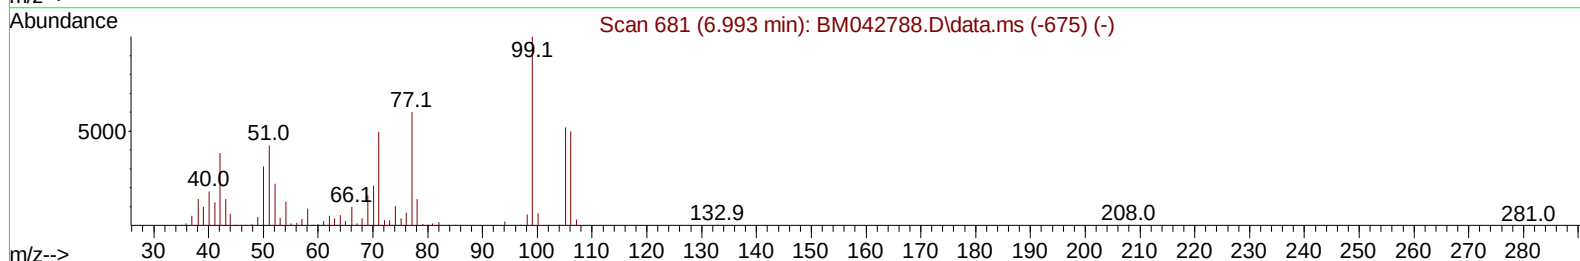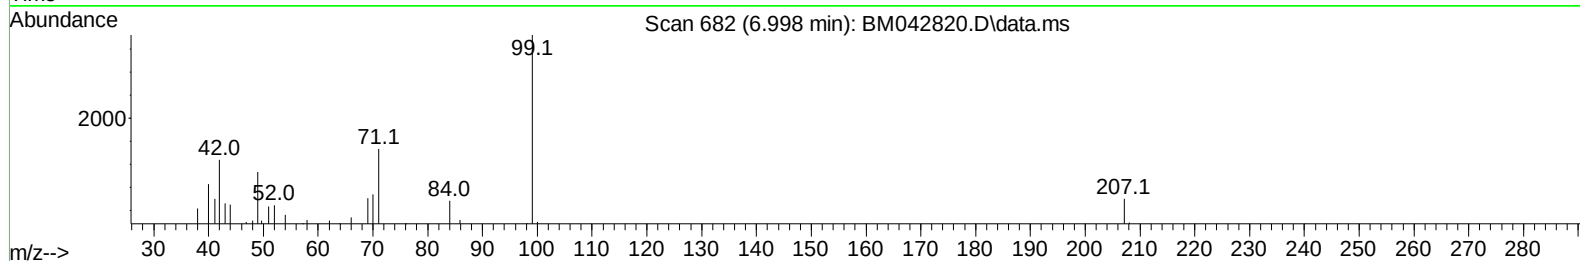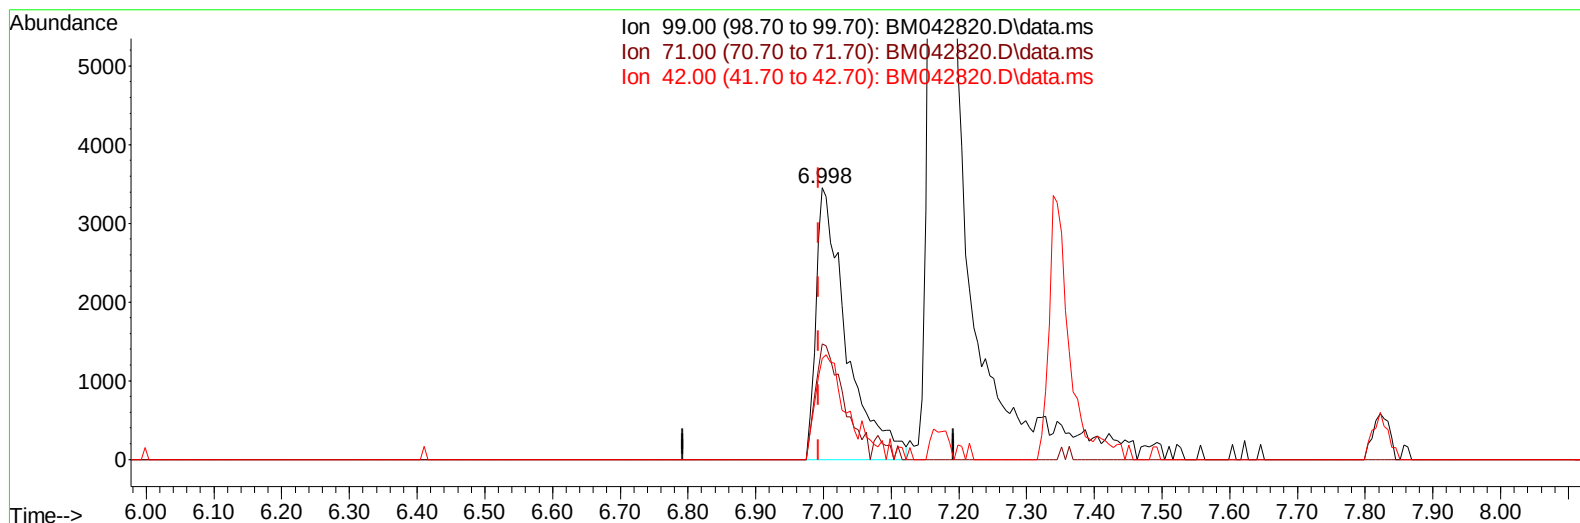

TIC: BM042820.D\data.ms

(7) Phenol-d5 (S)

6.998min (+ 0.006) 5.10 ng/ul m

response 10737

Ion	Exp%	Act%
99.00	100.00	100.00
71.00	43.50	42.64
42.00	32.20	37.07
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
 Data File : BM042820.D
 Acq On : 16 Nov 2023 23:57
 Operator : MA/JU
 Sample : 05268-11
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCKD3

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/17/2023
 Supervised By :mohammad ahmed 11/19/2023

Quant Time: Nov 17 00:48:05 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 15 22:28:07 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.822	152	21615	20.000	ng/ul	0.00
20) Naphthalene-d8	10.633	136	86444	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.480	164	54892	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.233	188	120255	20.000	ng/ul	0.00
79) Chrysene-d12	21.415	240	119400	20.000	ng/ul	0.00
88) Perylene-d12	23.774	264	155982	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.175	96	2564	3.722	ng/uL	0.00
4) Pyridine-d5	3.622	84	13892	8.107	ng/ul	0.00
7) Phenol-d5	6.998	99	10737m	5.104	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.169	67	51726	34.992	ng/ul	0.00
11) 2-Chlorophenol-d4	7.345	132	35711	22.000	ng/ul	0.00
15) 4-Methylphenol-d8	8.551	113	19067	11.511	ng/ul	0.00
21) Nitrobenzene-d5	9.028	128	21707	28.641	ng/ul	0.00
24) 2-Nitrophenol-d4	9.733	143	23384	26.375	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.263	165	38550	23.384	ng/ul	0.00
31) 4-Chloroaniline-d4	10.816	131	43803	20.927	ng/ul	0.00
46) Dimethylphthalate-d6	13.904	166	182639	35.156	ng/ul	0.00
49) Acenaphthylene-d8	14.180	160	186654	33.579	ng/ul	0.00
54) 4-Nitrophenol-d4	14.798	143	120	0.204	ng/ul	0.06
60) Fluorene-d10	15.474	176	156582	36.397	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.627	200	20406	22.402	ng/ul	0.00
73) Anthracene-d10	17.333	188	270263	40.102	ng/ul	0.00
81) Pyrene-d10	19.627	212	356939	45.652	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.621	264	377051	40.412	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042820.D
Acq On : 16 Nov 2023 23:57
Operator : MA/JU
Sample : 05268-11
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCKD3

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/17/2023
Supervised By :mohammad ahmed 11/19/2023

Quant Time: Nov 17 00:48:05 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 15 22:28:07 2023
Response via : Initial Calibration

