

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
 Data File : BM042758.D
 Acq On : 15 Nov 2023 06:24
 Operator : MA/JU
 Sample : 05057-24
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A49Y7

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/15/2023
 Supervised By :mohammad ahmed 11/19/2023

Quant Time: Nov 15 09:25:44 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 14 00:02:28 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.834	152	24941	20.000	ng/u1	0.00
20) Naphthalene-d8	10.645	136	101055	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.486	164	66367	20.000	ng/u1	-0.01
64) Phenanthrene-d10	17.239	188	151791	20.000	ng/u1	#-0.01
79) Chrysene-d12	21.421	240	155701	20.000	ng/u1	-0.01
88) Perylene-d12	23.786	264	187737	20.000	ng/u1	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.181	96	3137	3.947	ng/uL	0.00
4) Pyridine-d5	3.640	84	8229	4.162	ng/u1	0.01
7) Phenol-d5	7.004	99	16108	6.636	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.181	67	50750	29.754	ng/u1	0.00
11) 2-Chlorophenol-d4	7.357	132	41411	22.109	ng/u1	0.00
15) 4-Methylphenol-d8	8.557	113	27941	14.619	ng/u1	0.00
21) Nitrobenzene-d5	9.034	128	23187	26.171	ng/u1	0.00
24) 2-Nitrophenol-d4	9.745	143	25298	24.408	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.275	165	46431	24.093	ng/u1	0.00
31) 4-Chloroaniline-d4	10.845	131	4292m	1.754	ng/u1	0.02
46) Dimethylphthalate-d6	13.910	166	202835	32.293	ng/u1	0.00
49) Acenaphthylene-d8	14.186	160	201092	29.922	ng/u1	-0.01
54) 4-Nitrophenol-d4	14.792	143	1815m	2.558	ng/u1	0.05
60) Fluorene-d10	15.480	176	165587	31.835	ng/u1	-0.01
65) 4,6-Dinitro-2-methylph...	15.627	200	26671	23.197	ng/u1	-0.01
73) Anthracene-d10	17.339	188	283073	33.276	ng/u1	-0.01
81) Pyrene-d10	19.633	212	422359	41.424	ng/u1	-0.01
92) Benzo(a)pyrene-d12	23.633	264	430676	38.352	ng/u1	-0.02
Target Compounds						
					Qvalue	
8) Phenol	7.034	94	2824	1.170	ng/u1#	89

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042758.D
Acq On : 15 Nov 2023 06:24
Operator : MA/JU
Sample : 05057-24
Misc :
ALS Vial : 61 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
A49Y7

Quant Time: Nov 15 09:25:44 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 14 00:02:28 2023
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 11/15/2023
Supervised By :mohammad ahmed 11/19/2023

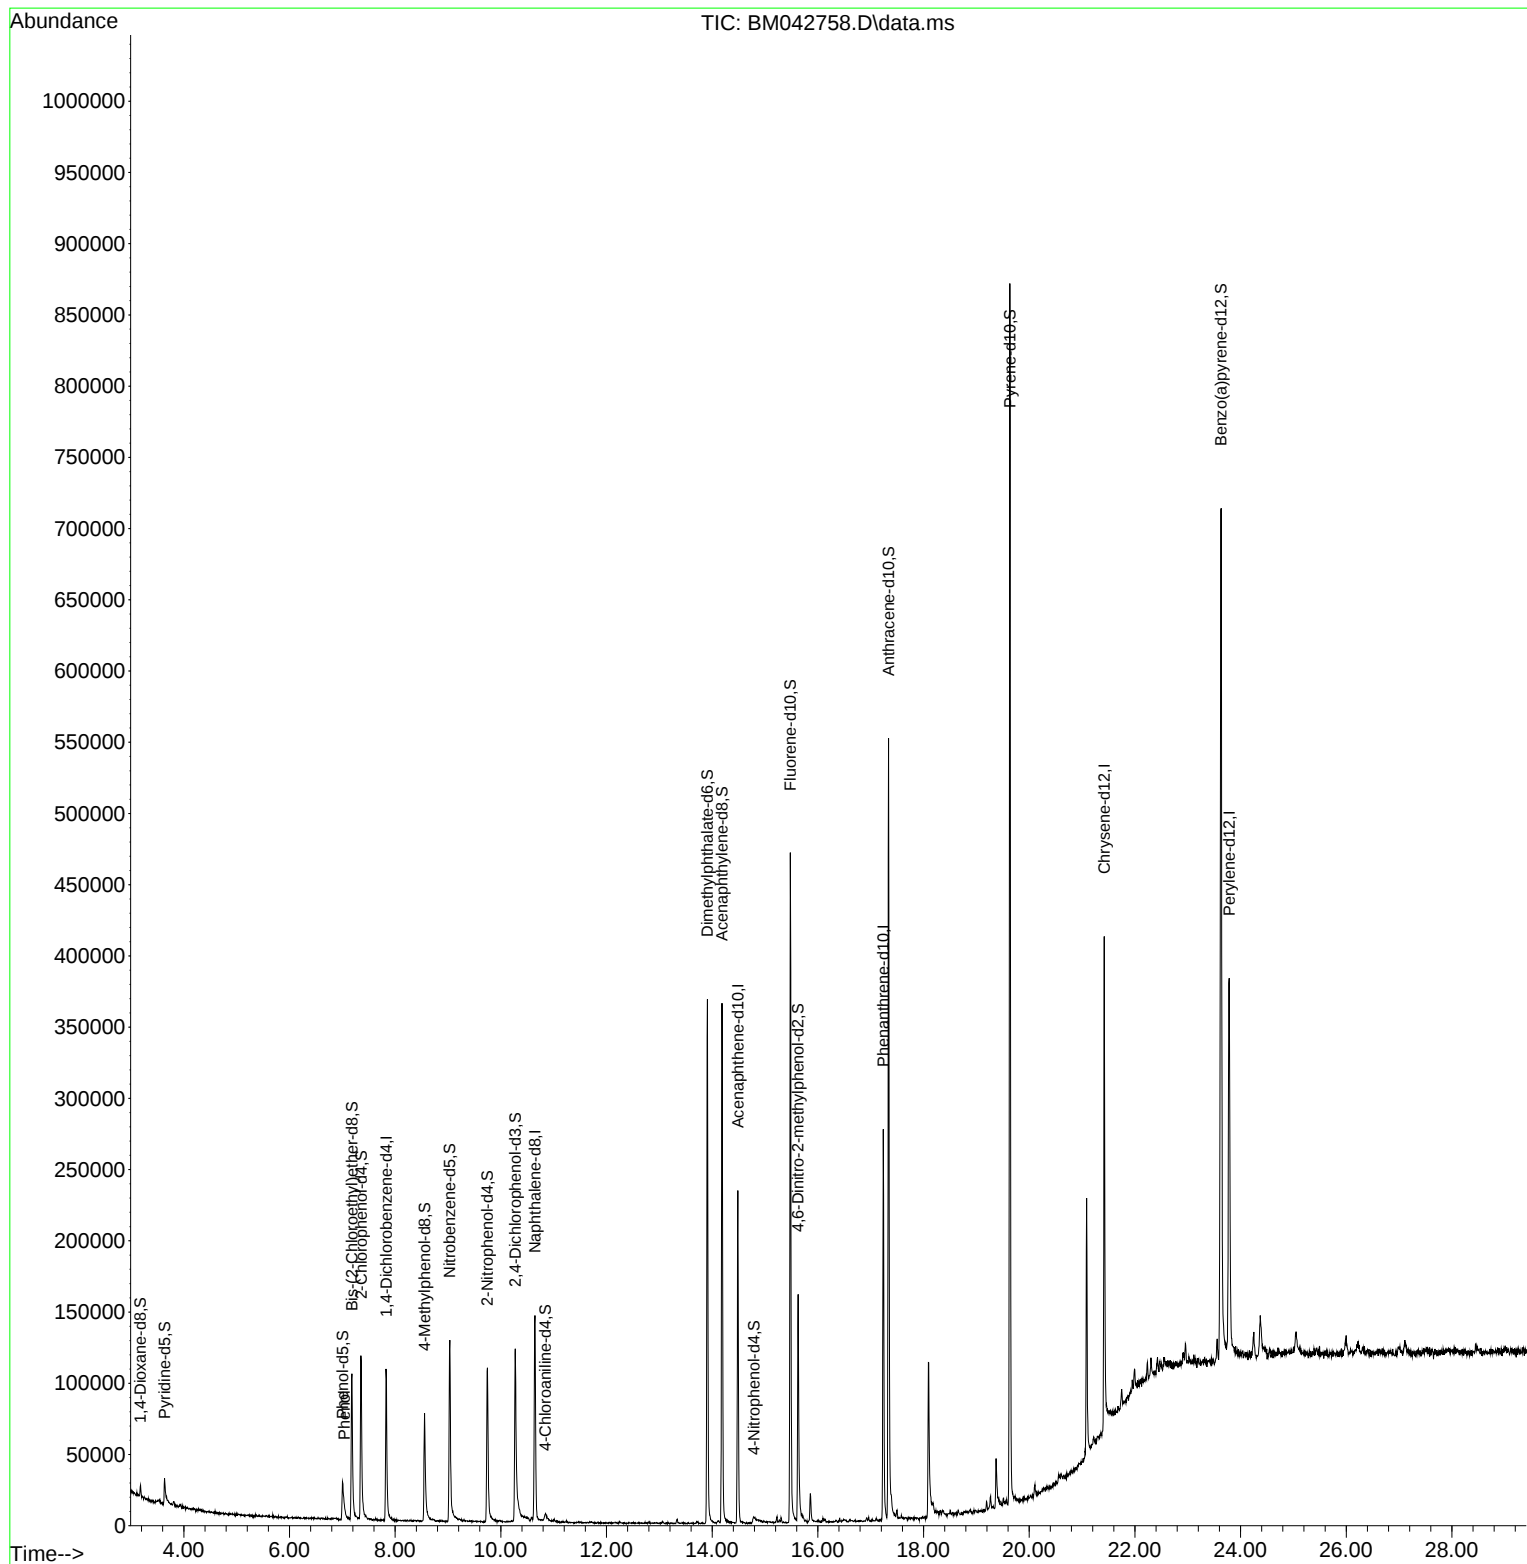

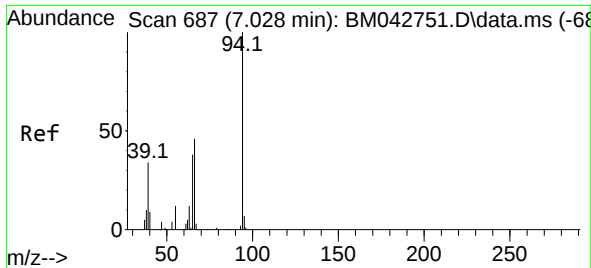

#8
Phenol
Concen: 1.170 ng/ul
RT: 7.034 min Scan# 687
Delta R.T. -0.000 min
Lab File: BM042758.D
Acq: 15 Nov 2023 06:24

Instrument :
BNA_M
ClientSampleId :
A49Y7

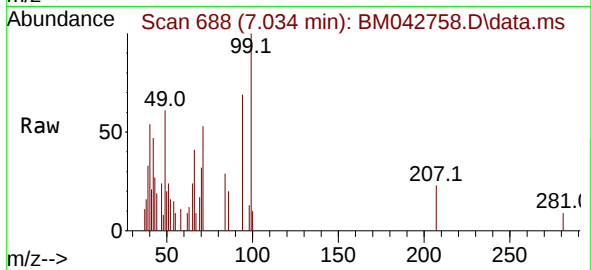

Tgt Ion: 94 Resp: 2824
Ion Ratio Lower Upper
94 100
65 35.1 30.3 45.5
66 60.3 39.9 59.9

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/15/2023
Supervised By :mohammad ahmed 11/19/2023

