

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
 Data File : BM042711.D
 Acq On : 13 Nov 2023 17:12
 Operator : MA/JU
 Sample : PB156652BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK652

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM042711.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	29	33	37	rVB	12690	15287	1.55%	0.161%
2	3.616	104	107	119	rBV	128922	210354	21.39%	2.211%
3	3.799	136	138	139	rVB	2210	993	0.10%	0.010%
4	3.922	156	159	170	rVB8	3257	7251	0.74%	0.076%
5	4.304	222	224	226	rBV3	1269	1190	0.12%	0.013%
6	4.804	308	309	311	rBV2	1475	1281	0.13%	0.013%
7	4.987	337	340	342	rBV3	1254	1633	0.17%	0.017%
8	5.169	369	371	372	rVB2	1737	1220	0.12%	0.013%
9	5.551	434	436	438	rBV	1105	1158	0.12%	0.012%
10	5.722	463	465	468	rBV2	1099	1130	0.11%	0.012%
11	5.887	489	493	496	rBV6	1145	1845	0.19%	0.019%
12	6.551	603	606	610	rBV3	784	1214	0.12%	0.013%
13	6.998	676	682	700	rBV	139860	278250	28.30%	2.924%
14	7.181	706	713	723	rBV	125223	216919	22.06%	2.280%
15	7.351	735	742	759	rBV	166336	296659	30.17%	3.118%
16	7.504	765	768	769	rBV3	1254	1221	0.12%	0.013%
17	7.581	779	781	783	rVB3	1425	1193	0.12%	0.013%
18	7.604	783	785	789	rBV5	1324	1951	0.20%	0.021%
19	7.645	791	792	798	rVB5	1182	1478	0.15%	0.016%
20	7.834	817	824	836	rBV	114951	204156	20.76%	2.145%
21	8.316	903	906	907	rBV2	1099	1142	0.12%	0.012%
22	8.551	940	946	965	rBV	143541	285593	29.05%	3.001%
23	8.681	965	968	970	rVV4	2531	2983	0.30%	0.031%
24	8.704	970	972	976	rVB4	1558	1642	0.17%	0.017%
25	9.034	1022	1028	1040	rBV	137189	257403	26.18%	2.705%
26	9.304	1073	1074	1077	rVB3	1184	1013	0.10%	0.011%
27	9.745	1140	1149	1163	rBV	124885	233914	23.79%	2.458%
28	9.969	1186	1187	1190	rBV4	1137	1069	0.11%	0.011%
29	10.134	1212	1215	1220	rBV5	685	1233	0.13%	0.013%
30	10.275	1232	1239	1252	rBV	143581	288313	29.32%	3.030%
31	10.410	1261	1262	1267	rVB3	2184	2039	0.21%	0.021%
32	10.645	1295	1302	1317	rBV	146669	258627	26.30%	2.718%
33	10.822	1326	1332	1348	rBV	111566	267972	27.25%	2.816%
34	10.998	1360	1362	1367	rVB4	1480	1236	0.13%	0.013%
35	11.086	1375	1377	1380	rVB4	966	1064	0.11%	0.011%
36	11.639	1468	1471	1474	rVB3	946	1343	0.14%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
 Data File : BM042711.D
 Acq On : 13 Nov 2023 17:12
 Operator : MA/JU
 Sample : PB156652BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK652

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

37	11.886	1508	1513	1516	rBV5	1050	1712	0.17%	0.018%
38	11.951	1522	1524	1528	rBV5	786	1236	0.13%	0.013%
39	12.257	1572	1576	1578	rBV4	943	1493	0.15%	0.016%
40	13.327	1757	1758	1759	rBV	1832	1070	0.11%	0.011%
41	13.345	1759	1761	1766	rVB5	2982	3707	0.38%	0.039%
42	13.533	1791	1793	1796	rBV4	1009	1317	0.13%	0.014%
43	13.627	1805	1809	1813	rVB4	923	1323	0.13%	0.014%
44	13.669	1813	1816	1819	rBV3	837	1145	0.12%	0.012%
45	13.916	1852	1858	1871	rBV	342835	508731	51.74%	5.346%
46	14.086	1884	1887	1889	rVB3	966	1172	0.12%	0.012%
47	14.192	1898	1905	1921	rBV	364907	548515	55.79%	5.764%
48	14.492	1950	1956	1966	rBV	243221	347094	35.30%	3.648%
49	14.751	1993	2000	2013	rBV3	36961	125912	12.81%	1.323%
50	15.057	2050	2052	2057	rVB6	1024	1558	0.16%	0.016%
51	15.110	2057	2061	2064	rVB5	1614	2153	0.22%	0.023%
52	15.133	2064	2065	2068	rBV3	1139	1203	0.12%	0.013%
53	15.286	2088	2091	2093	rBV4	926	1168	0.12%	0.012%
54	15.321	2093	2097	2099	rVB2	962	1207	0.12%	0.013%
55	15.486	2119	2125	2139	rBV	463185	673081	68.46%	7.073%
56	15.633	2144	2150	2162	rBV	145217	232251	23.62%	2.441%
57	16.115	2227	2232	2237	rBV6	599	1359	0.14%	0.014%
58	17.245	2418	2424	2435	rBV	286344	432827	44.02%	4.549%
59	17.345	2435	2441	2462	rVB	498757	764079	77.71%	8.030%
60	17.533	2469	2473	2476	rVB4	1404	2330	0.24%	0.024%
61	17.651	2491	2493	2495	rBV3	1342	1338	0.14%	0.014%
62	18.104	2566	2570	2580	rBV8	9497	27805	2.83%	0.292%
63	18.168	2580	2581	2586	rVB3	3042	3242	0.33%	0.034%
64	18.204	2586	2587	2591	rBV4	832	1069	0.11%	0.011%
65	18.380	2613	2617	2619	rBV5	1196	1387	0.14%	0.015%
66	18.545	2643	2645	2648	rVB4	1205	1275	0.13%	0.013%
67	18.609	2655	2656	2659	rBV3	1440	1298	0.13%	0.014%
68	18.751	2676	2680	2682	rVB4	1410	1751	0.18%	0.018%
69	18.780	2682	2685	2686	rBV3	1628	1085	0.11%	0.011%
70	18.798	2686	2688	2690	rBV3	870	986	0.10%	0.010%
71	19.004	2722	2723	2725	rVB2	1978	1217	0.12%	0.013%
72	19.204	2754	2757	2764	rVB6	4963	6692	0.68%	0.070%
73	19.280	2767	2770	2774	rBV4	3974	5279	0.54%	0.055%
74	19.404	2786	2791	2793	rBV5	4044	5703	0.58%	0.060%
75	19.645	2826	2832	2847	rBV	656124	919231	93.49%	9.660%
76	21.433	3131	3136	3147	rBV	319391	493966	50.24%	5.191%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042711.D
Acq On : 13 Nov 2023 17:12
Operator : MA/JU
Sample : PB156652BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK652

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Title : SVOA CALIBRATION

77	23.650	3506	3513	3528	rBV2	462814	983212	100.00%	10.333%
78	23.803	3533	3539	3551	rVB	260591	548465	55.78%	5.764%




Sum of corrected areas: 9515613

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042711.D
Acq On : 13 Nov 2023 17:12
Operator : MA/JU
Sample : PB156652BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK652

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

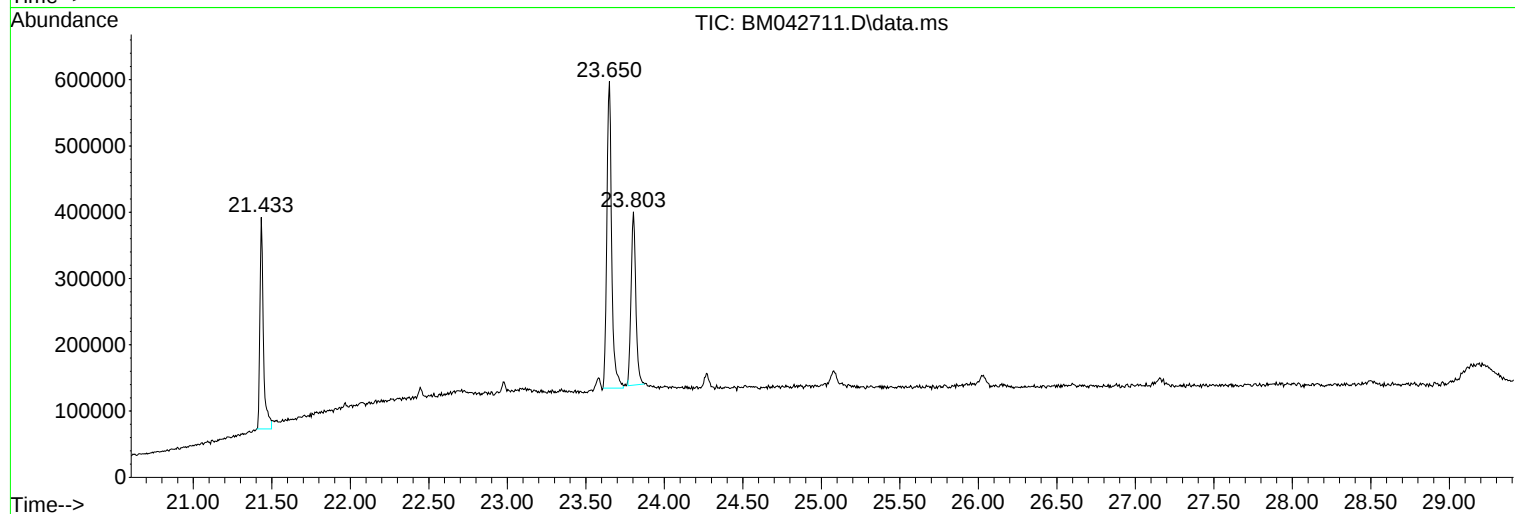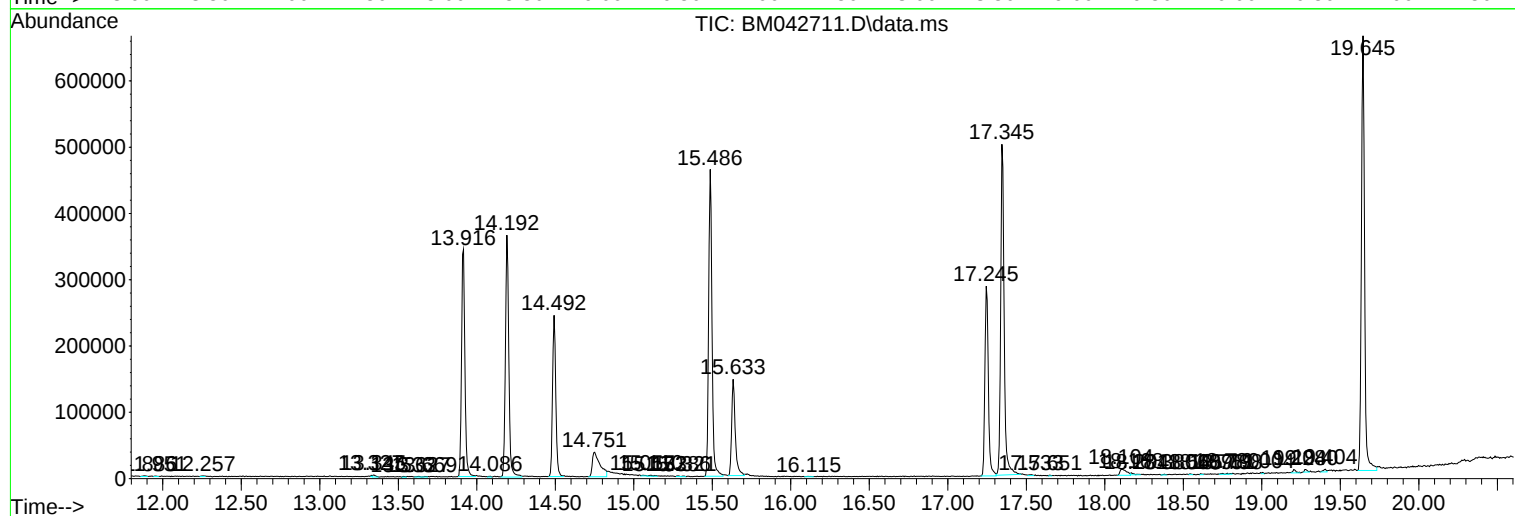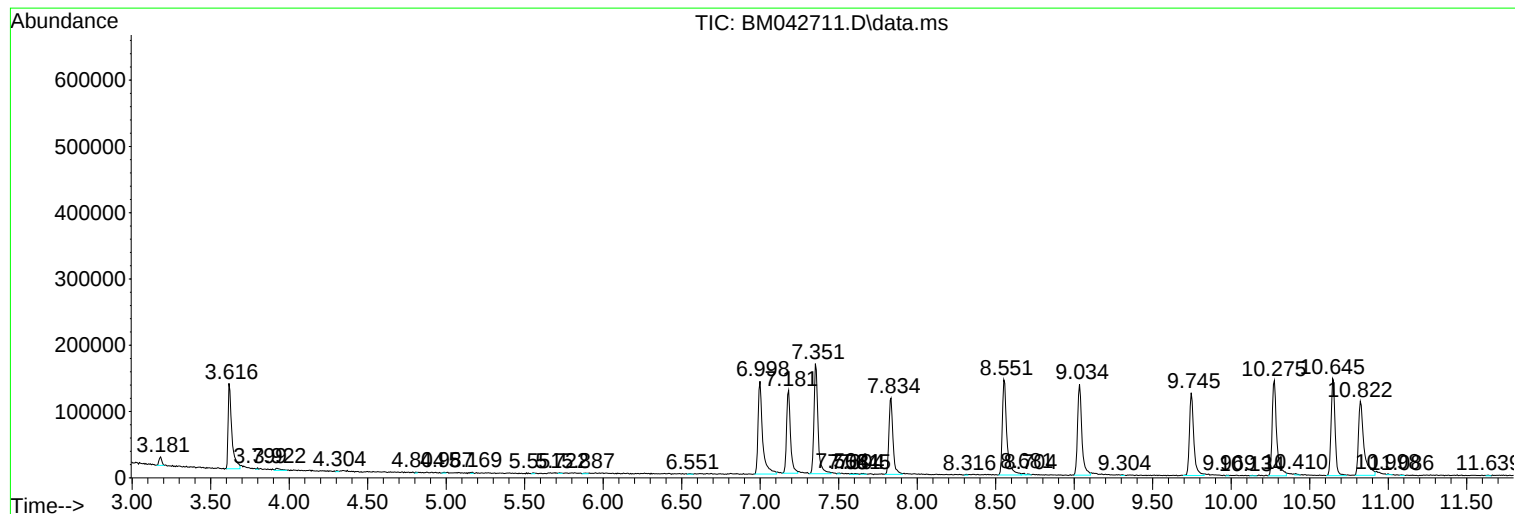

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042711.D
Acq On : 13 Nov 2023 17:12
Operator : MA/JU
Sample : PB156652BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK652

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042711.D
Acq On : 13 Nov 2023 17:12
Operator : MA/JU
Sample : PB156652BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK652

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc