

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
 Data File : BM042715.D
 Acq On : 13 Nov 2023 23:12
 Operator : MA/JU
 Sample : PB156684BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK684

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM042715.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	30	33	39	rVB	15801	19297	1.67%	0.180%
2	3.622	105	108	127	rBV	149847	252388	21.83%	2.357%
3	5.122	361	363	366	rBV3	958	1239	0.11%	0.012%
4	5.275	387	389	391	rBV2	1750	1793	0.16%	0.017%
5	5.599	442	444	448	rBV3	1269	1498	0.13%	0.014%
6	5.699	459	461	464	rBV3	1288	1204	0.10%	0.011%
7	6.304	563	564	570	rBV5	1370	1711	0.15%	0.016%
8	6.622	616	618	621	rVB4	1364	1199	0.10%	0.011%
9	6.998	676	682	703	rBV	145898	295374	25.55%	2.759%
10	7.181	708	713	725	rVV	121024	209725	18.14%	1.959%
11	7.357	737	743	758	rBV	178551	305848	26.45%	2.856%
12	7.781	813	815	818	rVB4	1408	1256	0.11%	0.012%
13	7.834	818	824	835	rBV	128942	231959	20.06%	2.166%
14	7.910	835	837	840	rVV3	2785	3959	0.34%	0.037%
15	7.957	844	845	850	rVV4	1251	1485	0.13%	0.014%
16	8.287	899	901	904	rBV2	1037	1382	0.12%	0.013%
17	8.557	940	947	965	rBV	195735	388383	33.59%	3.627%
18	9.039	1022	1029	1043	rBV	180007	349315	30.21%	3.262%
19	9.263	1065	1067	1072	rVB4	1221	2034	0.18%	0.019%
20	9.751	1144	1150	1164	rBV	148908	288486	24.95%	2.694%
21	10.275	1233	1239	1251	rBV	179825	348817	30.17%	3.258%
22	10.386	1256	1258	1263	rVV6	3327	6331	0.55%	0.059%
23	10.598	1292	1294	1297	rBV2	1413	1200	0.10%	0.011%
24	10.651	1297	1303	1314	rVV	164316	290726	25.15%	2.715%
25	10.828	1326	1333	1354	rBV	126302	310395	26.85%	2.899%
26	11.045	1368	1370	1375	rVB3	1398	1553	0.13%	0.015%
27	11.233	1398	1402	1405	rVB4	965	1327	0.11%	0.012%
28	12.263	1573	1577	1583	rBV6	1111	2021	0.17%	0.019%
29	12.663	1640	1645	1646	rBV3	1096	1168	0.10%	0.011%
30	12.698	1649	1651	1657	rVB4	869	1198	0.10%	0.011%
31	13.345	1754	1761	1765	rBV3	3690	6111	0.53%	0.057%
32	13.916	1852	1858	1870	rBV	400879	559031	48.35%	5.221%
33	14.192	1899	1905	1920	rBV2	388567	598568	51.77%	5.590%
34	14.492	1950	1956	1969	rBV	259615	381596	33.01%	3.564%
35	14.745	1993	1999	2023	rBV2	42371	167916	14.52%	1.568%
36	15.333	2096	2099	2101	rBV3	1329	1798	0.16%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
 Data File : BM042715.D
 Acq On : 13 Nov 2023 23:12
 Operator : MA/JU
 Sample : PB156684BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK684

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

37	15.486	2119	2125	2144	rVV	497185	746212	64.54%	6.969%
38	15.633	2144	2150	2164	rVV	155629	264094	22.84%	2.466%
39	15.727	2164	2166	2170	rVV4	4387	6291	0.54%	0.059%
40	15.780	2174	2175	2180	rVB5	1529	2081	0.18%	0.019%
41	17.245	2419	2424	2435	rBV	303186	450950	39.00%	4.212%
42	17.345	2435	2441	2456	rVV	497320	788717	68.22%	7.366%
43	17.833	2520	2524	2527	rVB3	770	1356	0.12%	0.013%
44	17.880	2527	2532	2535	rBV4	902	1655	0.14%	0.015%
45	18.068	2562	2564	2567	rBV	1222	1719	0.15%	0.016%
46	18.115	2567	2572	2573	rVV4	3434	4794	0.41%	0.045%
47	18.145	2575	2577	2579	rVV4	3270	3835	0.33%	0.036%
48	18.186	2583	2584	2586	rVV2	1680	1405	0.12%	0.013%
49	18.209	2586	2588	2591	rVB3	1252	1377	0.12%	0.013%
50	18.245	2591	2594	2595	rBV2	1199	1308	0.11%	0.012%
51	18.392	2614	2619	2621	rVV4	1058	1481	0.13%	0.014%
52	18.668	2663	2666	2668	rBV3	1555	1758	0.15%	0.016%
53	18.756	2676	2681	2682	rVB4	1244	1664	0.14%	0.016%
54	18.780	2682	2685	2686	rBV3	1036	1190	0.10%	0.011%
55	19.051	2728	2731	2734	rVB3	2068	2075	0.18%	0.019%
56	19.074	2734	2735	2738	rBV3	1344	1378	0.12%	0.013%
57	19.133	2743	2745	2749	rVB3	1460	1797	0.16%	0.017%
58	19.204	2754	2757	2764	rVB3	5736	7545	0.65%	0.070%
59	19.280	2766	2770	2777	rBV4	4474	7664	0.66%	0.072%
60	19.409	2790	2792	2793	rBV2	1474	1221	0.11%	0.011%
61	19.515	2809	2810	2815	rBV4	1558	1570	0.14%	0.015%
62	19.639	2826	2831	2849	rBV	698556	1004370	86.87%	9.380%
63	20.080	2904	2906	2907	rBV	3176	2461	0.21%	0.023%
64	21.427	3130	3135	3148	rBV	364212	577912	49.99%	5.397%
65	23.639	3505	3511	3528	rBV	562152	1156141	100.00%	10.798%
66	23.797	3532	3538	3549	rVB	305485	622080	53.81%	5.810%


Sum of corrected areas: 10707392

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042715.D
Acq On : 13 Nov 2023 23:12
Operator : MA/JU
Sample : PB156684BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK684

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

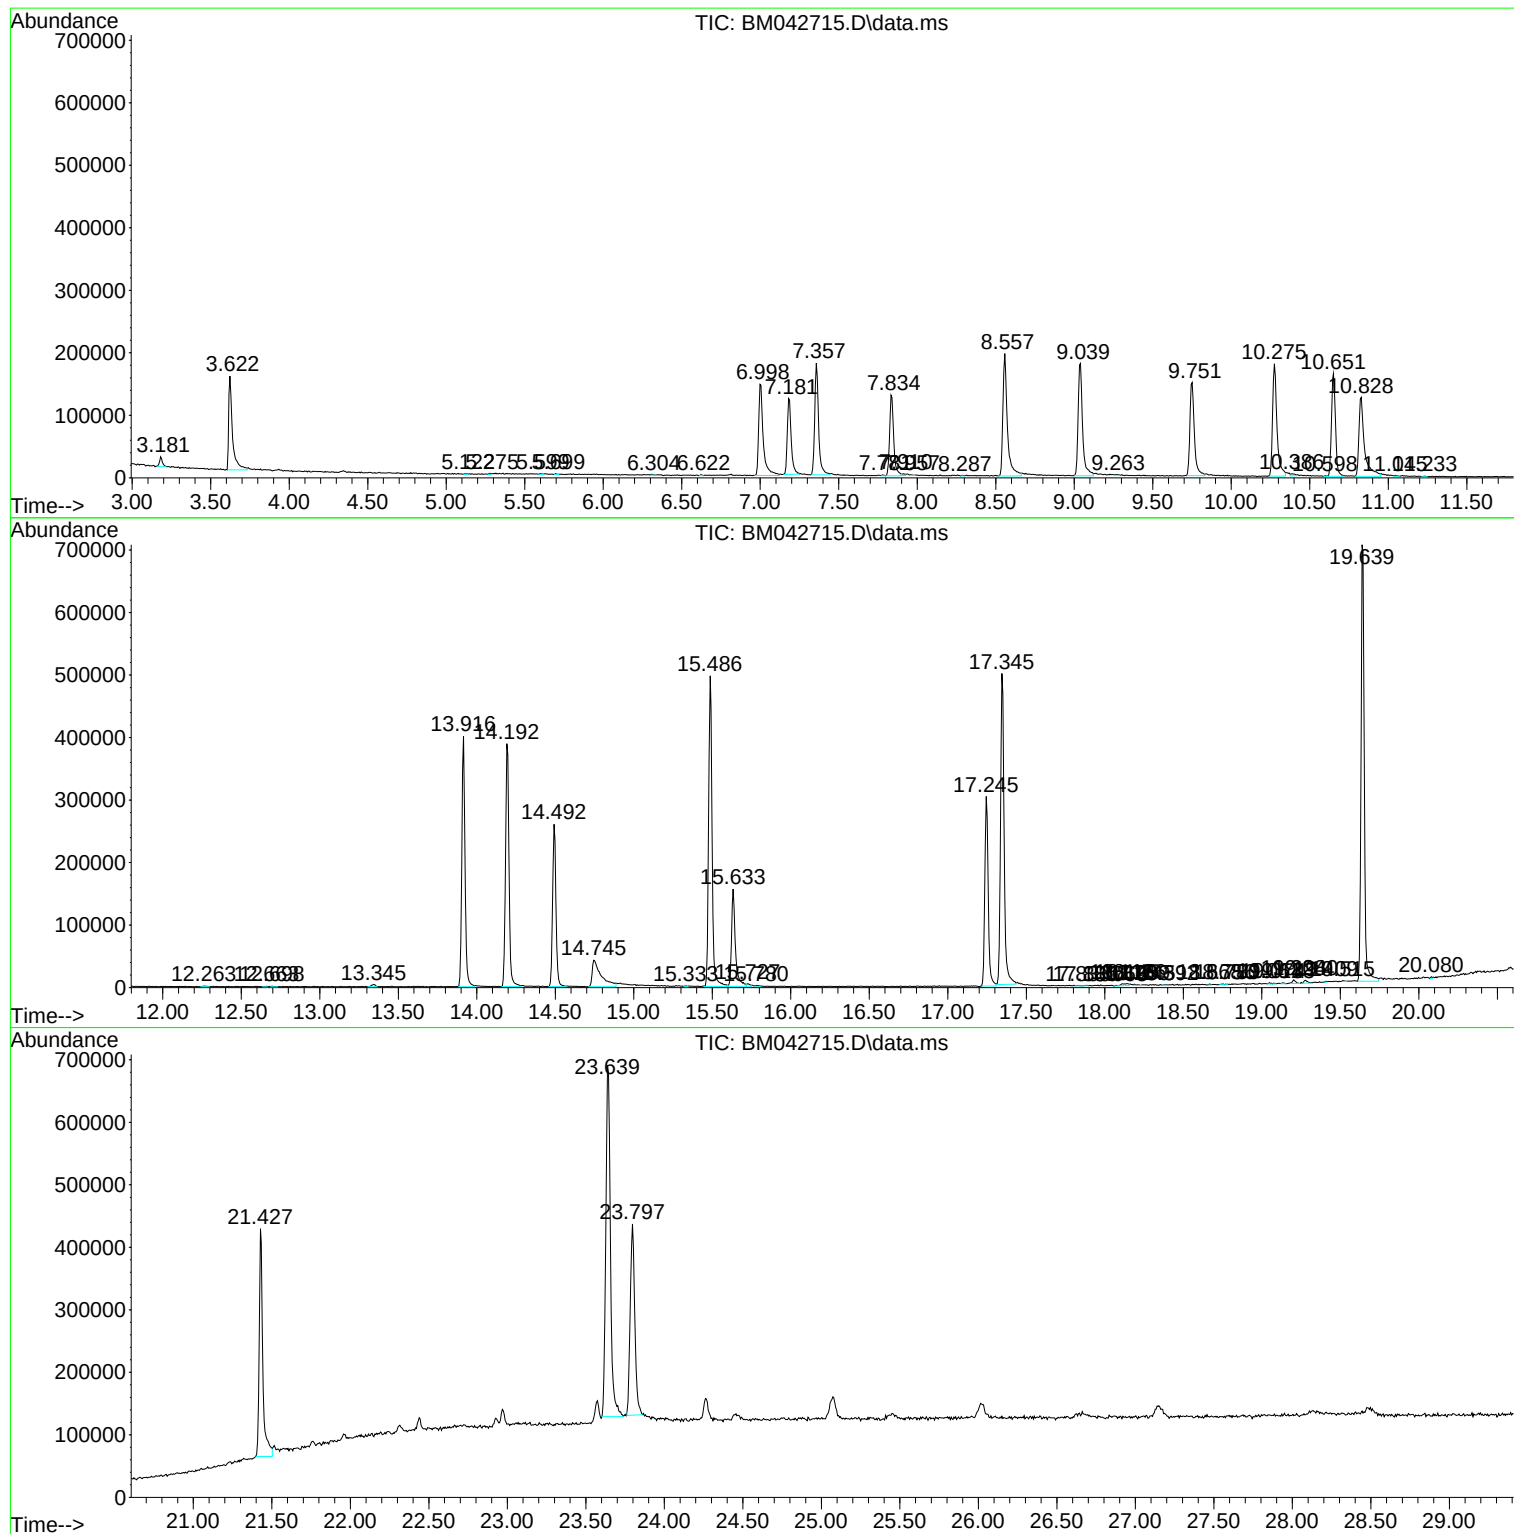

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042715.D
Acq On : 13 Nov 2023 23:12
Operator : MA/JU
Sample : PB156684BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK684

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042715.D
Acq On : 13 Nov 2023 23:12
Operator : MA/JU
Sample : PB156684BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK684

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc