

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
 Data File : BM042716.D
 Acq On : 13 Nov 2023 23:48
 Operator : MA/JU
 Sample : PB156721BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK721

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM042716.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.028	5	7	8	rBV2	3709	1442	0.13%	0.014%
2	3.181	30	33	39	rVB	16040	21510	1.98%	0.202%
3	3.622	105	108	120	rBV	173392	282176	25.95%	2.652%
4	5.410	409	412	413	rBV3	1636	1453	0.13%	0.014%
5	5.640	449	451	455	rVB4	1254	1156	0.11%	0.011%
6	6.134	534	535	538	rBV2	1110	1257	0.12%	0.012%
7	6.287	558	561	563	rBV2	1096	1456	0.13%	0.014%
8	6.381	576	577	579	rBV2	1871	1355	0.12%	0.013%
9	6.604	612	615	617	rBV3	1530	1426	0.13%	0.013%
10	6.634	617	620	623	rVB4	1435	2137	0.20%	0.020%
11	6.810	646	650	653	rVV5	1270	1414	0.13%	0.013%
12	7.004	676	683	706	rBV	166436	347443	31.95%	3.266%
13	7.181	708	713	725	rBV	146572	255737	23.52%	2.404%
14	7.357	737	743	762	rBV	198281	350534	32.24%	3.295%
15	7.839	817	825	836	rBV	112433	206141	18.96%	1.938%
16	8.004	851	853	858	rVB4	1402	2042	0.19%	0.019%
17	8.275	896	899	902	rBV5	753	1175	0.11%	0.011%
18	8.469	929	932	935	rVB4	1136	1264	0.12%	0.012%
19	8.504	935	938	940	rBV3	977	1130	0.10%	0.011%
20	8.557	940	947	963	rBV	186153	371112	34.13%	3.488%
21	9.039	1021	1029	1042	rBV	173600	337463	31.04%	3.172%
22	9.263	1066	1067	1070	rBV2	1200	1270	0.12%	0.012%
23	9.286	1070	1071	1074	rVB3	1602	1202	0.11%	0.011%
24	9.375	1083	1086	1088	rVB4	1100	1230	0.11%	0.012%
25	9.557	1115	1117	1122	rBV5	900	1444	0.13%	0.014%
26	9.639	1130	1131	1137	rVB5	1093	1119	0.10%	0.011%
27	9.751	1143	1150	1166	rBV	145681	288805	26.56%	2.714%
28	9.904	1175	1176	1179	rBV2	1658	1809	0.17%	0.017%
29	10.004	1191	1193	1195	rBV2	1252	1091	0.10%	0.010%
30	10.275	1233	1239	1259	rBV	178071	371482	34.17%	3.492%
31	10.651	1296	1303	1315	rBV	156691	271062	24.93%	2.548%
32	10.828	1326	1333	1355	rBV	137566	349711	32.16%	3.287%
33	10.975	1357	1358	1360	rVV2	2235	1419	0.13%	0.013%
34	11.086	1374	1377	1383	rVB7	1135	2341	0.22%	0.022%
35	11.669	1473	1476	1477	rBV3	1457	1115	0.10%	0.010%
36	11.804	1493	1499	1500	rBV3	959	1189	0.11%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
 Data File : BM042716.D
 Acq On : 13 Nov 2023 23:48
 Operator : MA/JU
 Sample : PB156721BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK721

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

37	12.192	1561	1565	1568	rVB5	1001	1571	0.14%	0.015%
38	13.339	1755	1760	1769	rVB5	1936	3315	0.30%	0.031%
39	13.616	1805	1807	1811	rVB4	1017	1139	0.10%	0.011%
40	13.916	1852	1858	1870	rBV	402007	590877	54.34%	5.554%
41	14.192	1899	1905	1920	rVV	440685	647104	59.52%	6.082%
42	14.286	1920	1921	1927	rVV3	2299	3117	0.29%	0.029%
43	14.327	1927	1928	1932	rVB3	990	1100	0.10%	0.010%
44	14.492	1950	1956	1971	rBV	233878	342517	31.50%	3.219%
45	14.592	1971	1973	1978	rVB4	826	1211	0.11%	0.011%
46	14.751	1993	2000	2018	rBV3	41838	158500	14.58%	1.490%
47	14.945	2032	2033	2036	rVB2	2337	1402	0.13%	0.013%
48	15.486	2119	2125	2142	rBV	539055	789483	72.61%	7.420%
49	15.633	2145	2150	2164	rVV	151739	253555	23.32%	2.383%
50	15.721	2164	2165	2168	rVB3	2579	2169	0.20%	0.020%
51	15.804	2178	2179	2183	rVB4	1326	1125	0.10%	0.011%
52	16.410	2277	2282	2285	rBV4	556	1227	0.11%	0.012%
53	17.245	2418	2424	2435	rVV	270595	397089	36.52%	3.732%
54	17.345	2435	2441	2465	rVB	553238	845282	77.74%	7.945%
55	17.704	2501	2502	2505	rBV3	1210	1247	0.11%	0.012%
56	17.886	2530	2533	2534	rBV2	1092	1179	0.11%	0.011%
57	17.956	2543	2545	2548	rVB3	909	1128	0.10%	0.011%
58	17.992	2548	2551	2552	rBV2	1211	1133	0.10%	0.011%
59	18.115	2567	2572	2573	rBV3	4277	5780	0.53%	0.054%
60	18.133	2573	2575	2581	rVV7	3891	7656	0.70%	0.072%
61	18.192	2583	2585	2586	rVB2	2056	1203	0.11%	0.011%
62	18.268	2597	2598	2602	rBV4	1920	2190	0.20%	0.021%
63	18.321	2605	2607	2610	rVV4	1150	1431	0.13%	0.013%
64	18.509	2637	2639	2642	rVB3	1190	1115	0.10%	0.010%
65	18.539	2642	2644	2645	rVB2	1647	1090	0.10%	0.010%
66	18.551	2645	2646	2648	rBV2	1793	1276	0.12%	0.012%
67	18.733	2673	2677	2679	rBV4	1655	2661	0.24%	0.025%
68	18.839	2693	2695	2697	rBV2	1452	1486	0.14%	0.014%
69	18.898	2702	2705	2707	rBV3	1364	2055	0.19%	0.019%
70	18.962	2714	2716	2720	rVB3	1393	1490	0.14%	0.014%
71	19.203	2754	2757	2762	rBV6	6064	6898	0.63%	0.065%
72	19.280	2767	2770	2773	rVV3	4207	4682	0.43%	0.044%
73	19.409	2787	2792	2793	rBV5	2535	4130	0.38%	0.039%
74	19.486	2803	2805	2806	rBV2	1833	1205	0.11%	0.011%
75	19.568	2817	2819	2820	rBV2	1634	1300	0.12%	0.012%
76	19.639	2825	2831	2842	rBV	747739	1032648	94.97%	9.706%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042716.D
Acq On : 13 Nov 2023 23:48
Operator : MA/JU
Sample : PB156721BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK721

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Title : SVOA CALIBRATION

77	21.427	3131	3135	3148	rBV	260860	433610	39.88%	4.075%
78	23.644	3505	3512	3525	rBV	534772	1087292	100.00%	10.219%
79	23.797	3532	3538	3553	rVB	226853	504698	46.42%	4.744%




Sum of corrected areas: 10639478

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042716.D
Acq On : 13 Nov 2023 23:48
Operator : MA/JU
Sample : PB156721BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK721

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

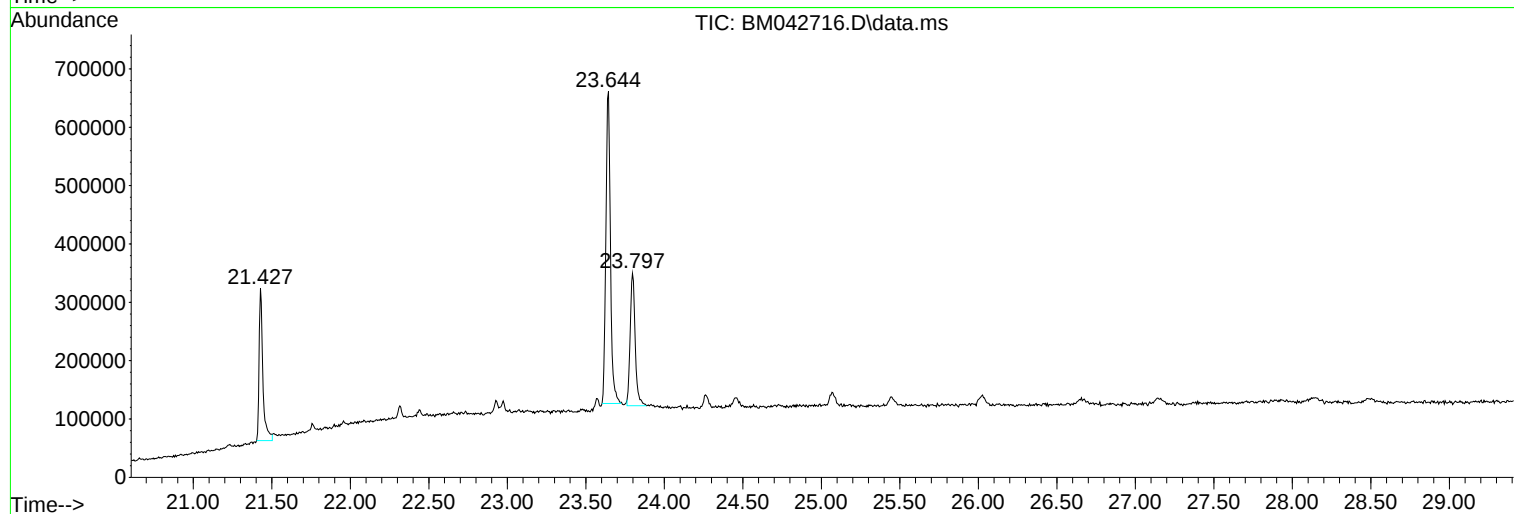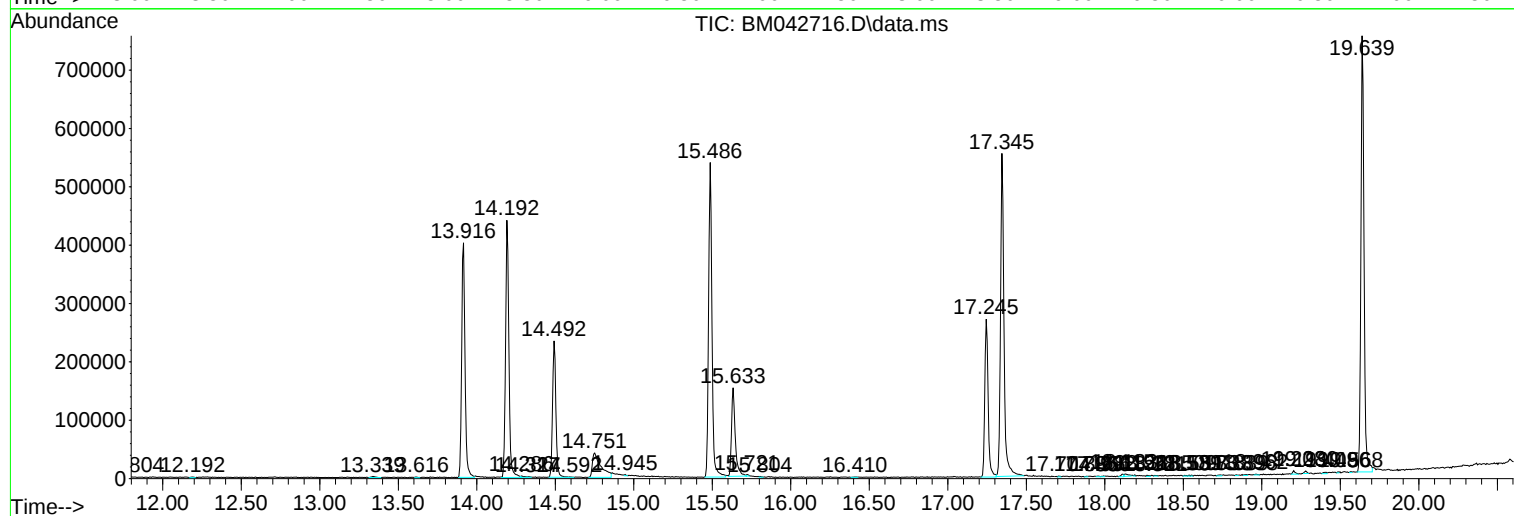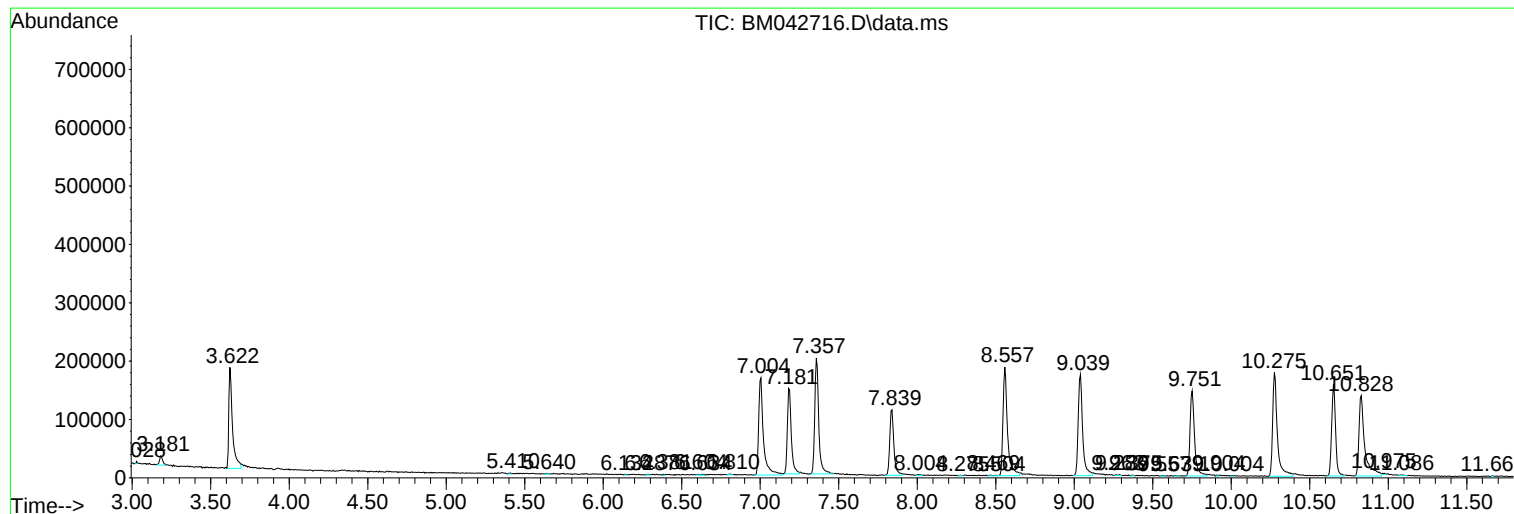

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042716.D
Acq On : 13 Nov 2023 23:48
Operator : MA/JU
Sample : PB156721BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK721

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042716.D
Acq On : 13 Nov 2023 23:48
Operator : MA/JU
Sample : PB156721BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK721

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc