

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
 Data File : BM042726.D
 Acq On : 14 Nov 2023 07:02
 Operator : MA/JU
 Sample : PB156765BL
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK765

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM042726.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	30	33	40	rVB2	19115	25739	1.89%	0.182%
2	3.622	104	108	123	rBV	212457	340776	25.01%	2.405%
3	3.928	158	160	165	rVB6	3982	5004	0.37%	0.035%
4	4.905	324	326	329	rBV3	1618	2157	0.16%	0.015%
5	5.875	489	491	495	rVB4	1330	1700	0.12%	0.012%
6	7.004	675	683	701	rBV	227607	425639	31.23%	3.004%
7	7.181	708	713	733	rVB	184506	312216	22.91%	2.203%
8	7.357	737	743	757	rBV	256133	421966	30.96%	2.978%
9	7.834	818	824	835	rBV	177858	307608	22.57%	2.171%
10	7.916	837	838	840	rVV2	2437	1866	0.14%	0.013%
11	8.557	941	947	964	rBV	252354	474874	34.85%	3.351%
12	9.034	1021	1028	1045	rBV	220794	413018	30.31%	2.915%
13	9.745	1142	1149	1164	rBV	194419	365971	26.86%	2.583%
14	9.892	1173	1174	1179	rVB5	1171	1514	0.11%	0.011%
15	10.275	1233	1239	1256	rBV	240697	481011	35.30%	3.395%
16	10.398	1258	1260	1263	rVB4	2144	2119	0.16%	0.015%
17	10.522	1280	1281	1286	rVB3	1221	1391	0.10%	0.010%
18	10.651	1296	1303	1314	rBV	233819	415865	30.52%	2.935%
19	10.828	1324	1333	1355	rBV	188283	452341	33.19%	3.192%
20	10.992	1359	1361	1365	rVV3	3587	5559	0.41%	0.039%
21	11.028	1365	1367	1369	rVV3	2480	2452	0.18%	0.017%
22	11.045	1369	1370	1372	rVV	2486	1484	0.11%	0.010%
23	11.834	1497	1504	1507	rVB4	671	1696	0.12%	0.012%
24	12.251	1571	1575	1578	rBV3	1681	2832	0.21%	0.020%
25	13.339	1755	1760	1767	rVB4	3104	5530	0.41%	0.039%
26	13.916	1851	1858	1871	rBV	536333	749529	55.00%	5.290%
27	14.045	1877	1880	1883	rVB4	1151	1482	0.11%	0.010%
28	14.192	1898	1905	1919	rBV	577844	827055	60.69%	5.837%
29	14.492	1950	1956	1965	rBV	385499	550493	40.40%	3.885%
30	14.751	1994	2000	2016	rBV2	65006	214810	15.76%	1.516%
31	15.304	2092	2094	2096	rVB3	1501	1400	0.10%	0.010%
32	15.486	2119	2125	2138	rBV	691669	1015443	74.52%	7.166%
33	15.627	2144	2149	2162	rBV	219772	347349	25.49%	2.451%
34	15.845	2184	2186	2191	rVB4	1431	1923	0.14%	0.014%
35	17.245	2418	2424	2434	rVV	441455	641191	47.05%	4.525%
36	17.345	2435	2441	2470	rVB	747870	1107633	81.28%	7.817%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
 Data File : BM042726.D
 Acq On : 14 Nov 2023 07:02
 Operator : MA/JU
 Sample : PB156765BL
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK765

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

37	17.915	2534	2538	2540	rBV4	850	1410	0.10%	0.010%
38	18.104	2566	2570	2571	rBV2	5329	5722	0.42%	0.040%
39	18.345	2610	2611	2617	rBV5	1717	2438	0.18%	0.017%
40	18.486	2633	2635	2639	rBV5	2038	2544	0.19%	0.018%
41	18.680	2665	2668	2672	rBV5	1229	1942	0.14%	0.014%
42	18.851	2695	2697	2700	rBV4	1442	1565	0.11%	0.011%
43	18.962	2715	2716	2719	rBV4	1381	1595	0.12%	0.011%
44	19.198	2750	2756	2761	rBV7	7805	16682	1.22%	0.118%
45	19.245	2761	2764	2765	rBV3	1331	1569	0.12%	0.011%
46	19.274	2765	2769	2774	rVV2	7547	11346	0.83%	0.080%
47	19.639	2825	2831	2846	rBV	1002603	1329730	97.58%	9.384%
48	21.427	3130	3135	3147	rBV	491684	721305	52.93%	5.090%
49	23.639	3505	3511	3523	rBV	668702	1362731	100.00%	9.617%
50	23.797	3531	3538	3548	rBV	376471	778857	57.15%	5.496%




Sum of corrected areas: 14170072

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042726.D
Acq On : 14 Nov 2023 07:02
Operator : MA/JU
Sample : PB156765BL
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK765

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

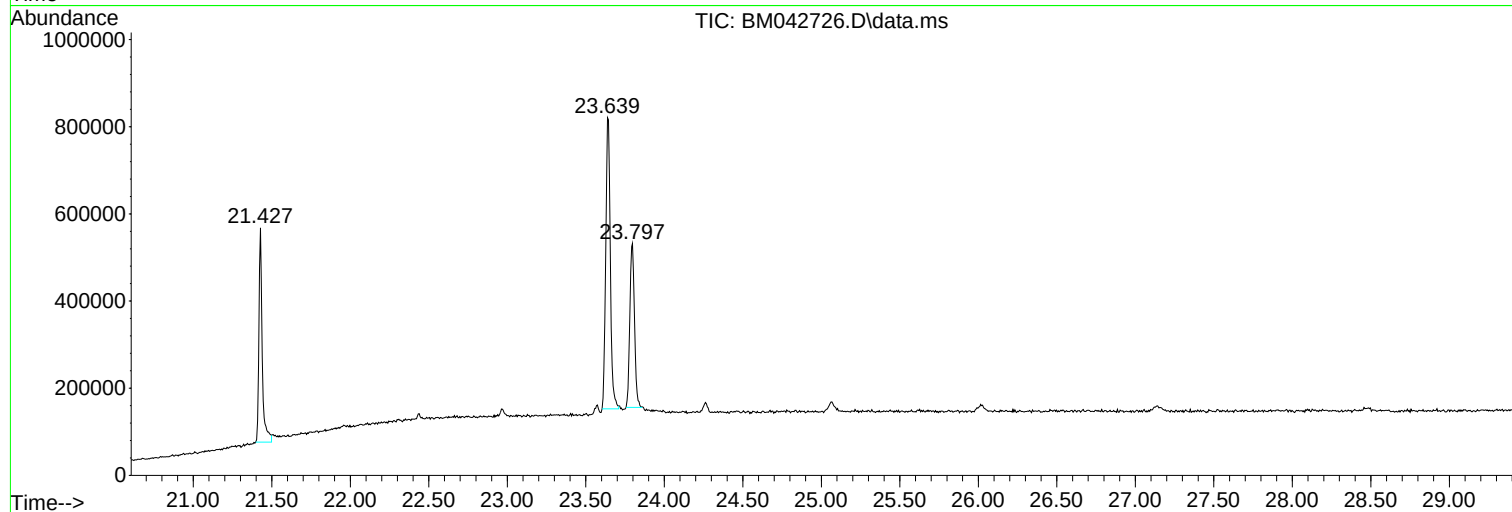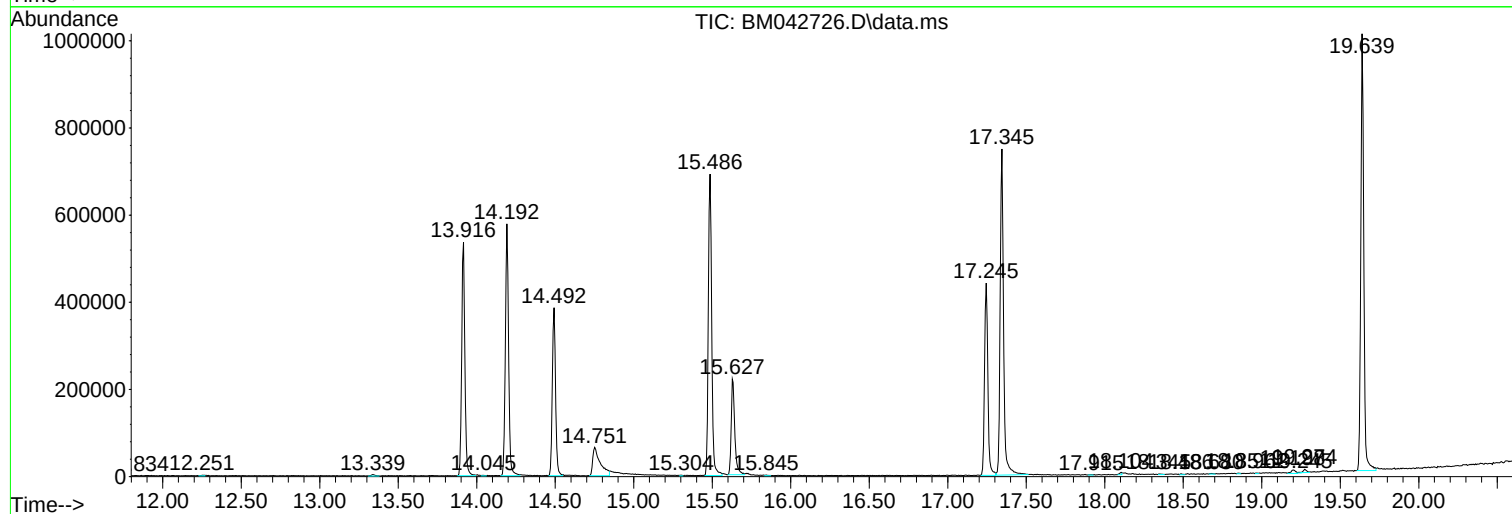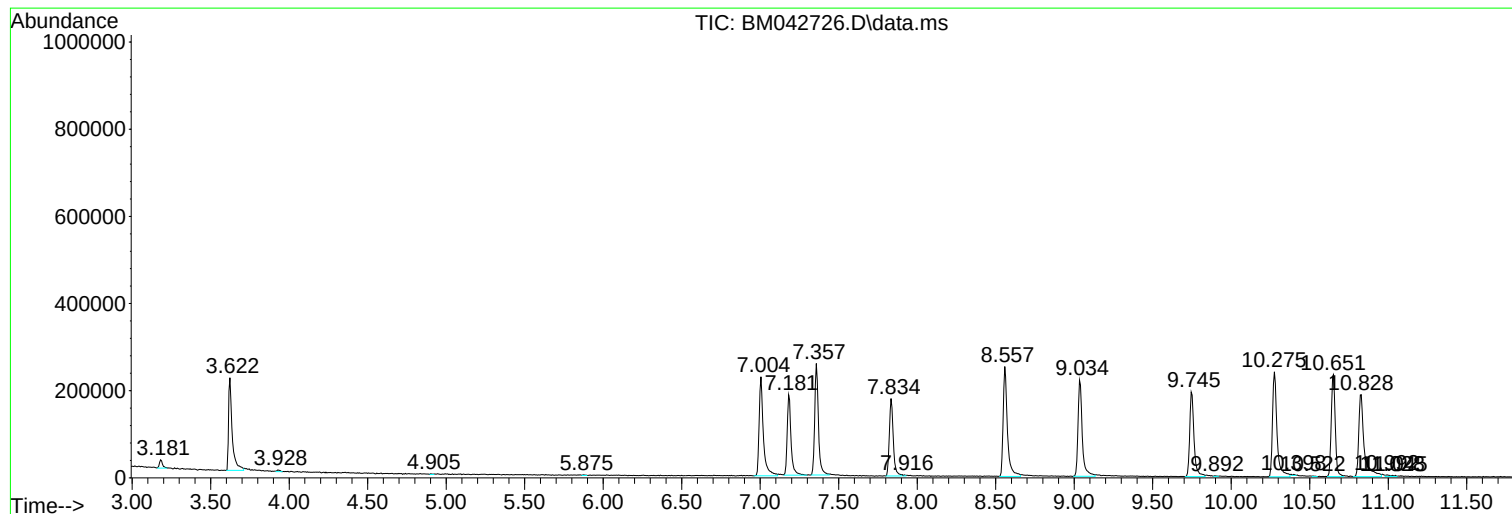

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042726.D
Acq On : 14 Nov 2023 07:02
Operator : MA/JU
Sample : PB156765BL
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK765

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042726.D
Acq On : 14 Nov 2023 07:02
Operator : MA/JU
Sample : PB156765BL
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK765

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc