

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
 Data File : BM042735.D
 Acq On : 14 Nov 2023 15:58
 Operator : MA/JU
 Sample : PB156764BL
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK764

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM042735.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	29	33	39	rVB2	15875	22231	1.68%	0.173%
2	3.616	104	107	123	rBV	184846	305574	23.04%	2.383%
3	4.587	270	272	277	rBV3	1545	2445	0.18%	0.019%
4	5.087	355	357	359	rBV3	1339	1491	0.11%	0.012%
5	6.998	676	682	698	rBV	191782	369732	27.87%	2.884%
6	7.181	707	713	727	rBV	163793	279193	21.05%	2.178%
7	7.357	737	743	759	rBV	209750	373873	28.19%	2.916%
8	7.534	771	773	777	rVB5	1311	1725	0.13%	0.013%
9	7.728	800	806	809	rBV4	1119	2042	0.15%	0.016%
10	7.834	817	824	838	rBV	158607	275449	20.77%	2.148%
11	7.928	838	840	842	rVV3	1691	1425	0.11%	0.011%
12	7.945	842	843	847	rVB4	1843	1602	0.12%	0.012%
13	8.557	941	947	962	rBV	207004	400995	30.23%	3.128%
14	9.034	1021	1028	1048	rBV	193286	369465	27.85%	2.882%
15	9.239	1061	1063	1067	rVB4	1391	1357	0.10%	0.011%
16	9.745	1140	1149	1162	rBV	170775	318152	23.99%	2.482%
17	9.875	1170	1171	1176	rVV5	1335	1425	0.11%	0.011%
18	9.975	1186	1188	1194	rVB4	952	1525	0.11%	0.012%
19	10.275	1232	1239	1255	rBV	205911	401879	30.30%	3.135%
20	10.645	1293	1302	1316	rBV	211337	370170	27.91%	2.887%
21	10.822	1326	1332	1356	rBV	155931	378719	28.55%	2.954%
22	11.033	1366	1368	1372	rVB2	1874	2806	0.21%	0.022%
23	11.704	1480	1482	1486	rVB5	1215	1485	0.11%	0.012%
24	12.245	1571	1574	1576	rBV3	1041	1330	0.10%	0.010%
25	12.745	1657	1659	1665	rVB3	1111	1402	0.11%	0.011%
26	13.339	1755	1760	1763	rVB2	2007	2706	0.20%	0.021%
27	13.910	1851	1857	1871	rBV	481387	676598	51.01%	5.277%
28	14.192	1898	1905	1924	rBV	483097	732062	55.19%	5.710%
29	14.486	1949	1955	1970	rBV	334983	490326	36.97%	3.825%
30	14.745	1993	1999	2019	rBV3	56304	207983	15.68%	1.622%
31	15.480	2119	2124	2143	rBV	601893	907568	68.42%	7.079%
32	15.627	2144	2149	2164	rVV	205223	321996	24.28%	2.512%
33	17.239	2417	2423	2435	rBV	383308	583166	43.97%	4.549%
34	17.339	2435	2440	2456	rVV	639904	973109	73.36%	7.590%
35	18.109	2565	2571	2576	rBV6	2712	6881	0.52%	0.054%
36	18.192	2582	2585	2590	rVB4	1496	1875	0.14%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
 Data File : BM042735.D
 Acq On : 14 Nov 2023 15:58
 Operator : MA/JU
 Sample : PB156764BL
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK764

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

37	18.257	2594	2596	2599	rBV3	1983	2237	0.17%	0.017%
38	18.580	2649	2651	2655	rBV2	1714	1925	0.15%	0.015%
39	18.633	2655	2660	2661	rVV4	1127	1472	0.11%	0.011%
40	18.774	2681	2684	2686	rBV2	1217	1531	0.12%	0.012%
41	18.804	2686	2689	2693	rBV5	1345	1902	0.14%	0.015%
42	18.898	2703	2705	2710	rVB5	1471	2121	0.16%	0.017%
43	19.198	2752	2756	2760	rVV3	7196	9729	0.73%	0.076%
44	19.274	2766	2769	2776	rBV3	5374	8338	0.63%	0.065%
45	19.392	2786	2789	2791	rBV3	2296	2980	0.22%	0.023%
46	19.509	2807	2809	2813	rVB4	2209	2214	0.17%	0.017%
47	19.639	2825	2831	2845	rBV	942114	1249579	94.21%	9.747%
48	21.427	3130	3135	3145	rBV	465761	672066	50.67%	5.242%
49	23.639	3504	3511	3524	rBV	674911	1326428	100.00%	10.346%
50	23.791	3530	3537	3549	rVB	352459	746351	56.27%	5.821%




Sum of corrected areas: 12820635

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042735.D
Acq On : 14 Nov 2023 15:58
Operator : MA/JU
Sample : PB156764BL
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK764

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

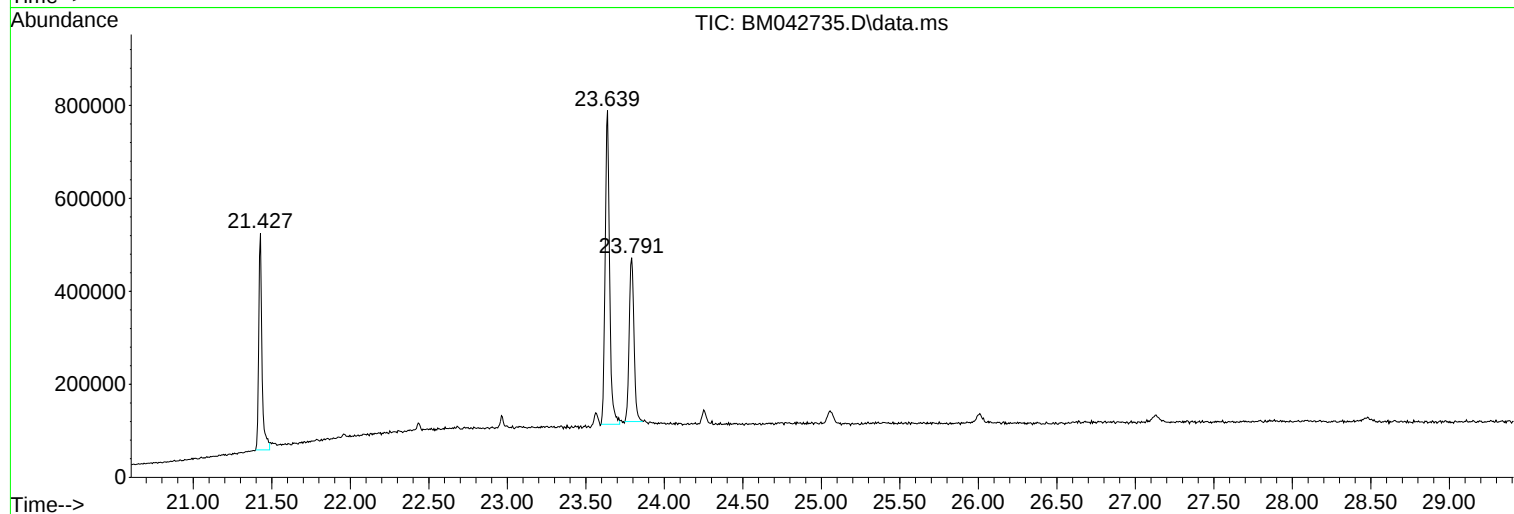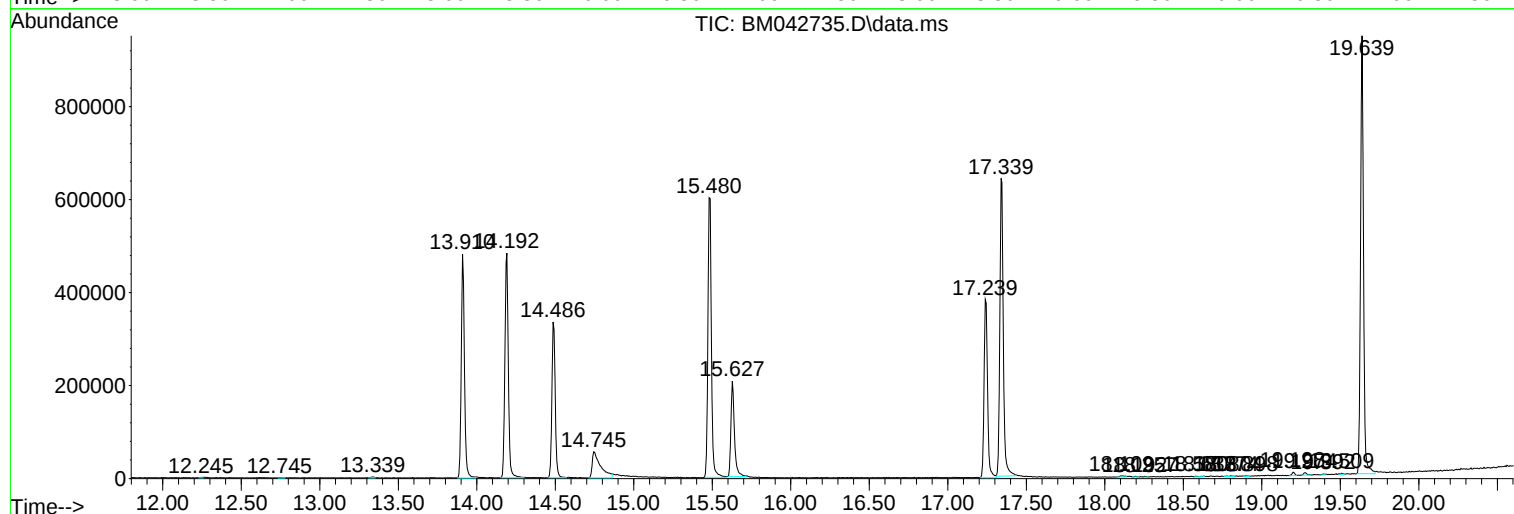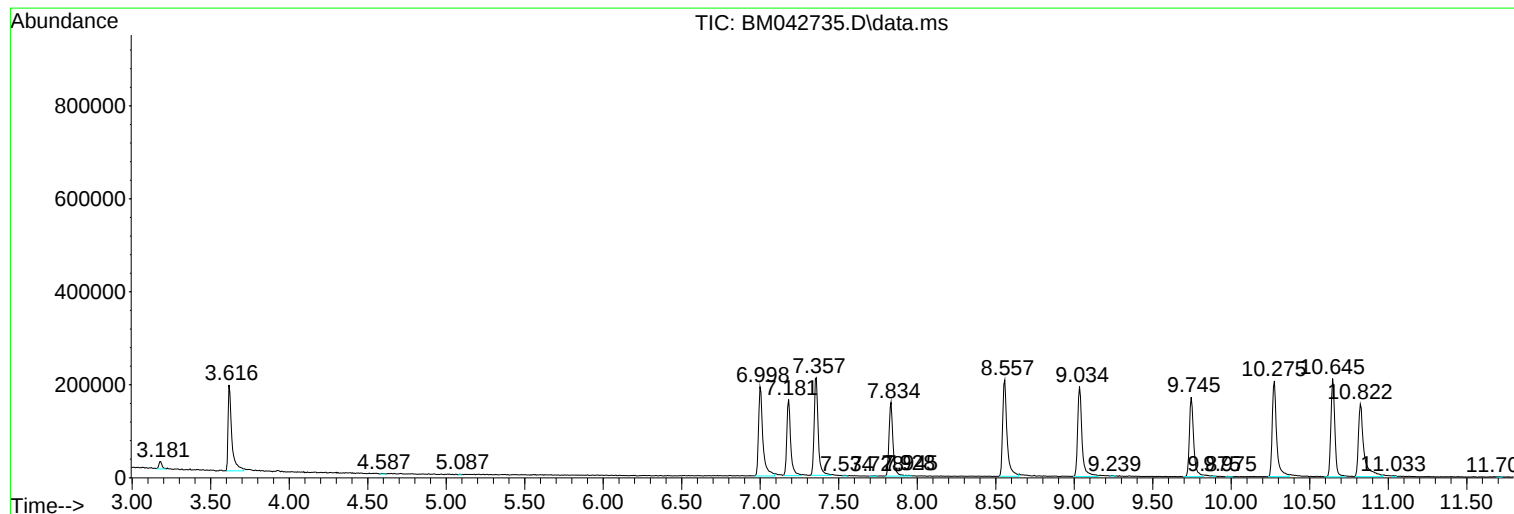

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042735.D
Acq On : 14 Nov 2023 15:58
Operator : MA/JU
Sample : PB156764BL
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK764

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042735.D
Acq On : 14 Nov 2023 15:58
Operator : MA/JU
Sample : PB156764BL
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK764

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc