

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
 Data File : BM042737.D
 Acq On : 14 Nov 2023 17:10
 Operator : MA/JU
 Sample : 05381-10
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SVOC-GPC2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M

Title : SVOA CALIBRATION

Signal : TIC: BM042737.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.687	458	459	461	rBV2	1430	1340	0.30%	0.070%
2	6.381	575	577	578	rBV	1094	687	0.15%	0.036%
3	6.746	635	639	642	rBV5	1461	1856	0.41%	0.097%
4	7.834	818	824	839	rBV	77906	164569	36.57%	8.615%
5	8.016	853	855	857	rVB3	1286	1151	0.26%	0.060%
6	8.322	905	907	911	rBV5	913	1063	0.24%	0.056%
7	8.681	967	968	970	rBV2	816	632	0.14%	0.033%
8	8.939	1010	1012	1015	rVB4	793	771	0.17%	0.040%
9	9.004	1020	1023	1025	rBV2	768	744	0.17%	0.039%
10	9.134	1043	1045	1047	rBV3	849	849	0.19%	0.044%
11	9.910	1175	1177	1182	rBV6	887	1246	0.28%	0.065%
12	10.010	1192	1194	1198	rBV4	667	971	0.22%	0.051%
13	10.098	1206	1209	1213	rBV4	444	635	0.14%	0.033%
14	10.363	1252	1254	1256	rBV3	633	647	0.14%	0.034%
15	10.481	1271	1274	1277	rVB5	567	639	0.14%	0.033%
16	10.651	1296	1303	1321	rBV	103126	213379	47.42%	11.170%
17	10.916	1346	1348	1349	rBV2	875	632	0.14%	0.033%
18	11.592	1460	1463	1465	rBV2	662	834	0.19%	0.044%
19	11.645	1469	1472	1474	rBV3	771	800	0.18%	0.042%
20	11.704	1480	1482	1487	rVB3	634	929	0.21%	0.049%
21	11.780	1490	1495	1498	rBV3	474	843	0.19%	0.044%
22	12.169	1557	1561	1563	rVB2	584	752	0.17%	0.039%
23	12.239	1569	1573	1574	rBV3	680	657	0.15%	0.034%
24	12.610	1634	1636	1639	rBV3	755	695	0.15%	0.036%
25	12.716	1652	1654	1657	rVB2	1054	923	0.21%	0.048%
26	12.892	1682	1684	1686	rBV2	612	673	0.15%	0.035%
27	13.351	1753	1762	1766	rVB4	1212	2367	0.53%	0.124%
28	13.380	1766	1767	1771	rBV3	742	716	0.16%	0.037%
29	13.886	1848	1853	1856	rBV4	625	1076	0.24%	0.056%
30	13.927	1858	1860	1863	rBV2	646	876	0.19%	0.046%
31	14.074	1883	1885	1888	rBV3	762	893	0.20%	0.047%
32	14.192	1902	1905	1908	rBV3	550	622	0.14%	0.033%
33	14.486	1950	1955	1965	rBV	179653	290208	64.50%	15.192%
34	14.833	2011	2014	2016	rVB	704	636	0.14%	0.033%
35	15.192	2072	2075	2079	rVB2	687	1028	0.23%	0.054%
36	15.363	2103	2104	2110	rVB3	466	656	0.15%	0.034%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
 Data File : BM042737.D
 Acq On : 14 Nov 2023 17:10
 Operator : MA/JU
 Sample : 05381-10
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SVOC-GPC2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

37	15.992	2208	2211	2213	rVB2	672	631	0.14%	0.033%
38	16.045	2217	2220	2221	rBV2	669	639	0.14%	0.033%
39	16.180	2241	2243	2248	rBV3	561	889	0.20%	0.047%
40	16.321	2261	2267	2269	rBV3	505	870	0.19%	0.046%
41	16.351	2269	2272	2274	rVB3	624	763	0.17%	0.040%
42	16.374	2274	2276	2279	rBV3	627	768	0.17%	0.040%
43	16.474	2289	2293	2294	rBV3	762	762	0.17%	0.040%
44	16.798	2345	2348	2350	rBV2	545	706	0.16%	0.037%
45	17.057	2389	2392	2393	rBV2	797	689	0.15%	0.036%
46	17.151	2404	2408	2410	rBV3	482	702	0.16%	0.037%
47	17.204	2413	2417	2418	rBV2	534	669	0.15%	0.035%
48	17.245	2418	2424	2443	rBV	178617	330583	73.47%	17.306%
49	17.398	2448	2450	2452	rVB3	1307	941	0.21%	0.049%
50	17.574	2479	2480	2482	rBV2	1069	848	0.19%	0.044%
51	17.745	2507	2509	2511	rBV2	1019	737	0.16%	0.039%
52	17.898	2531	2535	2536	rBV3	742	852	0.19%	0.045%
53	17.939	2540	2542	2543	rBV2	774	788	0.18%	0.041%
54	17.986	2545	2550	2552	rBV3	832	1284	0.29%	0.067%
55	18.045	2558	2560	2563	rBV4	662	785	0.17%	0.041%
56	18.115	2570	2572	2573	rBV	1384	662	0.15%	0.035%
57	18.251	2593	2595	2598	rBV2	1281	1004	0.22%	0.053%
58	18.327	2606	2608	2609	rBV2	858	616	0.14%	0.032%
59	18.415	2621	2623	2624	rBV2	921	618	0.14%	0.032%
60	21.427	3130	3135	3146	rBV	252713	414485	92.12%	21.698%
61	23.791	3531	3537	3547	rBV	212146	449953	100.00%	23.555%




Sum of corrected areas: 1910239

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042737.D
Acq On : 14 Nov 2023 17:10
Operator : MA/JU
Sample : 05381-10
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

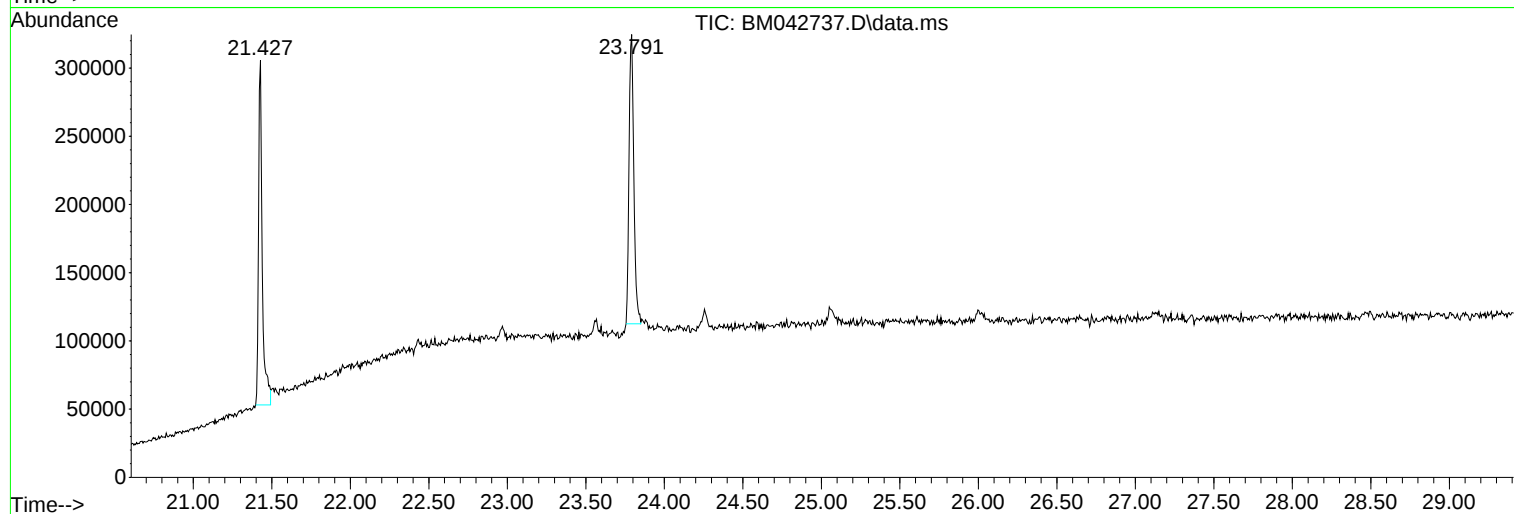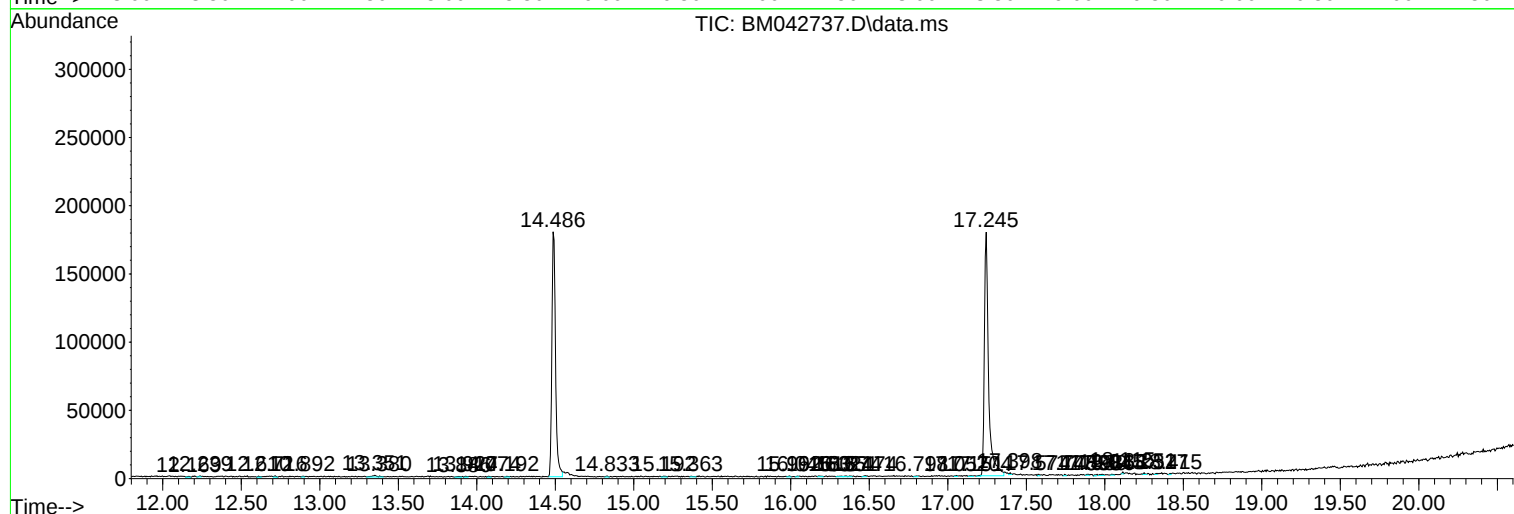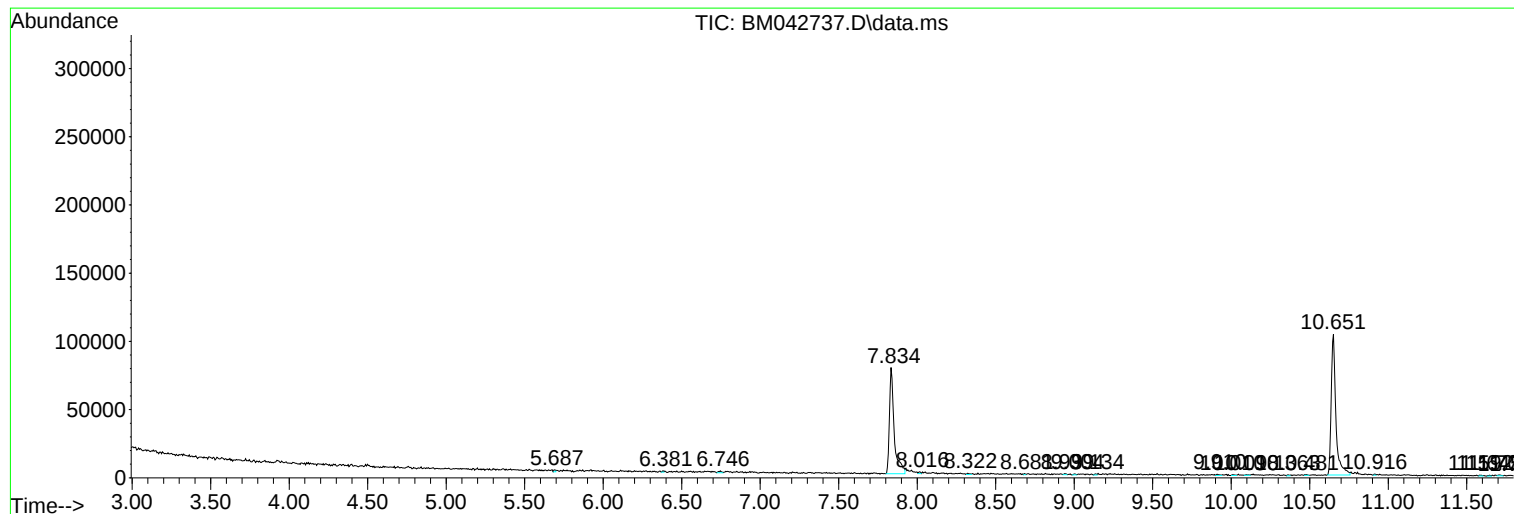

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042737.D
Acq On : 14 Nov 2023 17:10
Operator : MA/JU
Sample : 05381-10
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042737.D
Acq On : 14 Nov 2023 17:10
Operator : MA/JU
Sample : 05381-10
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc