

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
 Data File : BM042761.D
 Acq On : 15 Nov 2023 10:24
 Operator : MA/JU
 Sample : PB156719BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK719

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM042761.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.169	28	31	38	rVB2	15874	21062	1.76%	0.183%
2	3.610	102	106	121	rBV	160394	270425	22.55%	2.345%
3	4.452	246	249	250	rBV3	1564	1591	0.13%	0.014%
4	4.799	307	308	311	rBV3	1667	1532	0.13%	0.013%
5	4.887	321	323	326	rBV4	1266	1736	0.14%	0.015%
6	5.040	348	349	351	rBV2	2029	1294	0.11%	0.011%
7	5.099	357	359	363	rVV4	1564	1274	0.11%	0.011%
8	5.146	365	367	369	rBV2	1856	1237	0.10%	0.011%
9	5.634	447	450	452	rBV3	1366	1208	0.10%	0.010%
10	5.816	479	481	484	rVB4	1491	1533	0.13%	0.013%
11	5.852	486	487	491	rBV4	1180	1299	0.11%	0.011%
12	5.993	508	511	515	rBV4	1355	2018	0.17%	0.017%
13	6.122	530	533	535	rBV3	1340	1411	0.12%	0.012%
14	6.163	539	540	542	rBV2	1381	1284	0.11%	0.011%
15	6.863	657	659	664	rBV3	1096	1350	0.11%	0.012%
16	6.987	674	680	694	rBV	193039	353342	29.47%	3.064%
17	7.169	705	711	721	rBV	153557	261005	21.77%	2.263%
18	7.340	733	740	753	rBV	208821	362095	30.20%	3.140%
19	7.822	815	822	835	rBV	124334	218056	18.19%	1.891%
20	8.393	916	919	924	rBV5	1086	2087	0.17%	0.018%
21	8.545	939	945	966	rBV	201101	390801	32.59%	3.388%
22	9.022	1017	1026	1045	rBV	189421	348958	29.10%	3.026%
23	9.734	1140	1147	1159	rBV	168366	299895	25.01%	2.600%
24	10.257	1230	1236	1255	rBV	198144	399707	33.33%	3.466%
25	10.634	1292	1300	1311	rBV	170379	296074	24.69%	2.567%
26	10.810	1324	1330	1344	rBV	148023	331076	27.61%	2.871%
27	13.327	1755	1758	1764	rVB5	2951	3813	0.32%	0.033%
28	13.451	1773	1779	1782	rVB5	1083	1823	0.15%	0.016%
29	13.639	1807	1811	1813	rBV3	1062	1388	0.12%	0.012%
30	13.904	1850	1856	1869	rBV	443146	618495	51.58%	5.363%
31	14.004	1869	1873	1875	rVB4	1254	1713	0.14%	0.015%
32	14.180	1897	1903	1918	rBV	457816	683639	57.01%	5.927%
33	14.480	1948	1954	1967	rBV	264087	380595	31.74%	3.300%
34	14.745	1991	1999	2014	rBV2	52754	184881	15.42%	1.603%
35	14.963	2034	2036	2040	rVB3	1632	2080	0.17%	0.018%
36	15.263	2080	2087	2094	rVB2	3746	6917	0.58%	0.060%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
 Data File : BM042761.D
 Acq On : 15 Nov 2023 10:24
 Operator : MA/JU
 Sample : PB156719BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK719

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

37	15.474	2117	2123	2143	rBV	572260	853626	71.19%	7.401%
38	15.621	2143	2148	2161	rBV	169162	266990	22.27%	2.315%
39	15.992	2206	2211	2213	rBV3	835	1535	0.13%	0.013%
40	16.386	2275	2278	2281	rVB3	814	1227	0.10%	0.011%
41	16.510	2295	2299	2304	rBV2	2283	3728	0.31%	0.032%
42	17.239	2417	2423	2434	rBV	304020	452613	37.75%	3.924%
43	17.339	2434	2440	2457	rVV	597729	903670	75.36%	7.835%
44	17.468	2460	2462	2467	rVB4	1094	1705	0.14%	0.015%
45	17.580	2478	2481	2484	rVB	2736	2790	0.23%	0.024%
46	18.092	2563	2568	2578	rBV5	14494	31134	2.60%	0.270%
47	18.362	2610	2614	2616	rBV3	1770	2230	0.19%	0.019%
48	18.421	2620	2624	2627	rVV5	1470	2397	0.20%	0.021%
49	18.521	2639	2641	2646	rVB4	3118	3079	0.26%	0.027%
50	18.662	2663	2665	2670	rVB4	1630	1615	0.13%	0.014%
51	18.710	2670	2673	2677	rBV4	1080	1258	0.10%	0.011%
52	19.198	2752	2756	2760	rBV3	5917	7751	0.65%	0.067%
53	19.268	2765	2768	2774	rBV5	10195	13850	1.16%	0.120%
54	19.327	2774	2778	2781	rVB5	2347	2448	0.20%	0.021%
55	19.380	2783	2787	2792	rBV8	6238	12844	1.07%	0.111%
56	19.509	2805	2809	2813	rBV2	20946	21555	1.80%	0.187%
57	19.633	2824	2830	2846	rBV	924945	1177106	98.17%	10.206%
58	20.351	2949	2952	2955	rBV4	4972	4893	0.41%	0.042%
59	20.556	2984	2987	2991	rBV3	16050	18267	1.52%	0.158%
60	20.651	3000	3003	3007	rBV5	6583	9900	0.83%	0.086%
61	21.421	3130	3134	3146	rBV	343651	513667	42.84%	4.454%
62	23.633	3503	3510	3523	rBV	592962	1199073	100.00%	10.397%
63	23.786	3530	3536	3549	rVB	262041	563753	47.02%	4.888%




Sum of corrected areas: 11533398

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042761.D
Acq On : 15 Nov 2023 10:24
Operator : MA/JU
Sample : PB156719BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK719

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

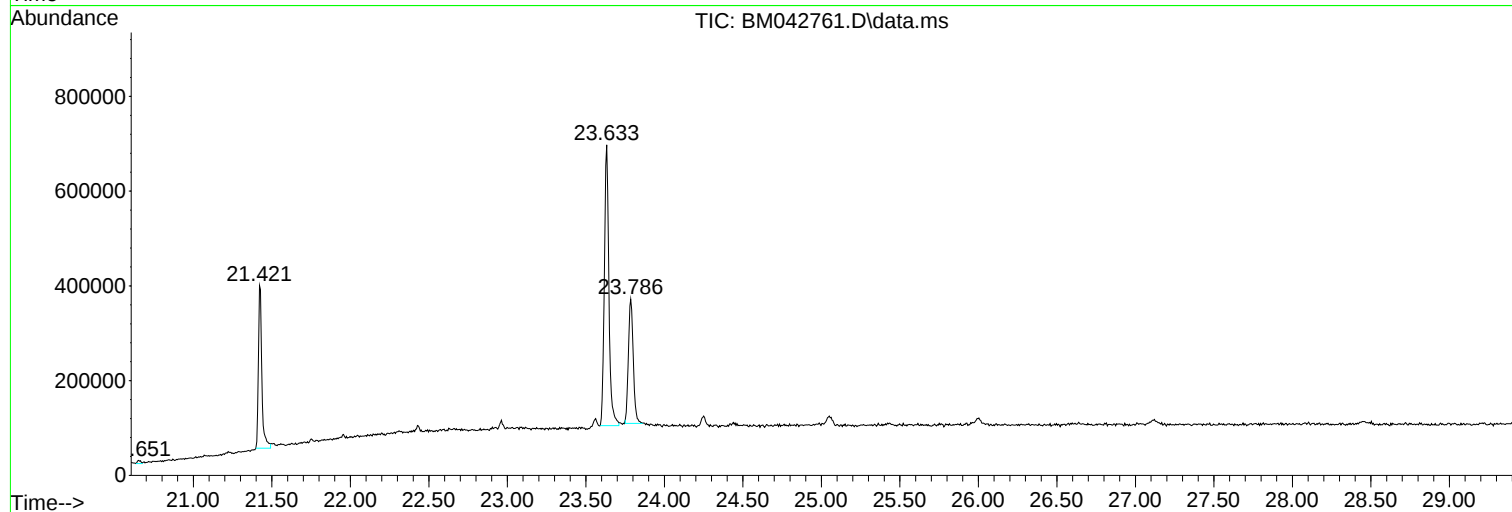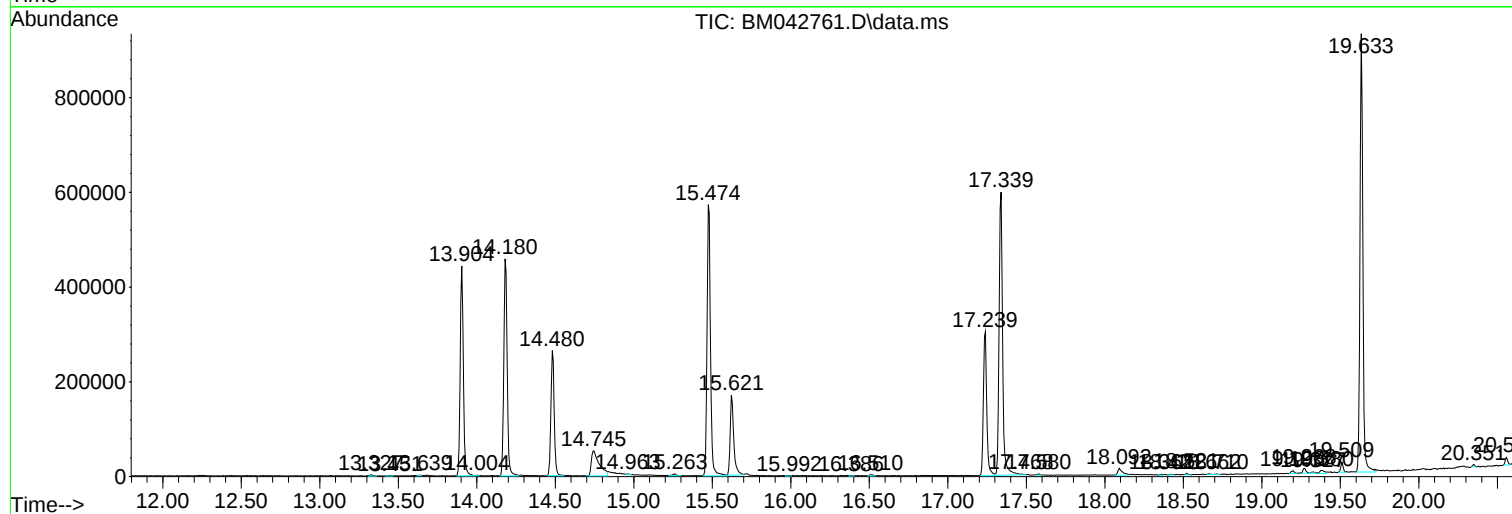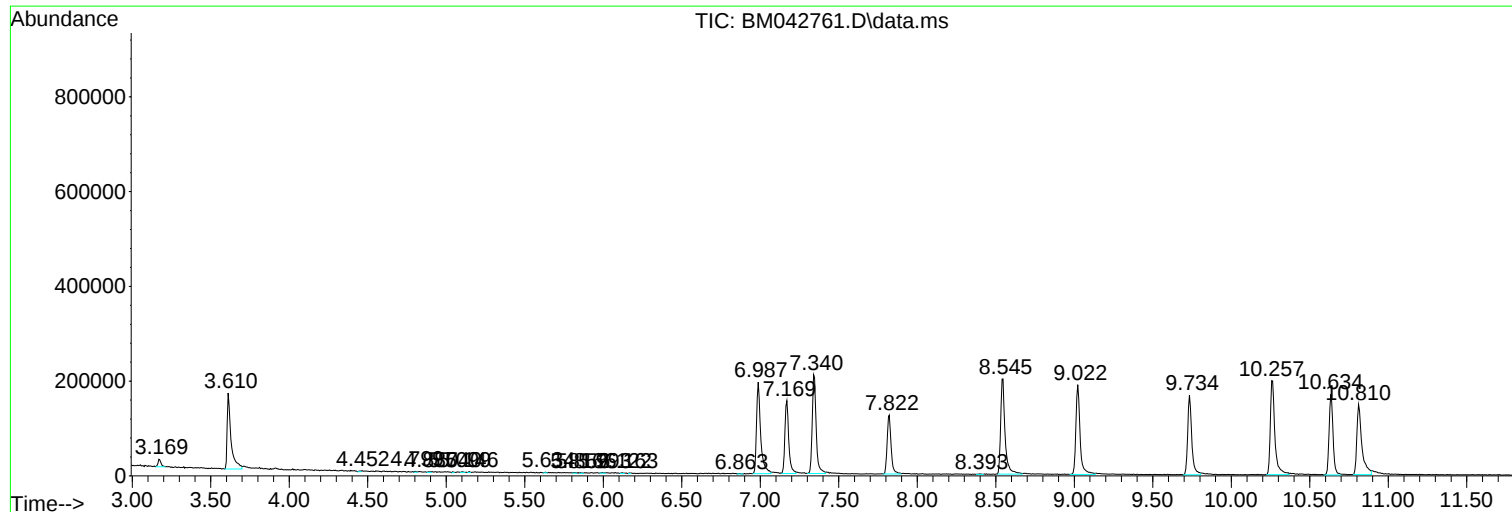

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042761.D
Acq On : 15 Nov 2023 10:24
Operator : MA/JU
Sample : PB156719BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK719

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042761.D
Acq On : 15 Nov 2023 10:24
Operator : MA/JU
Sample : PB156719BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK719

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------