

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
 Data File : BM042772.D
 Acq On : 15 Nov 2023 17:14
 Operator : MA/JU
 Sample : PB156739BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK739

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM042772.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	29	32	42	rVB2	18180	26950	2.07%	0.229%
2	3.616	103	107	126	rBV	198879	330925	25.40%	2.810%
3	4.257	214	216	219	rVB4	1745	1340	0.10%	0.011%
4	4.787	303	306	307	rBV3	1323	1385	0.11%	0.012%
5	5.381	406	407	409	rBV2	1825	1329	0.10%	0.011%
6	5.404	409	411	415	rVB4	1221	1425	0.11%	0.012%
7	6.087	526	527	531	rBV3	1352	1676	0.13%	0.014%
8	6.634	617	620	622	rBV4	1732	2070	0.16%	0.018%
9	6.775	640	644	647	rBV5	1434	2875	0.22%	0.024%
10	6.992	676	681	700	rBV	206470	400870	30.77%	3.403%
11	7.175	706	712	724	rBV	173673	286345	21.98%	2.431%
12	7.351	735	742	760	rBV	234968	408976	31.39%	3.472%
13	7.828	815	823	834	rBV	97316	174807	13.42%	1.484%
14	8.116	869	872	875	rBV3	1679	2337	0.18%	0.020%
15	8.310	902	905	908	rBV4	1011	1394	0.11%	0.012%
16	8.551	940	946	965	rBV	222462	437399	33.57%	3.714%
17	9.028	1021	1027	1045	rBV	200893	387811	29.76%	3.293%
18	9.333	1078	1079	1083	rVB3	1289	1526	0.12%	0.013%
19	9.739	1140	1148	1161	rBV	176166	336026	25.79%	2.853%
20	9.845	1164	1166	1169	rVB2	1339	1442	0.11%	0.012%
21	10.028	1194	1197	1202	rVB4	1117	1788	0.14%	0.015%
22	10.269	1231	1238	1257	rBV	214127	449390	34.49%	3.815%
23	10.410	1261	1262	1268	rVV6	2814	3293	0.25%	0.028%
24	10.639	1295	1301	1314	rBV	133412	230132	17.66%	1.954%
25	10.816	1324	1331	1351	rBV	172224	405387	31.11%	3.442%
26	10.939	1351	1352	1358	rVB4	4512	4475	0.34%	0.038%
27	11.357	1417	1423	1426	rVB4	1051	1677	0.13%	0.014%
28	11.822	1498	1502	1506	rVB3	1127	1882	0.14%	0.016%
29	12.257	1573	1576	1578	rBV4	1079	1323	0.10%	0.011%
30	12.586	1630	1632	1637	rVB3	822	1306	0.10%	0.011%
31	13.251	1741	1745	1748	rVB3	916	1605	0.12%	0.014%
32	13.333	1755	1759	1765	rBV5	4182	6963	0.53%	0.059%
33	13.698	1820	1821	1828	rBV3	954	1514	0.12%	0.013%
34	13.904	1850	1856	1870	rBV	481290	686943	52.72%	5.832%
35	14.186	1898	1904	1920	rBV	512985	757503	58.14%	6.431%
36	14.286	1920	1921	1925	rVB4	1479	1443	0.11%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
 Data File : BM042772.D
 Acq On : 15 Nov 2023 17:14
 Operator : MA/JU
 Sample : PB156739BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK739

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

37	14.486	1949	1955	1965	rBV	198332	294178	22.58%	2.498%
38	14.745	1993	1999	2011	rBV2	52602	174791	13.42%	1.484%
39	15.480	2117	2124	2142	rBV	643417	946919	72.68%	8.040%
40	15.627	2144	2149	2161	rBV	154300	258237	19.82%	2.192%
41	16.421	2280	2284	2290	rBV3	688	1463	0.11%	0.012%
42	17.239	2417	2423	2434	rBV	230218	342113	26.26%	2.905%
43	17.339	2434	2440	2462	rVB	657592	997433	76.55%	8.468%
44	17.739	2504	2508	2511	rVB3	1131	1509	0.12%	0.013%
45	17.827	2519	2523	2525	rVB4	1131	1466	0.11%	0.012%
46	18.121	2572	2573	2581	rVB6	1476	2514	0.19%	0.021%
47	18.421	2621	2624	2627	rBV4	1483	1851	0.14%	0.016%
48	19.003	2719	2723	2725	rBV4	978	1330	0.10%	0.011%
49	19.198	2750	2756	2760	rBV7	6261	10677	0.82%	0.091%
50	19.268	2764	2768	2776	rBV2	6095	9521	0.73%	0.081%
51	19.439	2795	2797	2799	rBV3	1127	1356	0.10%	0.012%
52	19.509	2807	2809	2811	rBV3	1551	1871	0.14%	0.016%
53	19.633	2824	2830	2846	rBV	976175	1260533	96.75%	10.702%
54	21.421	3129	3134	3146	rBV	242336	375964	28.86%	3.192%
55	23.627	3502	3509	3524	rBV	659836	1302915	100.00%	11.062%
56	23.780	3529	3535	3546	rVB	206933	426089	32.70%	3.618%




Sum of corrected areas: 11778262

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042772.D
Acq On : 15 Nov 2023 17:14
Operator : MA/JU
Sample : PB156739BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK739

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

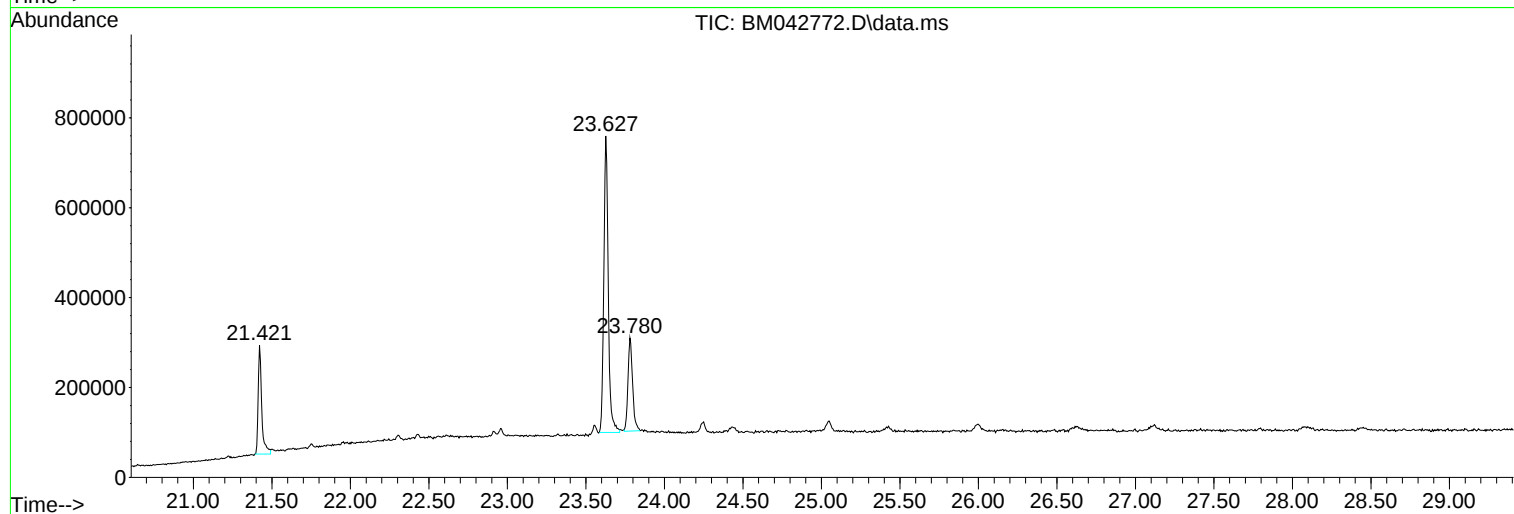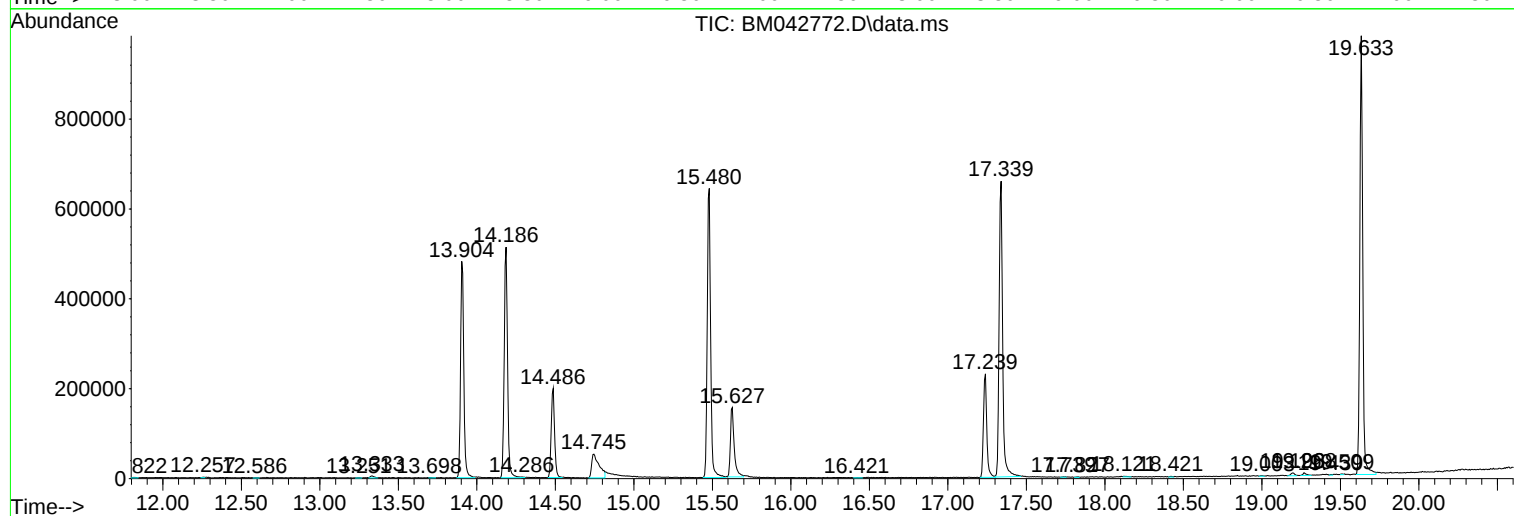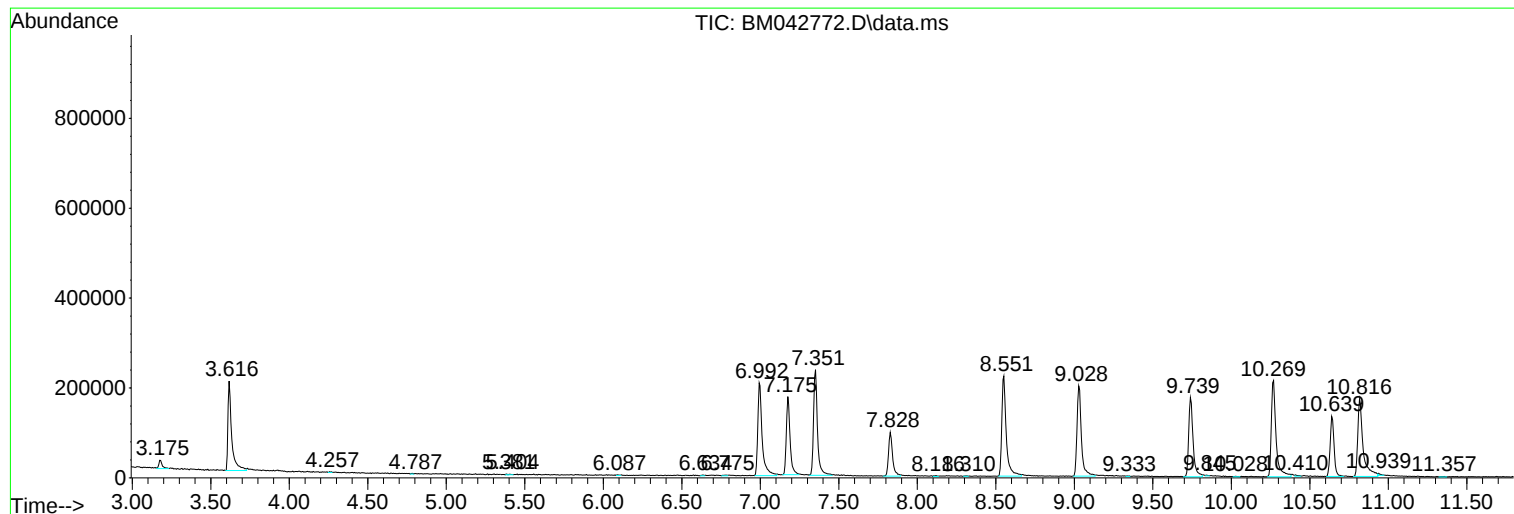

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042772.D
Acq On : 15 Nov 2023 17:14
Operator : MA/JU
Sample : PB156739BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK739

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042772.D
Acq On : 15 Nov 2023 17:14
Operator : MA/JU
Sample : PB156739BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK739

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------