

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
 Data File : BM042773.D
 Acq On : 15 Nov 2023 17:54
 Operator : MA/JU
 Sample : PB156781BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK781

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM042773.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	29	32	40	rVB	15946	19829	1.99%	0.193%
2	3.616	103	107	125	rBV	137285	242154	24.30%	2.358%
3	4.128	192	194	196	rBV3	2018	1292	0.13%	0.013%
4	4.857	316	318	321	rBV3	1349	1353	0.14%	0.013%
5	5.028	346	347	349	rBV2	1693	1005	0.10%	0.010%
6	5.257	384	386	388	rVB2	1418	1159	0.12%	0.011%
7	5.557	435	437	439	rVB3	1417	1000	0.10%	0.010%
8	5.845	484	486	489	rVB3	1638	1342	0.13%	0.013%
9	6.298	561	563	565	rBV3	1548	1364	0.14%	0.013%
10	6.351	570	572	574	rVV2	1354	1300	0.13%	0.013%
11	6.451	588	589	592	rBV2	1450	1245	0.12%	0.012%
12	6.710	632	633	637	rBV4	1169	1176	0.12%	0.011%
13	6.745	637	639	642	rBV5	961	1183	0.12%	0.012%
14	6.992	676	681	694	rBV	153945	298670	29.97%	2.908%
15	7.175	706	712	728	rVB	132235	227035	22.78%	2.211%
16	7.345	736	741	757	rBV	179608	310537	31.16%	3.024%
17	7.822	817	822	835	rBV	138909	252990	25.38%	2.464%
18	7.969	846	847	850	rBV2	1298	1013	0.10%	0.010%
19	8.051	859	861	864	rVB3	943	1015	0.10%	0.010%
20	8.210	886	888	892	rVB4	1025	1121	0.11%	0.011%
21	8.545	940	945	963	rBV	165019	328183	32.93%	3.196%
22	8.863	997	999	1003	rVB5	1337	1193	0.12%	0.012%
23	9.028	1021	1027	1046	rBV	153655	301436	30.24%	2.935%
24	9.739	1141	1148	1160	rBV	129901	252932	25.38%	2.463%
25	9.863	1167	1169	1172	rVB3	1693	1249	0.13%	0.012%
26	9.928	1177	1180	1183	rVB4	1057	1334	0.13%	0.013%
27	10.269	1231	1238	1253	rBV	150096	315947	31.70%	3.077%
28	10.510	1276	1279	1282	rBV4	1403	2015	0.20%	0.020%
29	10.639	1294	1301	1314	rBV	197241	335086	33.62%	3.263%
30	10.728	1314	1316	1321	rVB5	964	1306	0.13%	0.013%
31	10.816	1325	1331	1345	rBV	108977	268636	26.95%	2.616%
32	10.992	1360	1361	1367	rVV6	1612	2016	0.20%	0.020%
33	11.692	1479	1480	1486	rVB4	793	1025	0.10%	0.010%
34	12.851	1675	1677	1680	rBV2	1090	1032	0.10%	0.010%
35	13.221	1739	1740	1746	rBV3	627	1015	0.10%	0.010%
36	13.333	1755	1759	1762	rBV4	1637	2619	0.26%	0.026%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
 Data File : BM042773.D
 Acq On : 15 Nov 2023 17:54
 Operator : MA/JU
 Sample : PB156781BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK781

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

37	13.904	1850	1856	1868	rBV	362651	528204	53.00%	5.144%
38	13.986	1868	1870	1872	rVB3	1216	1037	0.10%	0.010%
39	14.186	1896	1904	1922	rBV	381487	576290	57.82%	5.612%
40	14.310	1922	1925	1927	rVV3	1060	1328	0.13%	0.013%
41	14.333	1927	1929	1933	rVB5	1043	1175	0.12%	0.011%
42	14.480	1947	1954	1967	rBV	289808	432835	43.43%	4.215%
43	14.751	1994	2000	2017	rBV4	31207	124973	12.54%	1.217%
44	14.963	2034	2036	2041	rVB5	1475	1875	0.19%	0.018%
45	15.321	2095	2097	2102	rVB4	881	999	0.10%	0.010%
46	15.480	2118	2124	2134	rBV	465309	703237	70.56%	6.848%
47	15.627	2144	2149	2164	rBV	118809	208167	20.89%	2.027%
48	16.110	2228	2231	2236	rVB5	706	1376	0.14%	0.013%
49	17.239	2416	2423	2434	rBV	340111	508129	50.98%	4.948%
50	17.339	2434	2440	2459	rVV	458065	736384	73.89%	7.171%
51	17.804	2516	2519	2520	rBV3	1287	1510	0.15%	0.015%
52	18.109	2568	2571	2573	rBV3	2150	2814	0.28%	0.027%
53	18.386	2616	2618	2620	rBV2	1584	1806	0.18%	0.018%
54	18.433	2623	2626	2627	rBV3	1647	1600	0.16%	0.016%
55	18.727	2675	2676	2680	rBV3	960	1180	0.12%	0.011%
56	18.945	2709	2713	2716	rBV4	816	1151	0.12%	0.011%
57	19.198	2753	2756	2759	rBV3	3972	5593	0.56%	0.054%
58	19.268	2765	2768	2774	rBV4	7162	9165	0.92%	0.089%
59	19.509	2805	2809	2815	rBV2	14436	19054	1.91%	0.186%
60	19.574	2818	2820	2823	rBV4	1414	1476	0.15%	0.014%
61	19.633	2824	2830	2843	rBV	735381	955495	95.87%	9.305%
62	20.556	2984	2987	2992	rBV2	12698	12294	1.23%	0.120%
63	21.421	3129	3134	3145	rBV	389374	573035	57.50%	5.580%
64	23.556	3494	3497	3502	rVB4	30188	44873	4.50%	0.437%
65	23.633	3503	3510	3522	rVV	495087	996656	100.00%	9.706%
66	23.786	3530	3536	3547	rVB	323958	630457	63.26%	6.139%




Sum of corrected areas: 10268975

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042773.D
Acq On : 15 Nov 2023 17:54
Operator : MA/JU
Sample : PB156781BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK781

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

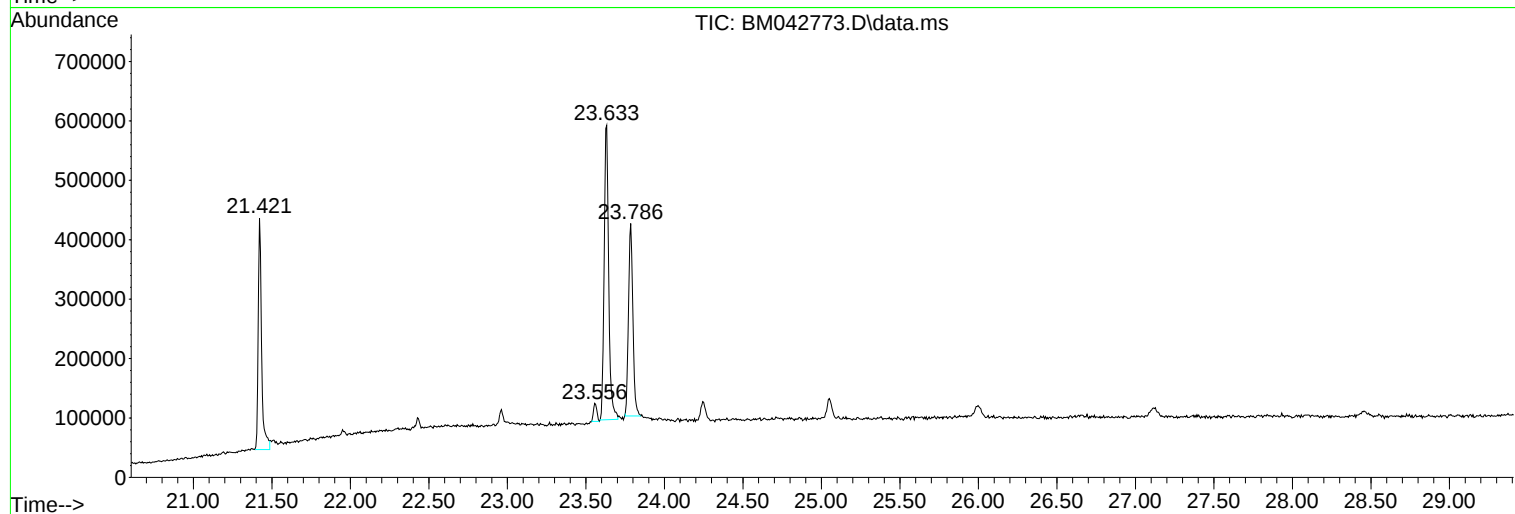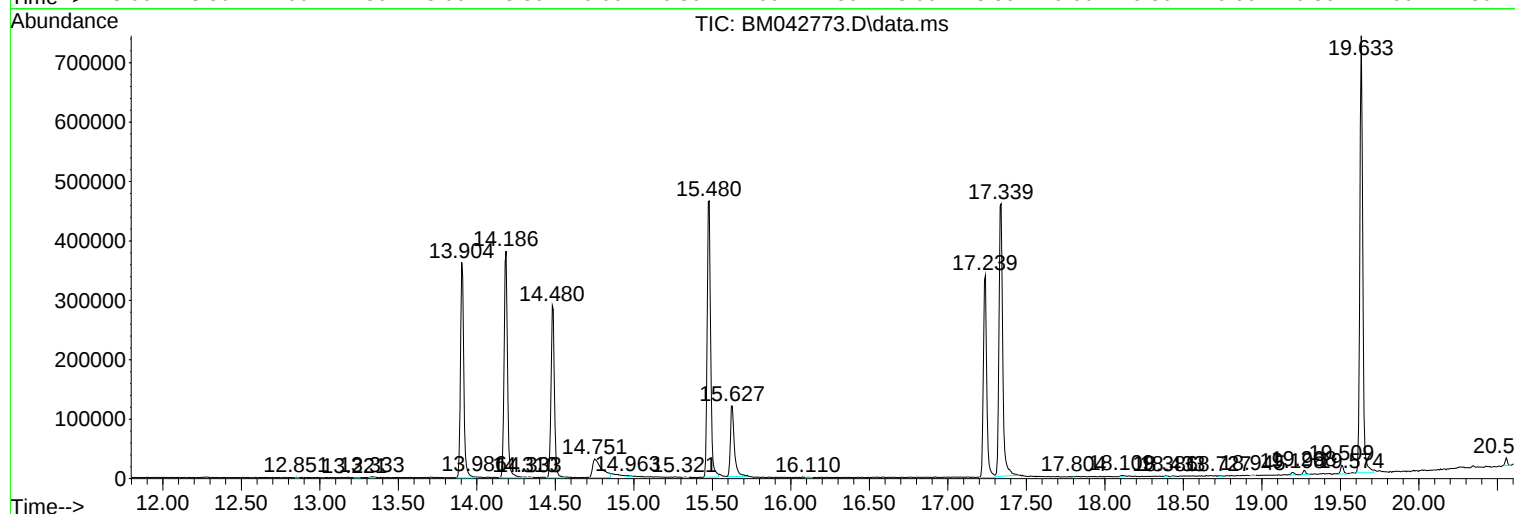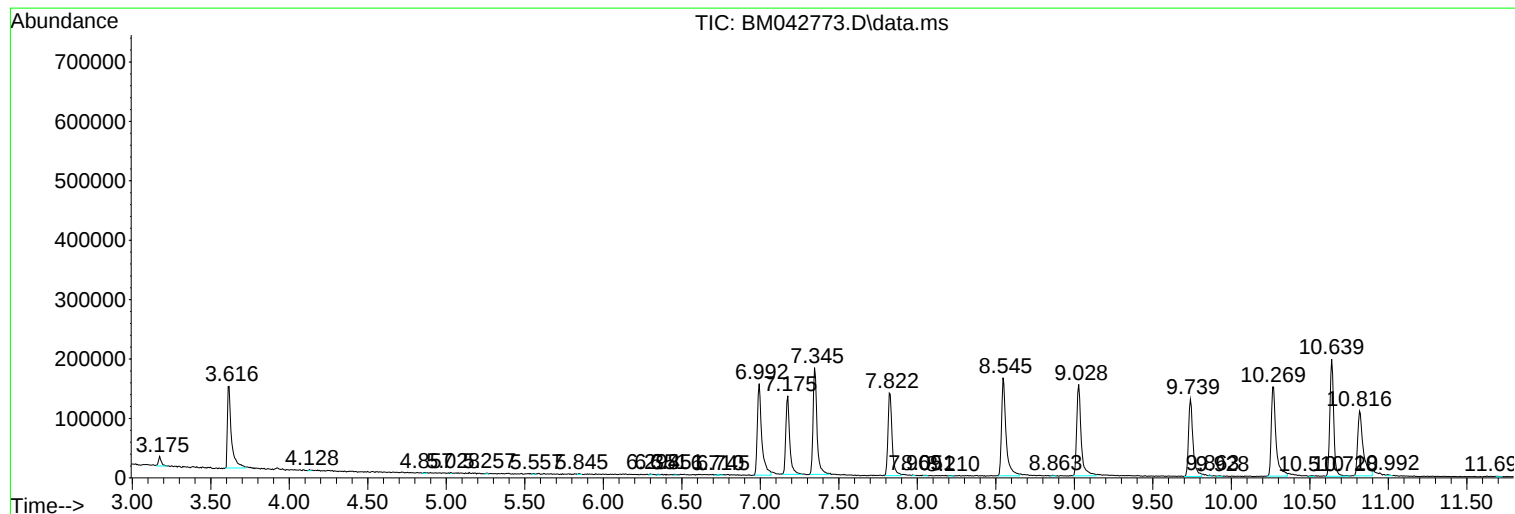

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042773.D
Acq On : 15 Nov 2023 17:54
Operator : MA/JU
Sample : PB156781BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK781

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042773.D
Acq On : 15 Nov 2023 17:54
Operator : MA/JU
Sample : PB156781BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK781

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc