

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
 Data File : BM042782.D
 Acq On : 15 Nov 2023 23:18
 Operator : MA/JU
 Sample : 05105-02
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0006

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM042782.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	29	32	41	rVB4	8602	12881	1.02%	0.130%
2	3.628	105	109	123	rBV	28356	59721	4.72%	0.604%
3	3.916	156	158	164	rVB4	2368	3309	0.26%	0.033%
4	4.681	286	288	290	rBV2	1433	1360	0.11%	0.014%
5	6.016	513	515	519	rBV4	1075	1478	0.12%	0.015%
6	6.181	540	543	546	rBV4	1227	1826	0.14%	0.018%
7	6.269	556	558	563	rBV6	1155	1556	0.12%	0.016%
8	6.716	632	634	638	rVB5	971	1276	0.10%	0.013%
9	7.004	678	683	696	rBV2	19545	49888	3.94%	0.504%
10	7.175	706	712	727	rVV	112304	203332	16.06%	2.055%
11	7.269	727	728	735	rVB6	2260	2207	0.17%	0.022%
12	7.351	735	742	759	rBV2	113635	218145	17.23%	2.205%
13	7.828	816	823	834	rBV	127364	225506	17.81%	2.280%
14	8.551	940	946	960	rBV	62703	137936	10.90%	1.394%
15	8.692	969	970	975	rVB4	1189	1439	0.11%	0.015%
16	8.840	991	995	998	rVB4	825	1500	0.12%	0.015%
17	9.028	1021	1027	1040	rBV	137838	268739	21.23%	2.717%
18	9.739	1142	1148	1162	rBV	115593	226668	17.91%	2.291%
19	10.269	1231	1238	1257	rBV	130490	286876	22.66%	2.900%
20	10.639	1295	1301	1311	rBV	177397	303956	24.01%	3.073%
21	10.704	1311	1312	1316	rVB3	1433	1481	0.12%	0.015%
22	10.822	1325	1332	1345	rBV2	73755	191548	15.13%	1.936%
23	13.333	1752	1759	1767	rBV3	4129	7942	0.63%	0.080%
24	13.710	1820	1823	1826	rVB4	1175	1411	0.11%	0.014%
25	13.904	1850	1856	1870	rBV	394927	565823	44.70%	5.720%
26	14.180	1897	1903	1917	rBV	372297	559632	44.21%	5.657%
27	14.480	1945	1954	1963	rBV	270952	398065	31.45%	4.024%
28	14.780	2001	2005	2013	rBV6	2698	8040	0.64%	0.081%
29	15.216	2076	2079	2083	rVB2	1293	1577	0.12%	0.016%
30	15.474	2117	2123	2137	rBV	501694	744036	58.78%	7.521%
31	15.569	2137	2139	2141	rVV3	3562	3744	0.30%	0.038%
32	15.621	2143	2148	2162	rVV	165752	278781	22.02%	2.818%
33	15.716	2162	2164	2169	rVB4	3491	4596	0.36%	0.046%
34	15.863	2185	2189	2192	rVB5	1978	2803	0.22%	0.028%
35	16.204	2243	2247	2248	rVB2	1445	1705	0.13%	0.017%
36	16.898	2360	2365	2368	rBV3	1534	2100	0.17%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
 Data File : BM042782.D
 Acq On : 15 Nov 2023 23:18
 Operator : MA/JU
 Sample : 05105-02
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0006

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

37	17.233	2417	2422	2433	rBV	300801	460324	36.37%	4.653%
38	17.333	2434	2439	2457	rVV	598614	878757	69.42%	8.883%
39	17.486	2463	2465	2470	rVB5	1837	2719	0.21%	0.027%
40	17.574	2475	2480	2482	rBV5	1288	2413	0.19%	0.024%
41	17.862	2525	2529	2534	rBV6	2180	4115	0.33%	0.042%
42	18.092	2564	2568	2576	rBV4	11310	19630	1.55%	0.198%
43	18.174	2581	2582	2587	rBV5	1929	2671	0.21%	0.027%
44	18.357	2611	2613	2618	rVB4	1395	1601	0.13%	0.016%
45	18.498	2634	2637	2638	rBV3	1185	1430	0.11%	0.014%
46	18.662	2661	2665	2667	rBV4	1876	2418	0.19%	0.024%
47	18.809	2688	2690	2693	rBV4	1628	2062	0.16%	0.021%
48	18.957	2710	2715	2717	rBV5	1853	2983	0.24%	0.030%
49	19.068	2732	2734	2739	rBV5	978	1572	0.12%	0.016%
50	19.192	2749	2755	2759	rBV6	6116	10658	0.84%	0.108%
51	19.268	2765	2768	2771	rBV2	6632	6703	0.53%	0.068%
52	19.374	2783	2786	2790	rBV5	4440	6655	0.53%	0.067%
53	19.509	2806	2809	2814	rVB6	4027	5382	0.43%	0.054%
54	19.562	2816	2818	2821	rBV4	1512	2088	0.16%	0.021%
55	19.633	2824	2830	2845	rBV	961106	1228297	97.03%	12.417%
56	19.880	2870	2872	2873	rBV2	2577	2014	0.16%	0.020%
57	21.086	3073	3077	3082	rBV7	15528	29739	2.35%	0.301%
58	21.415	3129	3133	3145	rBV	362328	544032	42.98%	5.500%
59	23.627	3502	3509	3520	rBV2	645898	1265842	100.00%	12.796%
60	23.780	3529	3535	3550	rVB	304221	625398	49.41%	6.322%




Sum of corrected areas: 9892386

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042782.D
Acq On : 15 Nov 2023 23:18
Operator : MA/JU
Sample : 05105-02
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0006

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

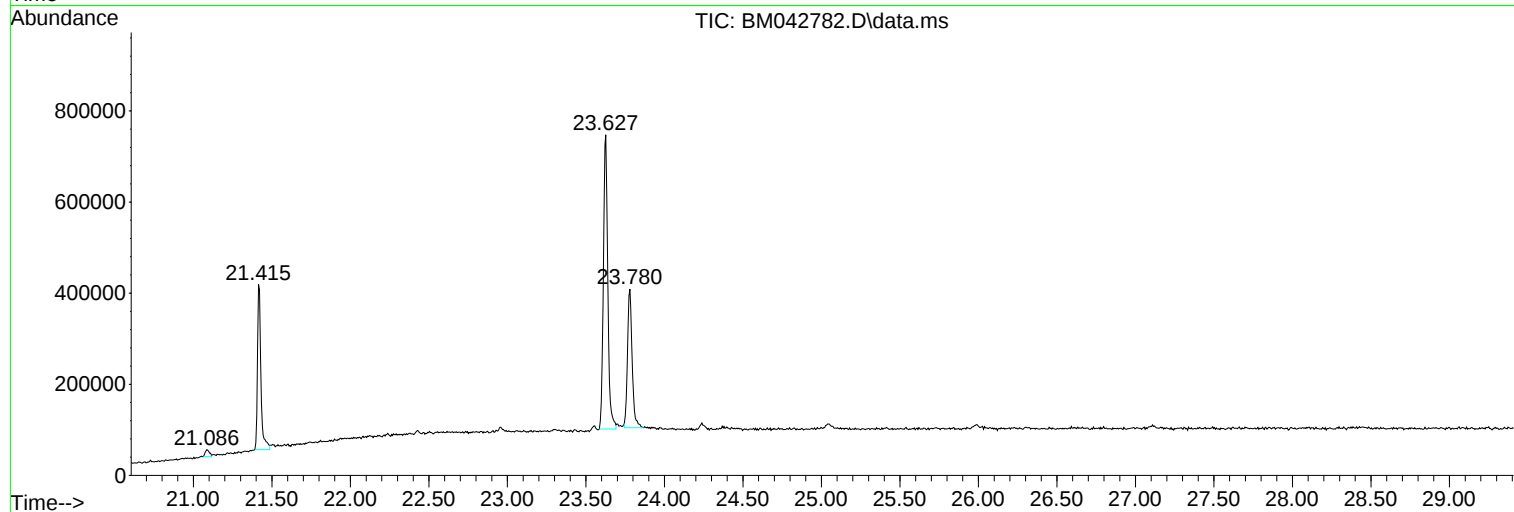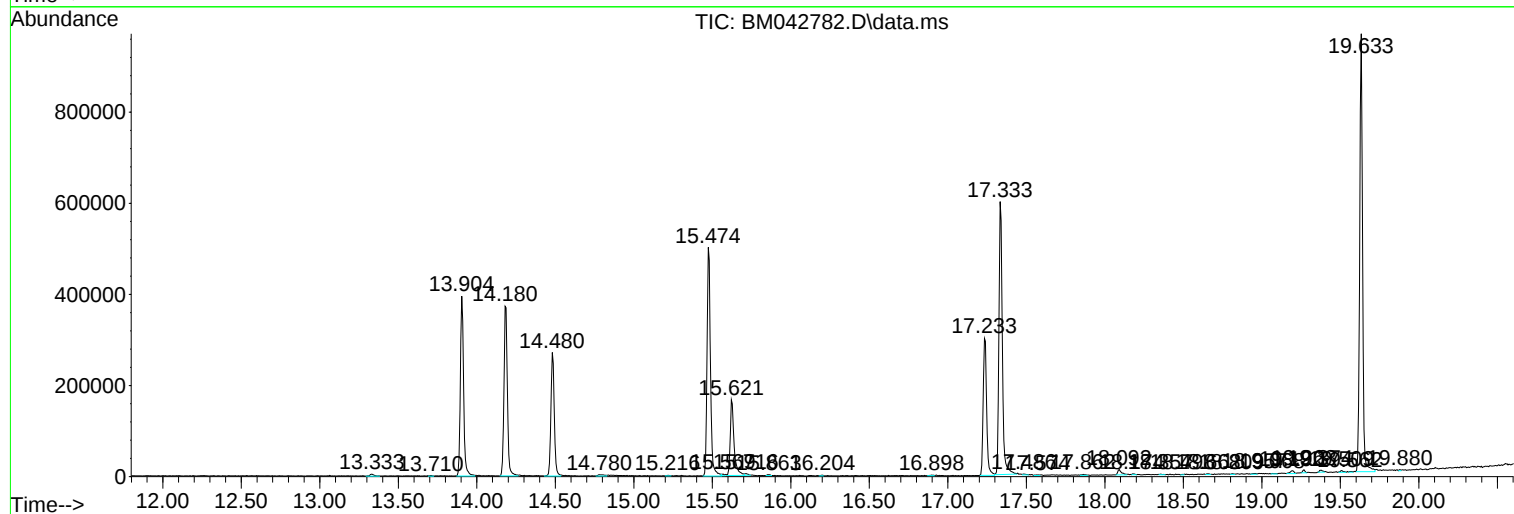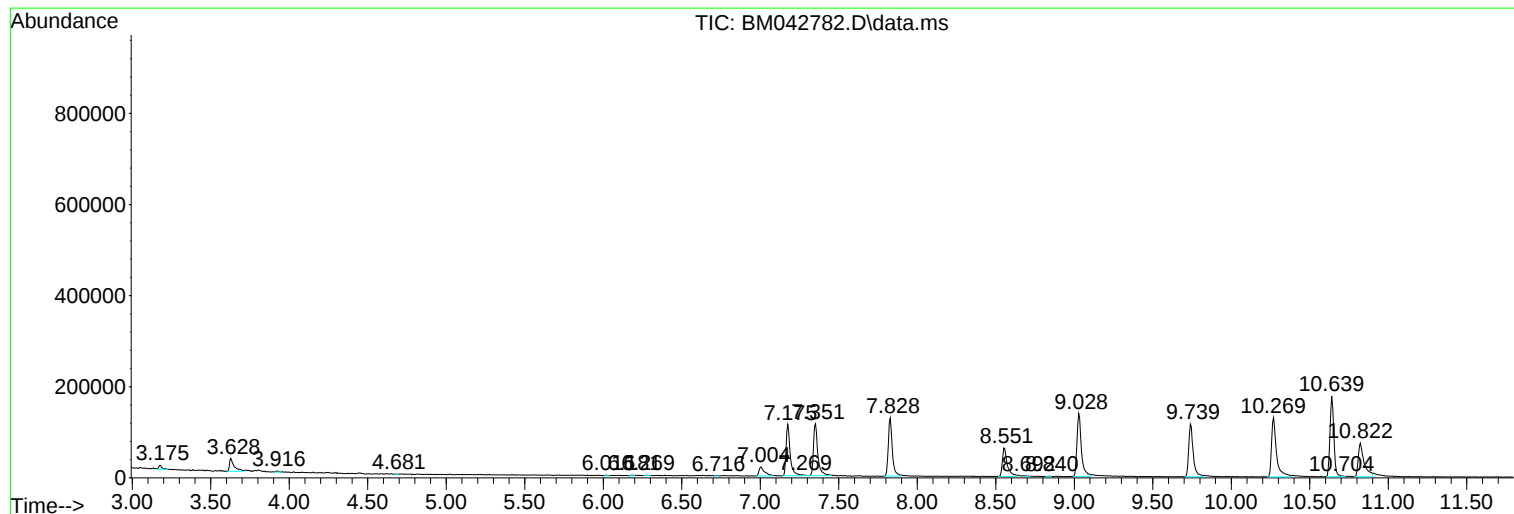

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042782.D
Acq On : 15 Nov 2023 23:18
Operator : MA/JU
Sample : 05105-02
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0006

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042782.D
Acq On : 15 Nov 2023 23:18
Operator : MA/JU
Sample : 05105-02
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0006

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc