

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
 Data File : BM042783.D
 Acq On : 15 Nov 2023 23:54
 Operator : MA/JU
 Sample : 05105-03
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0007

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM042783.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	29	32	37	rVB2	7220	7999	0.75%	0.088%
2	3.634	106	110	122	rBV2	16356	34710	3.24%	0.383%
3	4.046	178	180	182	rBV3	1664	1541	0.14%	0.017%
4	6.316	563	566	568	rBV3	1104	1348	0.13%	0.015%
5	6.393	575	579	581	rBV4	816	1223	0.11%	0.013%
6	7.004	677	683	696	rVV3	18680	49148	4.58%	0.542%
7	7.175	707	712	728	rBV	105131	194545	18.13%	2.146%
8	7.351	736	742	753	rBV	105601	199196	18.57%	2.198%
9	7.828	816	823	840	rBV	124534	229604	21.40%	2.533%
10	8.551	941	946	960	rBV	55181	122587	11.43%	1.352%
11	9.028	1021	1027	1042	rBV	130434	253079	23.59%	2.792%
12	9.739	1140	1148	1163	rBV2	108540	213194	19.87%	2.352%
13	9.857	1166	1168	1177	rVB6	1533	3147	0.29%	0.035%
14	10.269	1231	1238	1257	rBV	113226	256708	23.93%	2.832%
15	10.386	1257	1258	1267	rVB6	2814	4188	0.39%	0.046%
16	10.639	1294	1301	1314	rBV	174335	301984	28.15%	3.331%
17	10.822	1326	1332	1354	rBV2	42661	132006	12.30%	1.456%
18	10.998	1359	1362	1363	rVB3	1235	1198	0.11%	0.013%
19	11.333	1417	1419	1423	rVB3	918	1131	0.11%	0.012%
20	11.380	1423	1427	1430	rBV2	771	1400	0.13%	0.015%
21	11.463	1434	1441	1442	rVB5	745	1274	0.12%	0.014%
22	11.698	1479	1481	1487	rVB2	1570	2453	0.23%	0.027%
23	12.327	1586	1588	1591	rBV4	1737	1903	0.18%	0.021%
24	12.798	1661	1668	1674	rBV5	1319	2994	0.28%	0.033%
25	13.057	1706	1712	1716	rBV3	1577	1816	0.17%	0.020%
26	13.333	1751	1759	1765	rBV	12732	20776	1.94%	0.229%
27	13.439	1774	1777	1782	rVB2	874	1293	0.12%	0.014%
28	13.710	1821	1823	1828	rVB4	1280	1559	0.15%	0.017%
29	13.904	1850	1856	1871	rBV	371917	518103	48.29%	5.716%
30	14.051	1878	1881	1883	rBV3	902	1099	0.10%	0.012%
31	14.180	1897	1903	1922	rBV	337976	526064	49.04%	5.803%
32	14.480	1947	1954	1965	rBV	272232	395546	36.87%	4.364%
33	14.604	1972	1975	1980	rVB4	881	1531	0.14%	0.017%
34	14.792	2001	2007	2008	rBV3	2502	3675	0.34%	0.041%
35	14.921	2028	2029	2034	rVB4	1127	1157	0.11%	0.013%
36	15.474	2117	2123	2137	rBV	463110	684934	63.85%	7.556%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
 Data File : BM042783.D
 Acq On : 15 Nov 2023 23:54
 Operator : MA/JU
 Sample : 05105-03
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0007

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

37	15.621	2143	2148	2162	rBV	140352	238806	22.26%	2.634%
38	15.715	2162	2164	2171	rVB5	2579	3487	0.33%	0.038%
39	15.851	2185	2187	2190	rBV3	977	1420	0.13%	0.016%
40	16.127	2231	2234	2236	rBV2	1072	1557	0.15%	0.017%
41	16.198	2243	2246	2250	rVB4	1054	1200	0.11%	0.013%
42	16.762	2337	2342	2344	rBV3	1888	2114	0.20%	0.023%
43	16.827	2350	2353	2357	rVB3	735	1213	0.11%	0.013%
44	16.904	2360	2366	2367	rBV3	1036	1687	0.16%	0.019%
45	16.968	2374	2377	2379	rBV4	1233	1424	0.13%	0.016%
46	17.233	2417	2422	2433	rBV	323262	473373	44.13%	5.222%
47	17.333	2433	2439	2456	rVV	499709	766123	71.41%	8.452%
48	17.492	2464	2466	2471	rVB5	2105	2500	0.23%	0.028%
49	17.839	2523	2525	2526	rBV2	1244	1110	0.10%	0.012%
50	17.851	2526	2527	2530	rVV3	2274	2687	0.25%	0.030%
51	17.998	2551	2552	2555	rVB2	1737	1216	0.11%	0.013%
52	18.092	2563	2568	2577	rBV4	16451	30926	2.88%	0.341%
53	18.156	2577	2579	2580	rVV2	1805	1259	0.12%	0.014%
54	18.180	2580	2583	2588	rVB5	2367	4187	0.39%	0.046%
55	18.274	2596	2599	2600	rBV2	1252	1102	0.10%	0.012%
56	18.651	2659	2663	2664	rBV3	2508	2610	0.24%	0.029%
57	18.821	2690	2692	2695	rBV2	1081	1306	0.12%	0.014%
58	19.003	2718	2723	2725	rBV5	1605	2467	0.23%	0.027%
59	19.192	2752	2755	2759	rVB4	4380	5859	0.55%	0.065%
60	19.262	2764	2767	2771	rBV4	5802	8454	0.79%	0.093%
61	19.321	2773	2777	2779	rBV3	1837	3345	0.31%	0.037%
62	19.380	2783	2787	2791	rBV6	6059	9864	0.92%	0.109%
63	19.503	2806	2808	2813	rBV5	3095	4024	0.38%	0.044%
64	19.633	2824	2830	2844	rBV	795308	1049748	97.85%	11.581%
65	21.086	3073	3077	3083	rBV6	12660	22262	2.08%	0.246%
66	21.421	3128	3134	3144	rBV	352530	538803	50.22%	5.944%
67	23.621	3502	3508	3523	rBV2	529483	1072789	100.00%	11.835%
68	23.780	3528	3535	3551	rVB	303805	629597	58.69%	6.946%




Sum of corrected areas: 9064632

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042783.D
Acq On : 15 Nov 2023 23:54
Operator : MA/JU
Sample : 05105-03
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0007

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

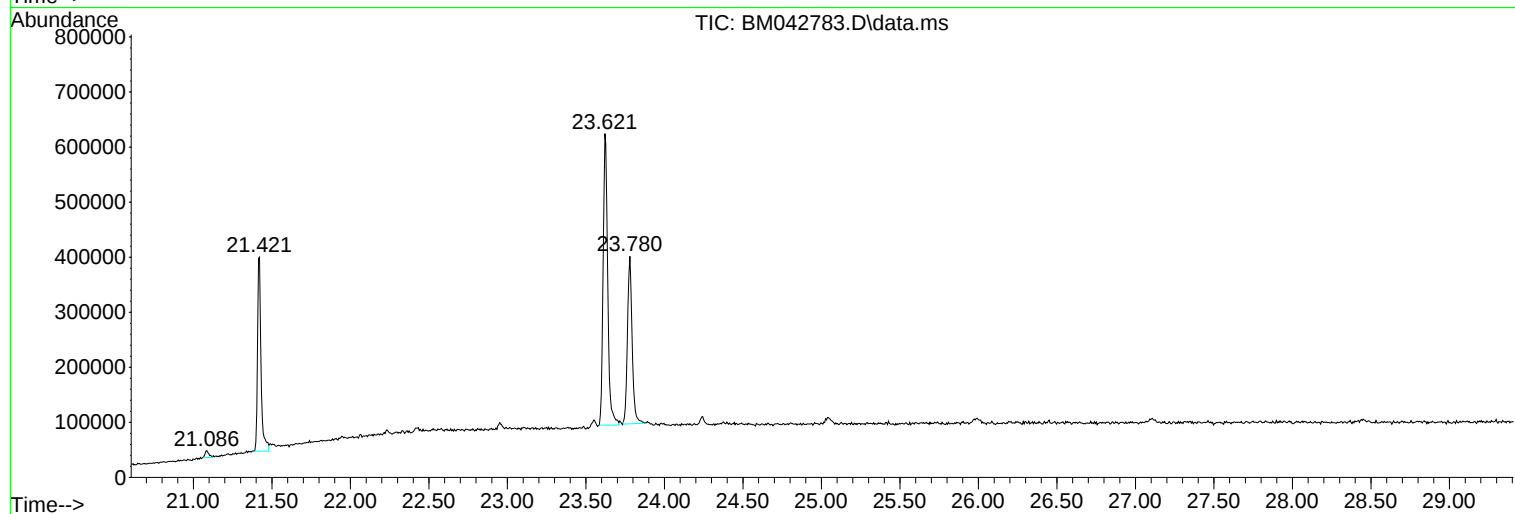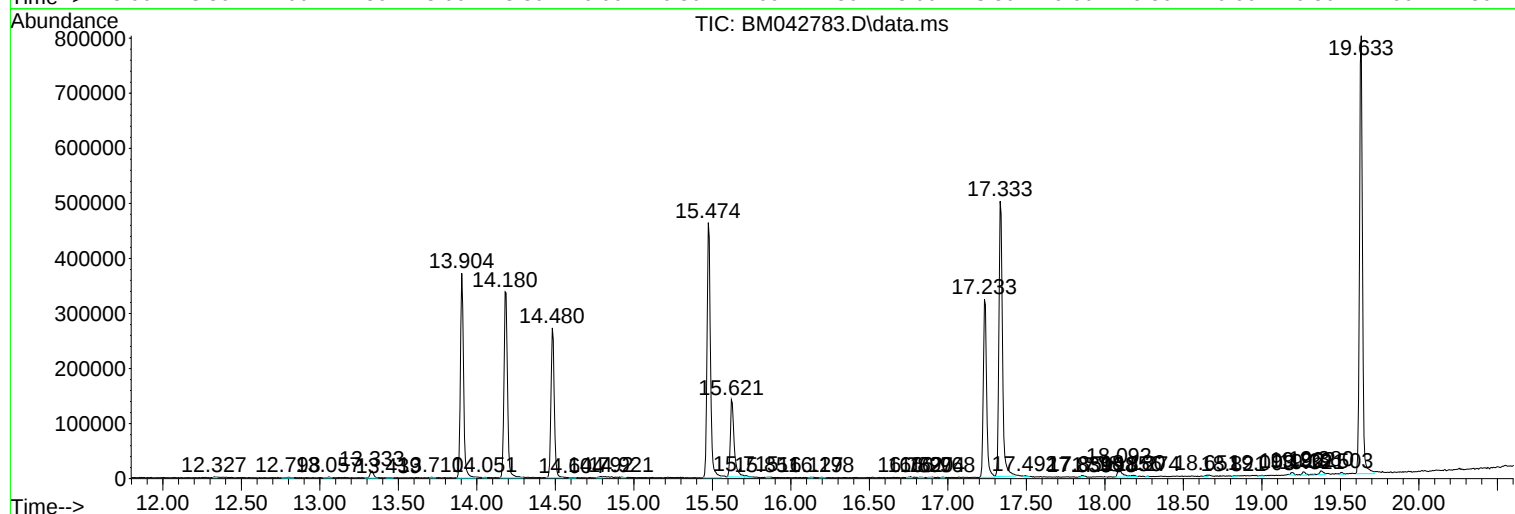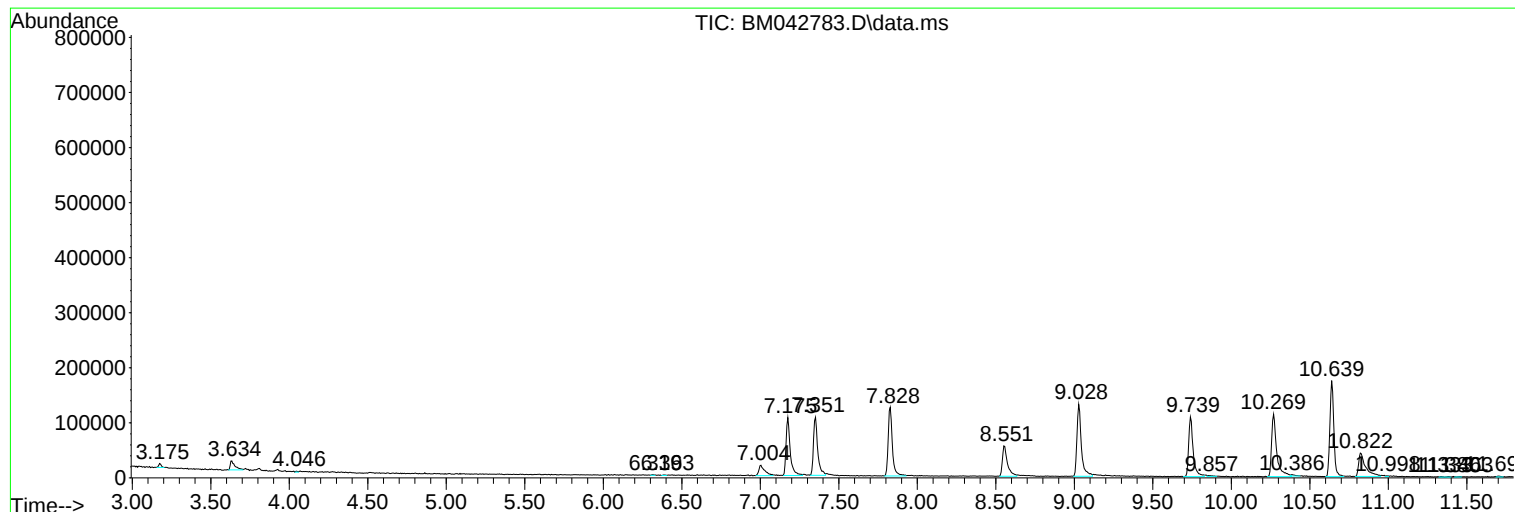

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042783.D
Acq On : 15 Nov 2023 23:54
Operator : MA/JU
Sample : 05105-03
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0007

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042783.D
Acq On : 15 Nov 2023 23:54
Operator : MA/JU
Sample : 05105-03
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0007

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------