

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
 Data File : BM042790.D
 Acq On : 16 Nov 2023 04:43
 Operator : MA/JU
 Sample : PB156744BL
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK744

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM042790.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	29	32	38	rVB2	15466	21769	2.02%	0.234%
2	3.616	103	107	128	rBV	133080	242811	22.54%	2.606%
3	5.110	359	361	363	rVB3	1560	1223	0.11%	0.013%
4	5.216	377	379	381	rBV3	1211	1321	0.12%	0.014%
5	5.722	462	465	466	rBV3	1212	1236	0.11%	0.013%
6	6.763	639	642	645	rVB4	953	1402	0.13%	0.015%
7	6.993	675	681	699	rBV	139420	281641	26.14%	3.023%
8	7.175	706	712	729	rVB	118334	208625	19.36%	2.240%
9	7.346	735	741	757	rBV	156666	287020	26.64%	3.081%
10	7.516	768	770	774	rVB5	1352	1732	0.16%	0.019%
11	7.828	816	823	834	rBV	93777	178678	16.58%	1.918%
12	7.969	846	847	852	rVB3	1265	1145	0.11%	0.012%
13	8.545	940	945	964	rBV	147893	302931	28.12%	3.252%
14	8.704	970	972	977	rVB4	1460	1790	0.17%	0.019%
15	9.028	1020	1027	1042	rBV	144370	275646	25.58%	2.959%
16	9.334	1076	1079	1082	rBV4	909	1103	0.10%	0.012%
17	9.528	1110	1112	1115	rBV3	898	1104	0.10%	0.012%
18	9.739	1142	1148	1163	rBV2	120012	238554	22.14%	2.561%
19	9.857	1166	1168	1173	rVB6	1810	1781	0.17%	0.019%
20	9.940	1179	1182	1185	rVB4	1114	1315	0.12%	0.014%
21	10.028	1196	1197	1201	rVB4	1107	1179	0.11%	0.013%
22	10.269	1229	1238	1252	rBV	143495	295820	27.46%	3.176%
23	10.639	1291	1301	1311	rBV	134132	238325	22.12%	2.558%
24	10.722	1313	1315	1319	rVB4	1048	1338	0.12%	0.014%
25	10.816	1325	1331	1349	rBV	107020	272340	25.28%	2.923%
26	12.269	1574	1578	1584	rVB4	1135	1905	0.18%	0.020%
27	12.675	1645	1647	1653	rVB4	753	1240	0.12%	0.013%
28	13.333	1752	1759	1764	rVB5	2567	4398	0.41%	0.047%
29	13.904	1850	1856	1868	rBV	348619	504081	46.78%	5.411%
30	14.180	1897	1903	1920	rBV	361903	544516	50.54%	5.845%
31	14.480	1948	1954	1968	rBV	207107	300579	27.90%	3.227%
32	14.751	1993	2000	2014	rBV3	29860	113839	10.57%	1.222%
33	15.004	2040	2043	2047	rVB2	1574	1853	0.17%	0.020%
34	15.474	2117	2123	2140	rBV	462530	688069	63.86%	7.386%
35	15.621	2143	2148	2161	rBV	117262	205836	19.10%	2.210%
36	15.733	2166	2167	2171	rVV4	3326	3233	0.30%	0.035%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
 Data File : BM042790.D
 Acq On : 16 Nov 2023 04:43
 Operator : MA/JU
 Sample : PB156744BL
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK744

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

37	16.016	2212	2215	2221	rVB4	972	1469	0.14%	0.016%
38	17.233	2417	2422	2434	rVV	247265	362861	33.68%	3.895%
39	17.333	2434	2439	2456	rVV	471217	730862	67.83%	7.846%
40	18.121	2571	2573	2577	rBV3	1096	1234	0.11%	0.013%
41	18.592	2652	2653	2656	rVB2	1581	1164	0.11%	0.012%
42	18.615	2656	2657	2661	rBV3	1594	2021	0.19%	0.022%
43	18.815	2687	2691	2694	rVV5	812	1162	0.11%	0.012%
44	19.192	2752	2755	2759	rBV5	3853	5814	0.54%	0.062%
45	19.268	2764	2768	2771	rBV5	4184	5778	0.54%	0.062%
46	19.339	2779	2780	2783	rVB3	1494	1185	0.11%	0.013%
47	19.439	2795	2797	2799	rBV2	1043	1190	0.11%	0.013%
48	19.568	2814	2819	2821	rBV5	1583	2777	0.26%	0.030%
49	19.633	2824	2830	2848	rVV	697583	963075	89.39%	10.338%
50	21.415	3129	3133	3147	rBV	270163	444673	41.27%	4.773%
51	23.627	3502	3509	3523	rBV	527651	1077442	100.00%	11.566%
52	23.780	3529	3535	3542	rBV	238777	481585	44.70%	5.170%




Sum of corrected areas: 9315670

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042790.D
Acq On : 16 Nov 2023 04:43
Operator : MA/JU
Sample : PB156744BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK744

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

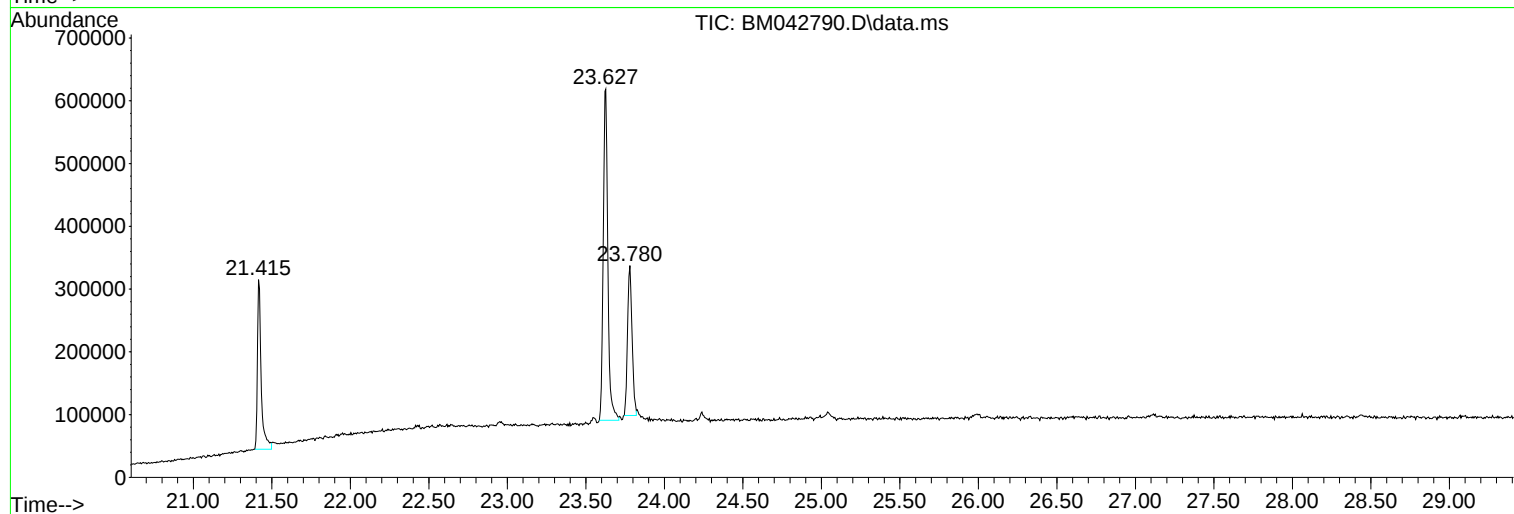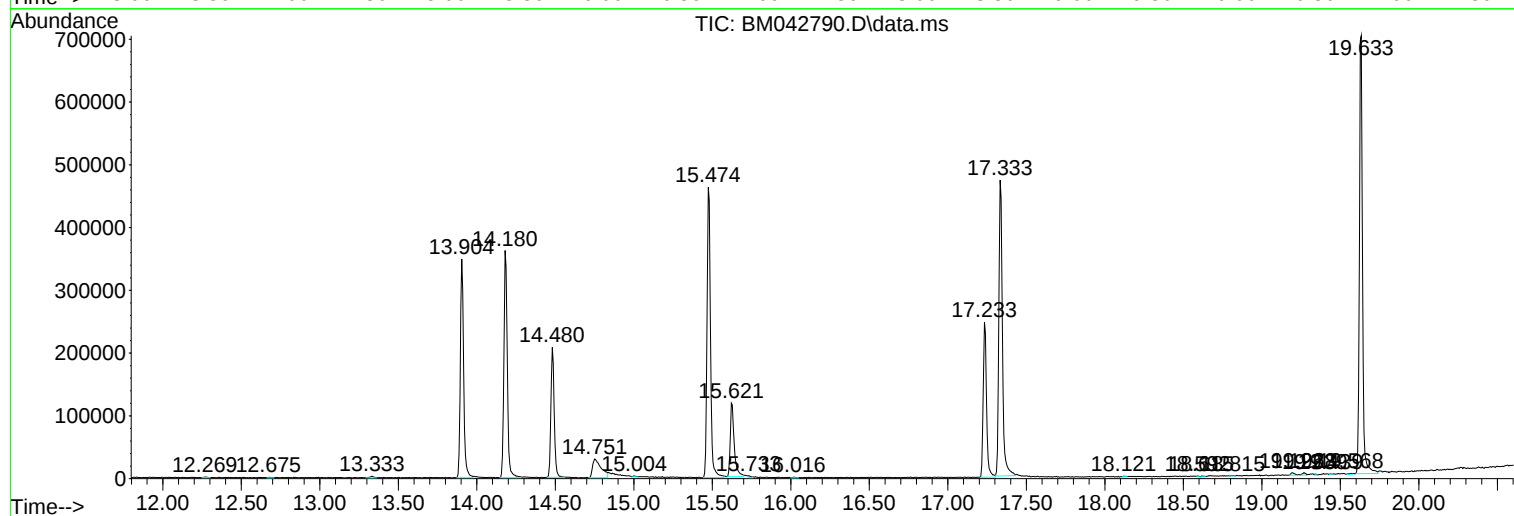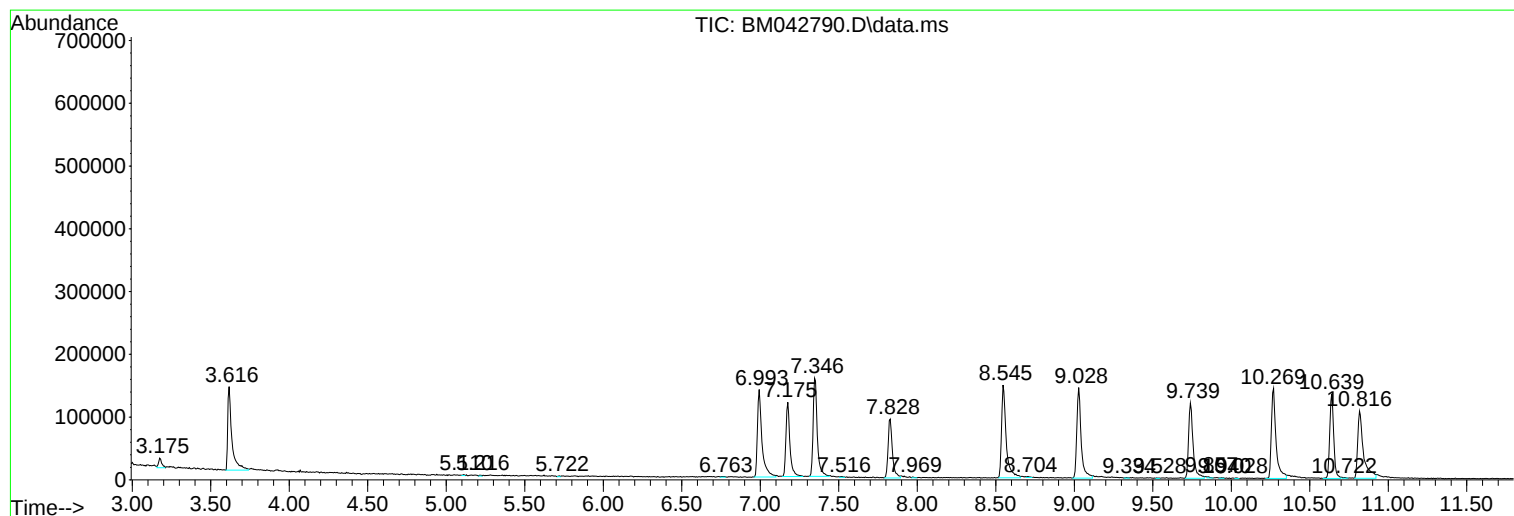

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042790.D
Acq On : 16 Nov 2023 04:43
Operator : MA/JU
Sample : PB156744BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK744

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042790.D
Acq On : 16 Nov 2023 04:43
Operator : MA/JU
Sample : PB156744BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK744

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------