

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
 Data File : BM042791.D
 Acq On : 16 Nov 2023 05:19
 Operator : MA/JU
 Sample : PB156745BL
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK745

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM042791.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	29	32	37	rVB2	15274	19347	1.84%	0.199%
2	3.616	103	107	123	rBV	145351	252567	24.00%	2.593%
3	4.493	254	256	258	rVB2	1735	1127	0.11%	0.012%
4	4.534	261	263	266	rBV4	1371	1557	0.15%	0.016%
5	5.151	366	368	369	rBV2	1232	1068	0.10%	0.011%
6	5.857	485	488	489	rBV3	912	1073	0.10%	0.011%
7	6.004	511	513	514	rBV2	1514	1152	0.11%	0.012%
8	6.634	619	620	624	rBV4	877	1121	0.11%	0.012%
9	6.763	638	642	643	rBV4	908	1366	0.13%	0.014%
10	6.992	675	681	702	rBV	151540	304740	28.95%	3.129%
11	7.175	706	712	725	rVV	131241	227427	21.61%	2.335%
12	7.298	729	733	735	rVB5	1013	1291	0.12%	0.013%
13	7.345	735	741	755	rBV	179729	313324	29.77%	3.217%
14	7.628	787	789	791	rVB2	1704	1248	0.12%	0.013%
15	7.828	817	823	838	rBV	105680	195123	18.54%	2.004%
16	8.133	871	875	876	rBV3	851	1234	0.12%	0.013%
17	8.269	894	898	901	rVV5	1152	1593	0.15%	0.016%
18	8.545	939	945	965	rBV	163386	334829	31.81%	3.438%
19	9.028	1021	1027	1045	rBV	156391	301001	28.60%	3.091%
20	9.739	1142	1148	1161	rBV2	133348	255761	24.30%	2.626%
21	10.086	1205	1207	1211	rVB2	1186	1307	0.12%	0.013%
22	10.269	1231	1238	1258	rBV	152612	331628	31.51%	3.405%
23	10.639	1293	1301	1312	rBV	152712	258900	24.60%	2.658%
24	10.710	1312	1313	1317	rVB4	1376	1422	0.14%	0.015%
25	10.816	1325	1331	1355	rBV	118945	304746	28.96%	3.129%
26	10.998	1361	1362	1367	rVB4	1581	2054	0.20%	0.021%
27	11.398	1428	1430	1432	rBV3	1027	1115	0.11%	0.011%
28	12.257	1572	1576	1577	rBV3	1115	1200	0.11%	0.012%
29	12.269	1577	1578	1582	rVB2	1270	1078	0.10%	0.011%
30	13.327	1755	1758	1766	rBV5	2789	4166	0.40%	0.043%
31	13.557	1791	1797	1800	rBV4	567	1102	0.10%	0.011%
32	13.704	1817	1822	1824	rBV4	911	1278	0.12%	0.013%
33	13.904	1850	1856	1869	rBV	370397	535567	50.89%	5.499%
34	14.180	1897	1903	1916	rBV	379563	574468	54.58%	5.899%
35	14.480	1948	1954	1969	rBV	212529	325099	30.89%	3.338%
36	14.757	1993	2001	2014	rBV4	31247	122588	11.65%	1.259%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
 Data File : BM042791.D
 Acq On : 16 Nov 2023 05:19
 Operator : MA/JU
 Sample : PB156745BL
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK745

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

37	14.933	2030	2031	2035	rVV3	1378	1116	0.11%	0.011%
38	15.133	2063	2065	2068	rVB4	1336	1442	0.14%	0.015%
39	15.474	2117	2123	2141	rBV	482222	721186	68.52%	7.405%
40	15.621	2143	2148	2160	rBV	123816	214079	20.34%	2.198%
41	16.215	2246	2249	2251	rBV3	960	1166	0.11%	0.012%
42	17.233	2417	2422	2433	rBV	260669	381273	36.23%	3.915%
43	17.333	2433	2439	2465	rVB	506293	771122	73.27%	7.918%
44	17.827	2519	2523	2526	rBV3	1067	1839	0.17%	0.019%
45	18.392	2613	2619	2621	rBV6	960	1477	0.14%	0.015%
46	18.962	2714	2716	2720	rBV4	1039	1063	0.10%	0.011%
47	19.192	2753	2755	2761	rVB5	4383	6162	0.59%	0.063%
48	19.268	2765	2768	2772	rVV4	2969	4718	0.45%	0.048%
49	19.374	2783	2786	2788	rVB3	1182	1324	0.13%	0.014%
50	19.397	2788	2790	2793	rBV3	1317	1440	0.14%	0.015%
51	19.633	2824	2830	2845	rBV	727935	969324	92.10%	9.953%
52	20.044	2898	2900	2902	rBV3	1933	1809	0.17%	0.019%
53	21.421	3129	3134	3146	rBV	277248	437658	41.58%	4.494%
54	23.627	3502	3509	3523	rBV2	517177	1052471	100.00%	10.807%
55	23.780	3529	3535	3545	rVB	232537	482649	45.86%	4.956%




Sum of corrected areas: 9738985

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042791.D
Acq On : 16 Nov 2023 05:19
Operator : MA/JU
Sample : PB156745BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK745

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

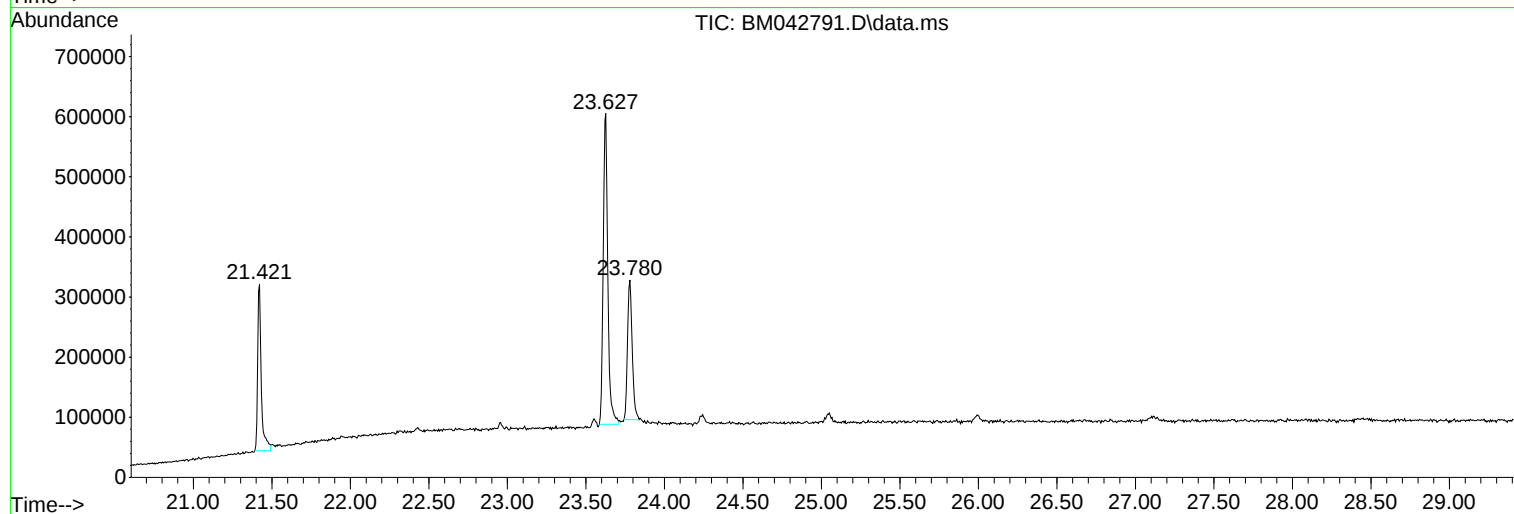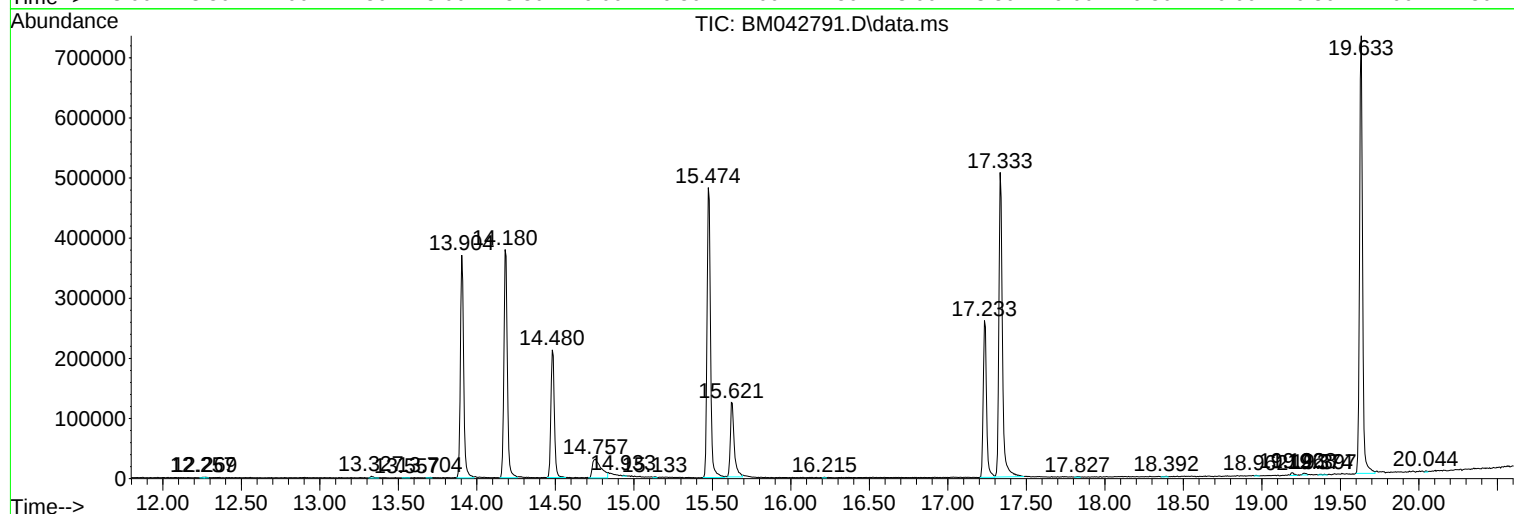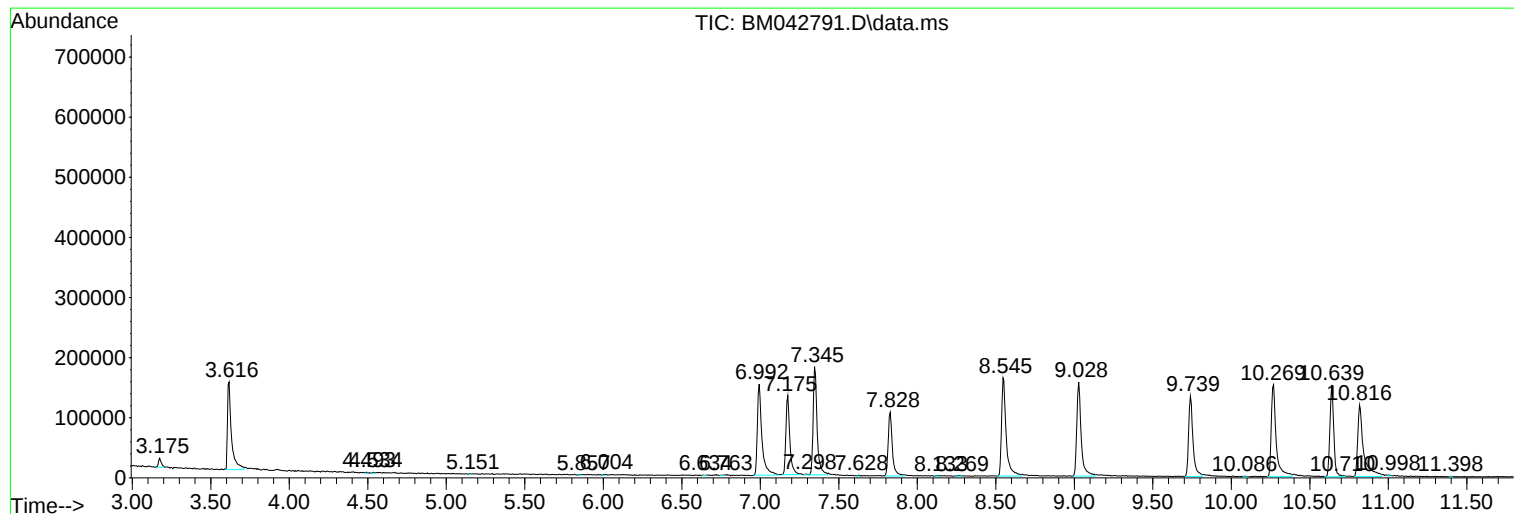

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042791.D
Acq On : 16 Nov 2023 05:19
Operator : MA/JU
Sample : PB156745BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK745

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042791.D
Acq On : 16 Nov 2023 05:19
Operator : MA/JU
Sample : PB156745BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK745

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------