

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
 Data File : BM042792.D
 Acq On : 16 Nov 2023 05:55
 Operator : MA/JU
 Sample : 05105-06
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0008

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM042792.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	30	33	37	rVB3	6421	8723	0.80%	0.105%
2	3.628	106	109	120	rBV2	20081	42325	3.87%	0.511%
3	5.604	442	445	449	rBV5	1179	2059	0.19%	0.025%
4	5.663	452	455	459	rVB4	1608	1723	0.16%	0.021%
5	5.704	459	462	463	rBV3	1078	1156	0.11%	0.014%
6	6.739	634	638	639	rBV3	1211	1281	0.12%	0.015%
7	6.857	657	658	663	rBV4	1488	1938	0.18%	0.023%
8	7.004	677	683	693	rBV2	16285	43356	3.97%	0.524%
9	7.175	706	712	725	rBV	103451	184799	16.90%	2.232%
10	7.351	736	742	753	rBV	103513	186324	17.04%	2.250%
11	7.828	816	823	839	rBV	114425	222716	20.37%	2.690%
12	8.551	941	946	960	rBV2	57979	122837	11.24%	1.484%
13	8.686	967	969	975	rVB4	1689	2661	0.24%	0.032%
14	8.845	993	996	998	rBV3	944	1181	0.11%	0.014%
15	8.939	1007	1012	1018	rBV2	9287	15403	1.41%	0.186%
16	9.028	1021	1027	1041	rBV	126850	243547	22.28%	2.941%
17	9.322	1075	1077	1082	rVB5	993	1557	0.14%	0.019%
18	9.380	1082	1087	1088	rVB4	853	1177	0.11%	0.014%
19	9.739	1142	1148	1159	rBV	68274	140060	12.81%	1.692%
20	10.269	1232	1238	1253	rBV2	109117	230480	21.08%	2.784%
21	10.639	1294	1301	1311	rBV	167102	282634	25.85%	3.413%
22	10.822	1325	1332	1350	rBV	75680	201594	18.44%	2.435%
23	11.163	1388	1390	1393	rVB3	951	1265	0.12%	0.015%
24	11.839	1499	1505	1507	rVB4	760	1412	0.13%	0.017%
25	12.251	1573	1575	1581	rVB4	828	1495	0.14%	0.018%
26	13.063	1709	1713	1716	rVB3	1469	1838	0.17%	0.022%
27	13.333	1754	1759	1762	rVB3	2972	4529	0.41%	0.055%
28	13.904	1850	1856	1870	rBV	306013	443566	40.57%	5.357%
29	14.180	1897	1903	1918	rBV	318556	476340	43.57%	5.753%
30	14.480	1945	1954	1967	rBV	254180	370213	33.86%	4.471%
31	15.168	2069	2071	2074	rVV2	937	1194	0.11%	0.014%
32	15.221	2078	2080	2082	rVB3	1371	1177	0.11%	0.014%
33	15.474	2118	2123	2143	rBV	401658	617043	56.44%	7.452%
34	15.609	2143	2146	2147	rVV3	1395	1607	0.15%	0.019%
35	15.639	2147	2151	2158	rVV4	8729	18846	1.72%	0.228%
36	15.733	2162	2167	2172	rVB7	2745	5968	0.55%	0.072%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
 Data File : BM042792.D
 Acq On : 16 Nov 2023 05:55
 Operator : MA/JU
 Sample : 05105-06
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0008

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

37	17.121	2400	2403	2406	rBV2	964	1263	0.12%	0.015%
38	17.233	2417	2422	2433	rBV	295429	422917	38.68%	5.108%
39	17.333	2433	2439	2457	rVV	488857	756292	69.18%	9.134%
40	17.451	2457	2459	2464	rVV4	3048	4937	0.45%	0.060%
41	17.486	2464	2465	2470	rVB4	1637	1604	0.15%	0.019%
42	17.868	2525	2530	2534	rBV2	27460	32266	2.95%	0.390%
43	18.074	2560	2565	2568	rBV2	1006	1300	0.12%	0.016%
44	18.109	2568	2571	2572	rBV2	1662	1759	0.16%	0.021%
45	18.350	2610	2612	2617	rVB4	2126	2735	0.25%	0.033%
46	18.650	2660	2663	2665	rBV4	998	1171	0.11%	0.014%
47	19.145	2746	2747	2751	rBV3	946	1297	0.12%	0.016%
48	19.192	2752	2755	2761	rVB5	3514	5522	0.51%	0.067%
49	19.268	2764	2768	2771	rBV4	4680	5885	0.54%	0.071%
50	19.509	2801	2809	2811	rBV6	2865	5054	0.46%	0.061%
51	19.574	2817	2820	2824	rBV3	1577	2828	0.26%	0.034%
52	19.633	2824	2830	2844	rBV	712739	954603	87.32%	11.529%
53	20.103	2908	2910	2911	rBV2	1944	1143	0.10%	0.014%
54	21.421	3129	3134	3146	rBV	322524	498864	45.63%	6.025%
55	23.627	3502	3509	3526	rBV2	531274	1093241	100.00%	13.203%
56	23.780	3528	3535	3547	rBV	276461	599278	54.82%	7.238%




Sum of corrected areas: 8279983

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042792.D
Acq On : 16 Nov 2023 05:55
Operator : MA/JU
Sample : 05105-06
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0008

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

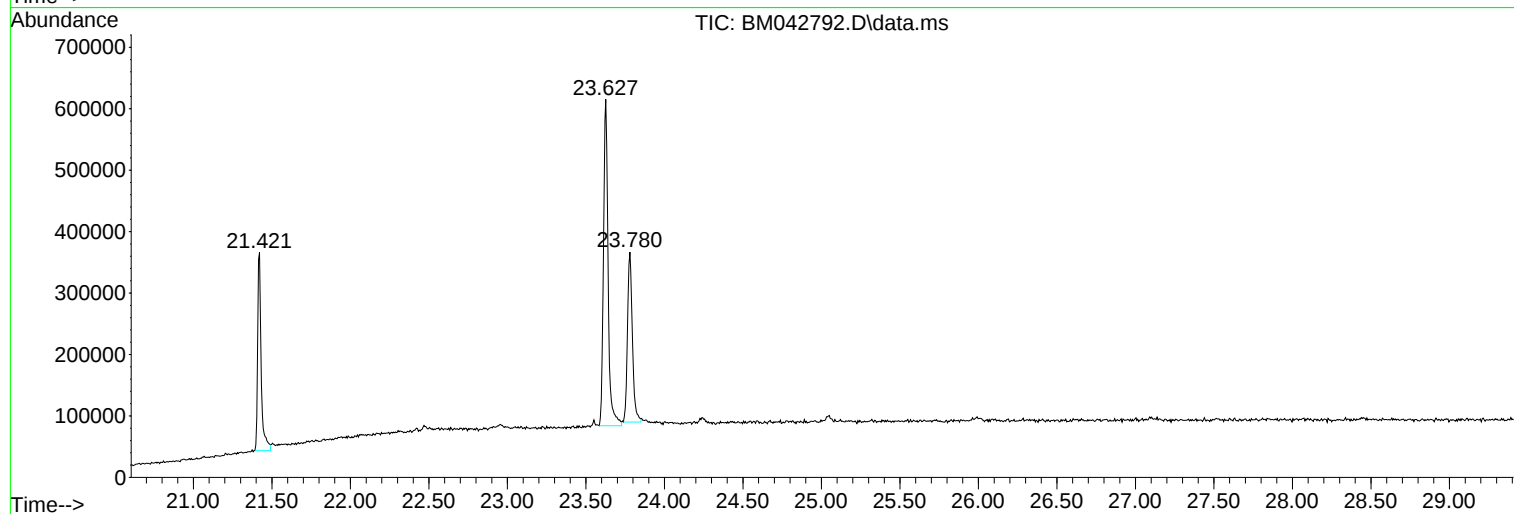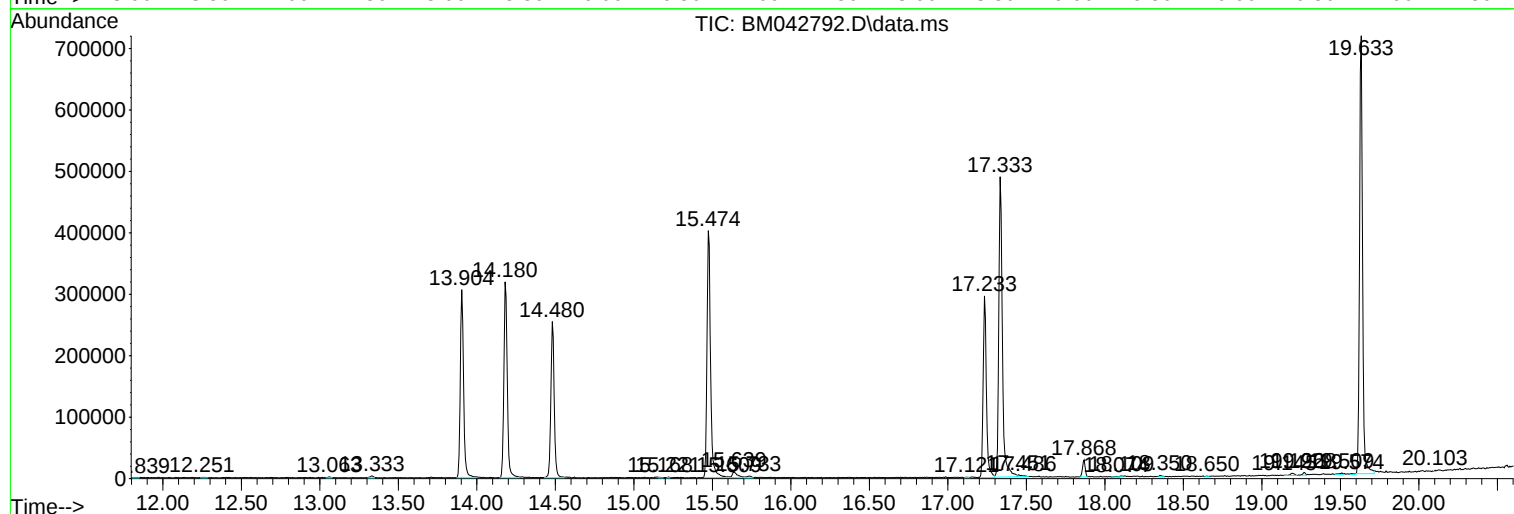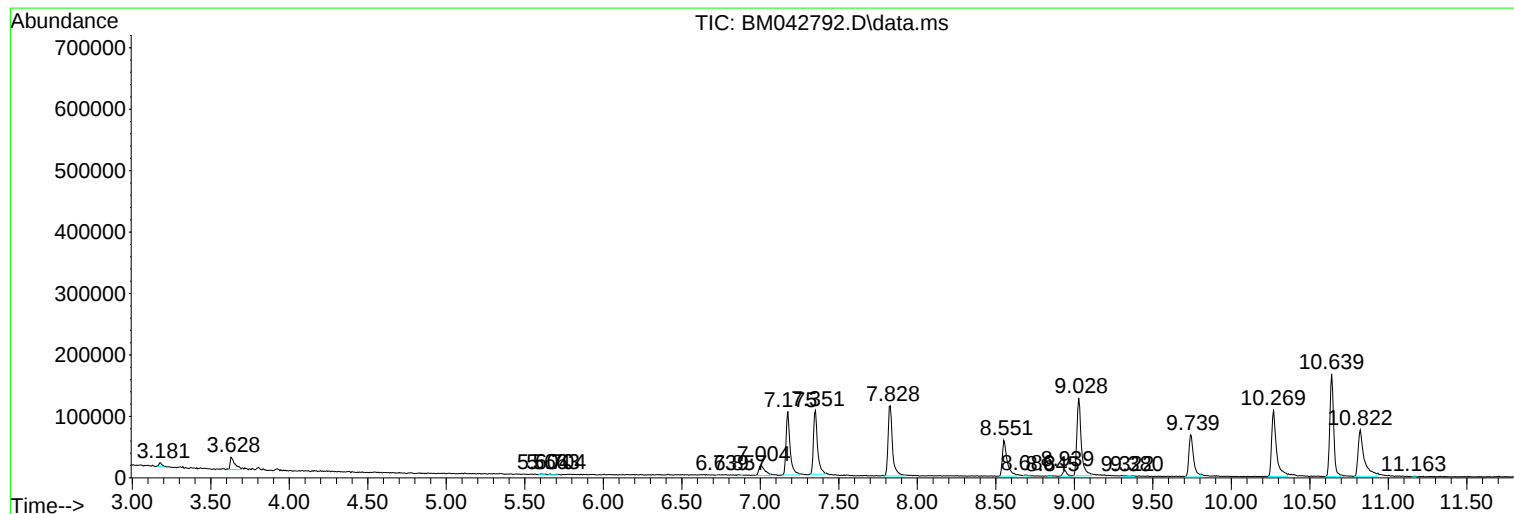

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042792.D
Acq On : 16 Nov 2023 05:55
Operator : MA/JU
Sample : 05105-06
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0008

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042792.D
Acq On : 16 Nov 2023 05:55
Operator : MA/JU
Sample : 05105-06
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0008

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc