

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
 Data File : BM042793.D
 Acq On : 16 Nov 2023 06:31
 Operator : MA/JU
 Sample : 05105-07
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0009

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM042793.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.128	20	24	30	rBV2	25441	33537	2.96%	0.385%
2	3.175	30	32	37	rVB2	7886	9388	0.83%	0.108%
3	3.628	106	109	121	rBV	23698	48834	4.31%	0.561%
4	3.922	156	159	163	rVB5	3573	5245	0.46%	0.060%
5	4.622	276	278	280	rBV4	1408	1360	0.12%	0.016%
6	4.887	321	323	326	rBV4	1034	1149	0.10%	0.013%
7	5.134	363	365	368	rBV3	1509	1745	0.15%	0.020%
8	5.310	393	395	398	rVB4	2056	1421	0.13%	0.016%
9	6.046	518	520	523	rVB4	1728	1956	0.17%	0.022%
10	6.081	523	526	529	rBV5	1597	2772	0.24%	0.032%
11	6.704	629	632	633	rBV2	2178	1601	0.14%	0.018%
12	6.998	678	682	694	rBV2	14482	38547	3.41%	0.443%
13	7.175	706	712	728	rBV	108754	200123	17.68%	2.298%
14	7.351	736	742	754	rBV	95987	184707	16.32%	2.121%
15	7.504	766	768	772	rBV4	1326	1601	0.14%	0.018%
16	7.828	816	823	837	rBV	116824	221922	19.61%	2.548%
17	8.010	851	854	858	rVB4	771	1147	0.10%	0.013%
18	8.351	911	912	917	rBV3	930	1273	0.11%	0.015%
19	8.557	942	947	958	rBV	40237	89542	7.91%	1.028%
20	9.028	1019	1027	1039	rBV	131136	255020	22.53%	2.928%
21	9.739	1142	1148	1163	rBV2	111125	214794	18.98%	2.466%
22	9.910	1176	1177	1184	rVB4	1118	1599	0.14%	0.018%
23	10.269	1232	1238	1261	rBV	103217	241460	21.33%	2.773%
24	10.639	1294	1301	1313	rBV	162439	280975	24.82%	3.226%
25	10.822	1325	1332	1344	rBV3	35540	101940	9.01%	1.171%
26	12.263	1573	1577	1581	rBV3	891	1426	0.13%	0.016%
27	13.327	1754	1758	1762	rBV5	1579	2251	0.20%	0.026%
28	13.904	1850	1856	1870	rBV	356333	502757	44.42%	5.773%
29	14.033	1877	1878	1883	rVB4	1097	1139	0.10%	0.013%
30	14.180	1897	1903	1915	rBV	347093	516851	45.66%	5.935%
31	14.480	1948	1954	1964	rVV	252866	364734	32.22%	4.188%
32	14.663	1980	1985	1986	rBV2	810	1236	0.11%	0.014%
33	14.792	2004	2007	2008	rBV3	1689	1948	0.17%	0.022%
34	15.474	2117	2123	2136	rBV	469787	676598	59.78%	7.769%
35	15.569	2136	2139	2143	rVV5	6897	11942	1.06%	0.137%
36	15.621	2143	2148	2166	rVB	124911	228004	20.14%	2.618%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
 Data File : BM042793.D
 Acq On : 16 Nov 2023 06:31
 Operator : MA/JU
 Sample : 05105-07
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0009

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

37	15.857	2186	2188	2196	rVB5	2595	4284	0.38%	0.049%
38	16.133	2230	2235	2240	rBV4	836	1540	0.14%	0.018%
39	16.192	2242	2245	2248	rVB3	2024	2325	0.21%	0.027%
40	16.580	2308	2311	2315	rVB4	950	1187	0.10%	0.014%
41	16.627	2318	2319	2323	rBV3	973	1273	0.11%	0.015%
42	17.233	2417	2422	2433	rBV	299366	427992	37.81%	4.914%
43	17.333	2433	2439	2457	rVV	467119	700807	61.92%	8.047%
44	17.662	2492	2495	2499	rVB5	1153	1334	0.12%	0.015%
45	17.851	2524	2527	2528	rBV2	1379	1470	0.13%	0.017%
46	18.086	2563	2567	2574	rBV5	11924	22467	1.98%	0.258%
47	18.174	2581	2582	2590	rVB5	1503	2193	0.19%	0.025%
48	18.651	2660	2663	2666	rBV4	3761	4690	0.41%	0.054%
49	18.768	2681	2683	2686	rVB2	1184	1151	0.10%	0.013%
50	19.192	2752	2755	2759	rVB5	5899	6072	0.54%	0.070%
51	19.239	2761	2763	2764	rBV2	1299	1136	0.10%	0.013%
52	19.262	2765	2767	2771	rVB3	4966	6023	0.53%	0.069%
53	19.374	2782	2786	2794	rBV8	5001	10133	0.90%	0.116%
54	19.480	2800	2804	2805	rBV2	1650	2344	0.21%	0.027%
55	19.633	2824	2830	2838	rBV	733623	990767	87.53%	11.377%
56	20.051	2900	2901	2902	rBV	2723	1145	0.10%	0.013%
57	20.374	2954	2956	2960	rVB4	2592	1644	0.15%	0.019%
58	20.556	2984	2987	2989	rBV4	4180	3791	0.33%	0.044%
59	21.086	3074	3077	3084	rBV5	12494	23487	2.08%	0.270%
60	21.421	3129	3134	3146	rBV	339623	519094	45.86%	5.961%
61	23.627	3502	3509	3522	rBV	565308	1131867	100.00%	12.997%
62	23.780	3529	3535	3546	rVB	296755	586052	51.78%	6.729%




Sum of corrected areas: 8708812

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042793.D
Acq On : 16 Nov 2023 06:31
Operator : MA/JU
Sample : 05105-07
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0009

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

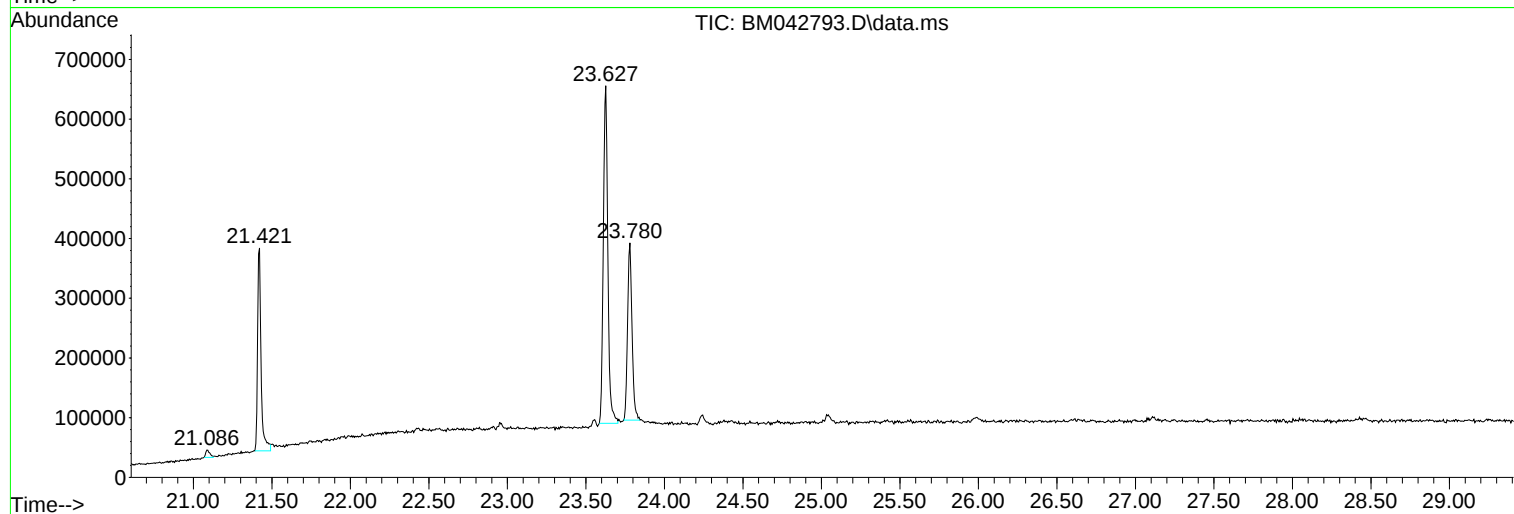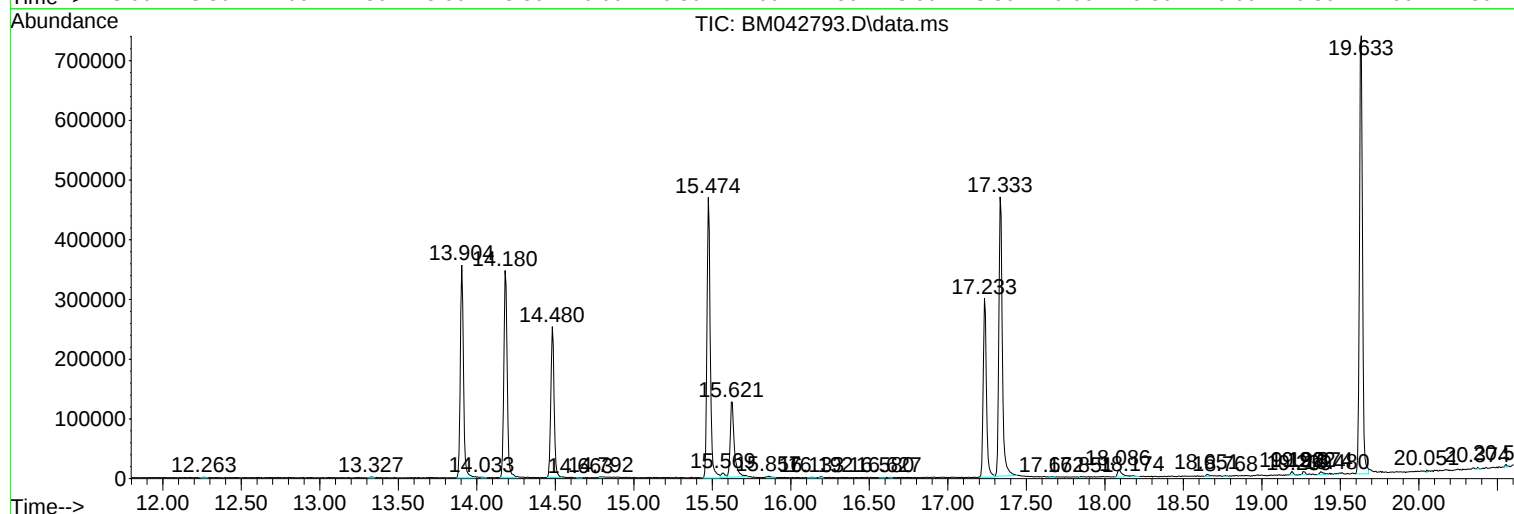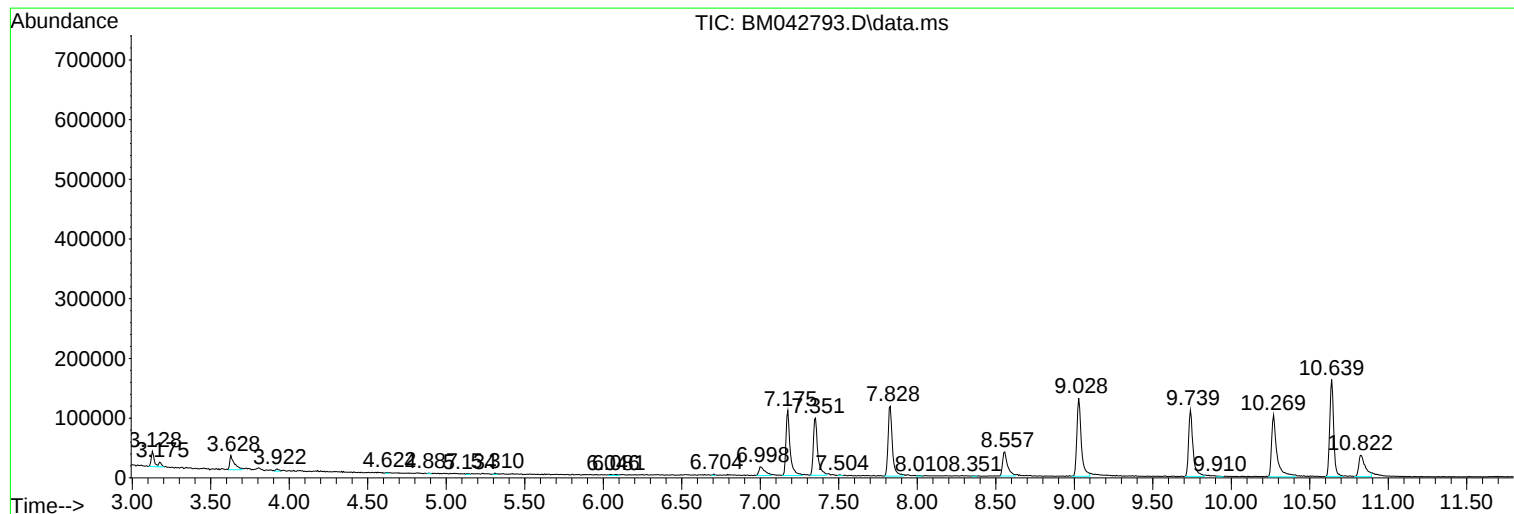

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042793.D
Acq On : 16 Nov 2023 06:31
Operator : MA/JU
Sample : 05105-07
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0009

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042793.D
Acq On : 16 Nov 2023 06:31
Operator : MA/JU
Sample : 05105-07
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0009

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc