

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
 Data File : BM042794.D
 Acq On : 16 Nov 2023 07:07
 Operator : MA/JU
 Sample : 05105-08
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0010

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM042794.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	29	33	37	rVB3	6497	8649	0.85%	0.101%
2	3.628	105	109	121	rBV	23967	46542	4.57%	0.544%
3	4.151	196	198	199	rVB2	2350	1070	0.11%	0.013%
4	5.198	374	376	378	rBV3	1370	1279	0.13%	0.015%
5	5.287	389	391	395	rBV5	849	1092	0.11%	0.013%
6	5.510	427	429	433	rVB4	979	1024	0.10%	0.012%
7	5.610	444	446	450	rBV4	1093	1466	0.14%	0.017%
8	5.887	491	493	495	rBV2	1029	1023	0.10%	0.012%
9	6.092	527	528	531	rBV2	1036	1062	0.10%	0.012%
10	6.998	678	682	690	rBV3	16228	38405	3.77%	0.449%
11	7.175	706	712	729	rBV	101856	188170	18.47%	2.199%
12	7.351	736	742	760	rVB	102625	191258	18.78%	2.236%
13	7.498	765	767	769	rBV3	1338	1335	0.13%	0.016%
14	7.704	798	802	805	rVV4	996	1412	0.14%	0.017%
15	7.822	816	822	835	rBV	120170	224254	22.02%	2.621%
16	8.551	941	946	965	rBV	56800	125302	12.30%	1.465%
17	8.751	979	980	986	rBV5	816	1138	0.11%	0.013%
18	9.028	1021	1027	1044	rBV	124348	245735	24.12%	2.872%
19	9.133	1044	1045	1048	rVB3	1360	1287	0.13%	0.015%
20	9.739	1140	1148	1161	rBV	100944	196917	19.33%	2.302%
21	9.922	1178	1179	1182	rVB2	1254	1024	0.10%	0.012%
22	9.957	1182	1185	1187	rBV3	914	1197	0.12%	0.014%
23	10.145	1212	1217	1218	rBV2	729	1053	0.10%	0.012%
24	10.269	1232	1238	1253	rBV	110964	241844	23.74%	2.827%
25	10.498	1274	1277	1279	rVB4	877	1019	0.10%	0.012%
26	10.522	1279	1281	1286	rVB6	1007	1209	0.12%	0.014%
27	10.639	1293	1301	1315	rBV	170809	294188	28.88%	3.439%
28	10.727	1315	1316	1319	rVB3	1680	1300	0.13%	0.015%
29	10.822	1325	1332	1349	rBV2	66975	183520	18.02%	2.145%
30	11.339	1416	1420	1423	rVB4	788	1128	0.11%	0.013%
31	11.845	1505	1506	1511	rVB3	988	1213	0.12%	0.014%
32	11.904	1511	1516	1518	rBV4	817	1247	0.12%	0.015%
33	12.257	1573	1576	1579	rBV	1153	1152	0.11%	0.013%
34	13.327	1754	1758	1761	rBV3	2476	3493	0.34%	0.041%
35	13.904	1850	1856	1871	rBV	319288	457377	44.90%	5.346%
36	14.180	1897	1903	1919	rBV	327212	486608	47.77%	5.688%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
 Data File : BM042794.D
 Acq On : 16 Nov 2023 07:07
 Operator : MA/JU
 Sample : 05105-08
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0010

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

37	14.480	1948	1954	1966	rBV	253595	373054	36.62%	4.361%
38	14.810	2004	2010	2012	rBV4	1274	2715	0.27%	0.032%
39	15.215	2074	2079	2080	rBV2	890	1052	0.10%	0.012%
40	15.274	2085	2089	2091	rVV4	1084	1491	0.15%	0.017%
41	15.304	2091	2094	2097	rVB3	878	1223	0.12%	0.014%
42	15.474	2117	2123	2134	rBV	410196	611334	60.01%	7.146%
43	15.627	2143	2149	2170	rVB	104860	198628	19.50%	2.322%
44	15.862	2182	2189	2194	rBV5	2812	6078	0.60%	0.071%
45	16.198	2242	2246	2250	rVB3	1468	1937	0.19%	0.023%
46	16.468	2289	2292	2294	rVB3	967	1113	0.11%	0.013%
47	16.509	2294	2299	2302	rBV3	1320	1957	0.19%	0.023%
48	16.898	2361	2365	2367	rBV3	1306	1474	0.14%	0.017%
49	17.033	2386	2388	2392	rVV3	798	1049	0.10%	0.012%
50	17.233	2416	2422	2433	rBV	307950	441491	43.34%	5.160%
51	17.333	2433	2439	2461	rVV	495918	752381	73.86%	8.794%
52	17.486	2464	2465	2466	rVV	2449	1325	0.13%	0.015%
53	17.674	2493	2497	2499	rVB3	849	1116	0.11%	0.013%
54	17.709	2499	2503	2505	rVB3	1945	2227	0.22%	0.026%
55	17.727	2505	2506	2509	rBV2	1285	1301	0.13%	0.015%
56	17.862	2526	2529	2536	rVB6	1203	2114	0.21%	0.025%
57	18.092	2564	2568	2574	rBV3	12719	25004	2.45%	0.292%
58	18.192	2583	2585	2590	rVB5	1788	2602	0.26%	0.030%
59	18.274	2597	2599	2603	rBV3	944	1103	0.11%	0.013%
60	18.392	2615	2619	2620	rBV2	1379	1654	0.16%	0.019%
61	18.462	2627	2631	2633	rBV3	1308	1605	0.16%	0.019%
62	18.515	2639	2640	2644	rVB3	1580	1398	0.14%	0.016%
63	18.556	2644	2647	2650	rBV3	1817	2550	0.25%	0.030%
64	18.786	2684	2686	2690	rBV4	1573	2344	0.23%	0.027%
65	19.080	2733	2736	2738	rBV3	983	1330	0.13%	0.016%
66	19.192	2751	2755	2761	rBV7	4845	7859	0.77%	0.092%
67	19.262	2764	2767	2772	rBV4	5464	8709	0.85%	0.102%
68	19.327	2775	2778	2780	rBV4	1343	1733	0.17%	0.020%
69	19.374	2782	2786	2790	rBV5	4721	7142	0.70%	0.083%
70	19.509	2806	2809	2812	rVB3	2307	2030	0.20%	0.024%
71	19.574	2818	2820	2821	rBV2	1491	1088	0.11%	0.013%
72	19.633	2824	2830	2842	rBV	702039	969398	95.17%	11.331%
73	19.850	2865	2867	2868	rBV	2159	1118	0.11%	0.013%
74	19.892	2873	2874	2876	rVV2	2518	1311	0.13%	0.015%
75	20.015	2891	2895	2897	rBV5	2983	4201	0.41%	0.049%
76	20.256	2934	2936	2937	rVB2	2436	1038	0.10%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042794.D
Acq On : 16 Nov 2023 07:07
Operator : MA/JU
Sample : 05105-08
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0010

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Title : SVOA CALIBRATION

77	21.091	3074	3078	3083	rBV7	9721	15039	1.48%	0.176%
78	21.415	3129	3133	3145	rBV	341105	523790	51.42%	6.122%
79	23.621	3502	3508	3521	rBV	518798	1018639	100.00%	11.907%
80	23.780	3529	3535	3548	rVB	293554	590537	57.97%	6.903%


Sum of corrected areas: 8555274

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042794.D
Acq On : 16 Nov 2023 07:07
Operator : MA/JU
Sample : 05105-08
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0010

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

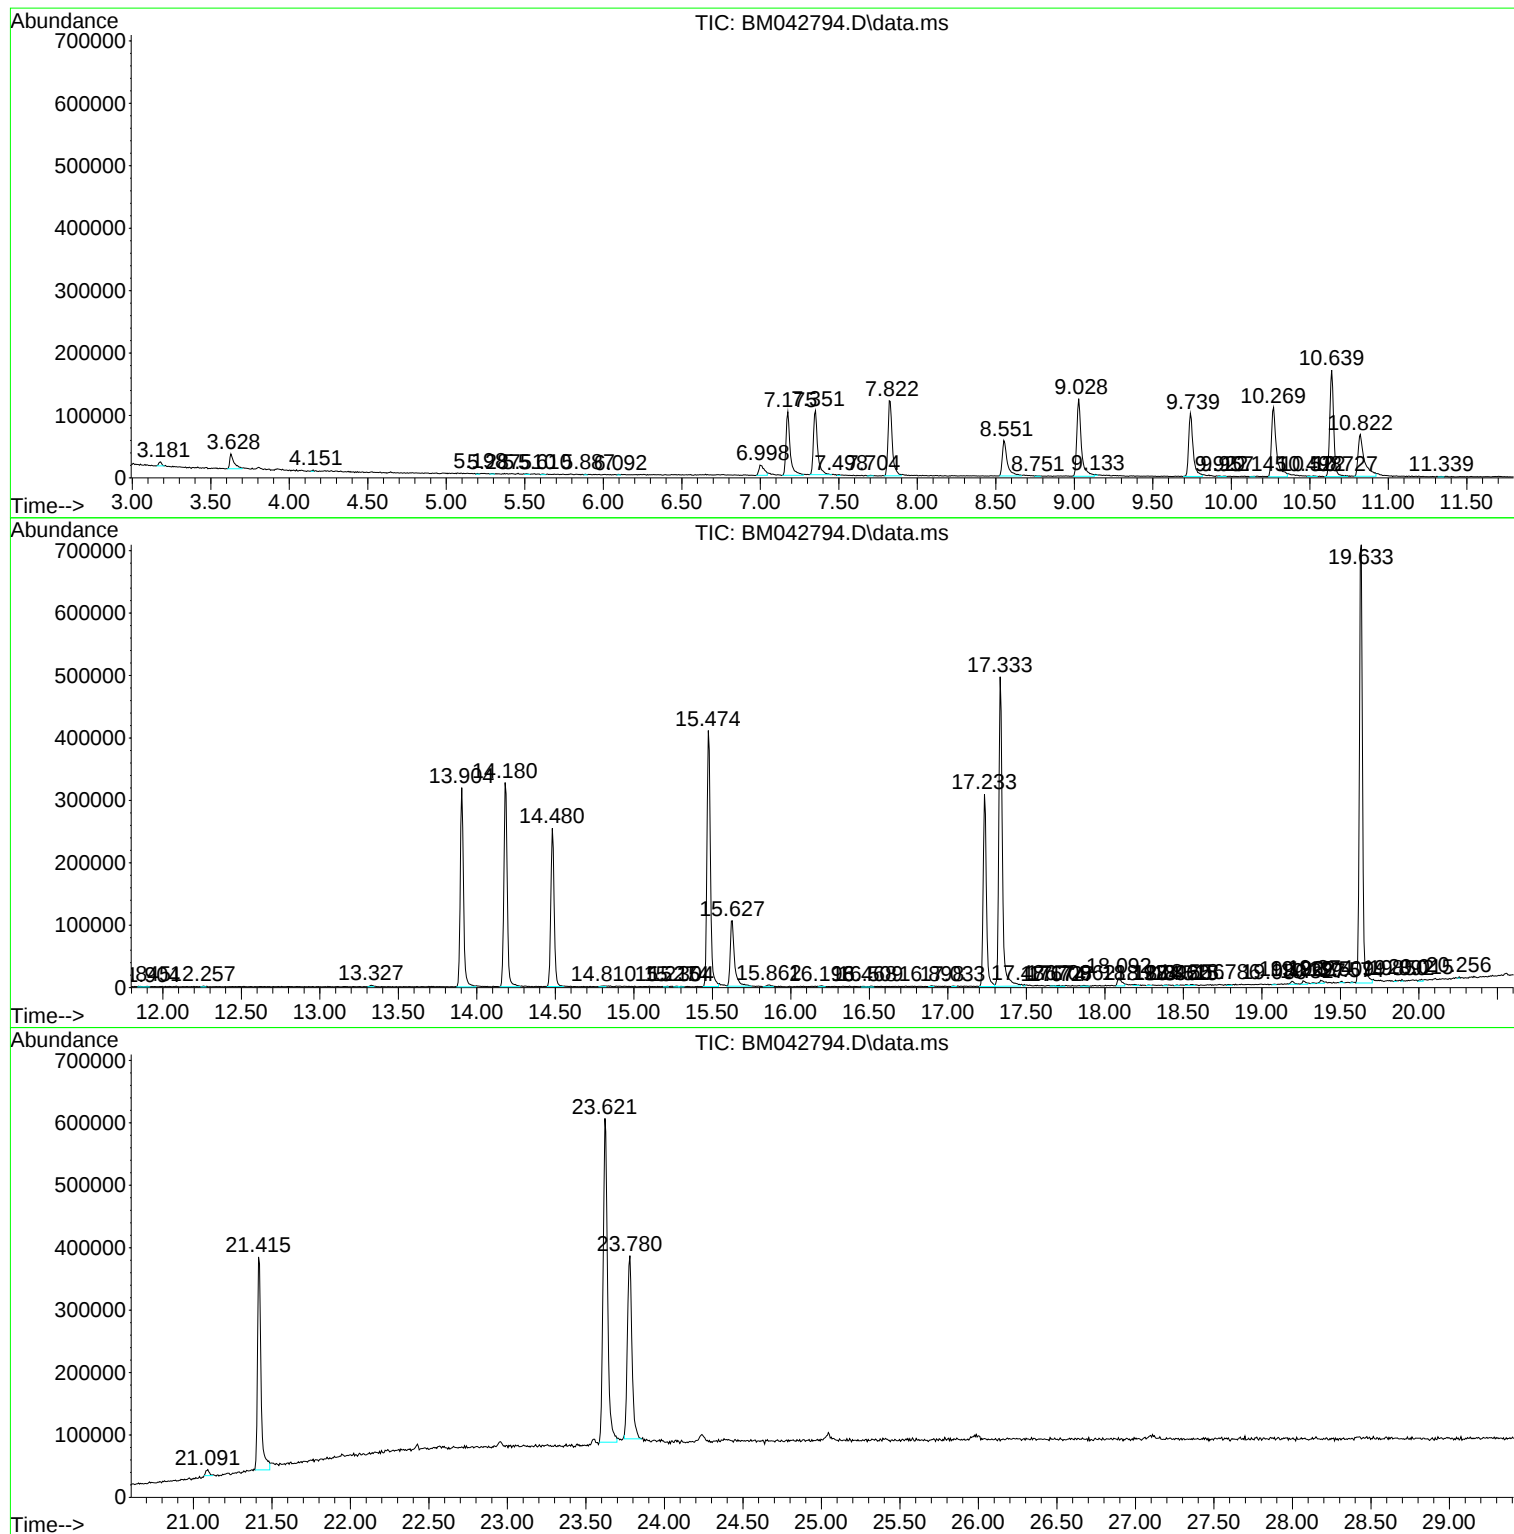

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042794.D
Acq On : 16 Nov 2023 07:07
Operator : MA/JU
Sample : 05105-08
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0010

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042794.D
Acq On : 16 Nov 2023 07:07
Operator : MA/JU
Sample : 05105-08
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0010

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc