

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
 Data File : BM042795.D
 Acq On : 16 Nov 2023 07:43
 Operator : MA/JU
 Sample : 05105-09
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0011

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM042795.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.134	21	25	28	rVB4	7479	10030	0.98%	0.117%
2	3.175	30	32	37	rVB2	8904	11234	1.10%	0.131%
3	3.628	105	109	119	rBV	23984	51523	5.04%	0.600%
4	4.381	235	237	240	rVV3	1603	1241	0.12%	0.014%
5	4.446	244	248	255	rVB2	27912	39747	3.89%	0.463%
6	5.022	345	346	350	rBV2	1531	1466	0.14%	0.017%
7	5.281	388	390	392	rBV2	1303	1376	0.13%	0.016%
8	6.104	529	530	533	rVB2	1429	1188	0.12%	0.014%
9	6.322	561	567	568	rBV3	1418	1785	0.17%	0.021%
10	6.681	626	628	631	rVB3	1238	1211	0.12%	0.014%
11	6.834	652	654	657	rVB4	996	1271	0.12%	0.015%
12	7.004	678	683	694	rBV	20617	48339	4.73%	0.563%
13	7.175	706	712	729	rBV	123269	219274	21.47%	2.552%
14	7.345	735	741	758	rBV	115129	219651	21.50%	2.557%
15	7.739	805	808	812	rBV3	749	1039	0.10%	0.012%
16	7.822	816	822	840	rVV	131246	244218	23.91%	2.843%
17	7.939	840	842	845	rVV3	1758	2383	0.23%	0.028%
18	7.981	847	849	854	rVB4	1189	1193	0.12%	0.014%
19	8.557	942	947	960	rBV3	27119	61290	6.00%	0.713%
20	9.028	1021	1027	1040	rBV	146999	280804	27.49%	3.269%
21	9.739	1142	1148	1160	rBV	123078	235431	23.05%	2.740%
22	9.822	1160	1162	1167	rVB6	2475	3597	0.35%	0.042%
23	10.269	1232	1238	1256	rBV	110418	257819	25.24%	3.001%
24	10.639	1295	1301	1317	rBV	174946	305817	29.94%	3.560%
25	10.827	1326	1333	1347	rBV4	20102	62027	6.07%	0.722%
26	11.516	1448	1450	1456	rBV4	971	1537	0.15%	0.018%
27	12.333	1587	1589	1596	rBV4	772	1207	0.12%	0.014%
28	13.333	1753	1759	1761	rBV3	2787	3980	0.39%	0.046%
29	13.904	1850	1856	1868	rBV	382897	536068	52.48%	6.240%
30	13.980	1868	1869	1875	rVV4	2012	2929	0.29%	0.034%
31	14.180	1897	1903	1915	rBV2	360673	532766	52.15%	6.201%
32	14.280	1919	1920	1927	rVB3	1482	1775	0.17%	0.021%
33	14.480	1948	1954	1965	rBV	264442	379725	37.17%	4.420%
34	14.792	2002	2007	2010	rBV4	1970	3300	0.32%	0.038%
35	15.227	2077	2081	2082	rBV3	1113	1269	0.12%	0.015%
36	15.304	2088	2094	2099	rVB	10556	14123	1.38%	0.164%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
 Data File : BM042795.D
 Acq On : 16 Nov 2023 07:43
 Operator : MA/JU
 Sample : 05105-09
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0011

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

37	15.474	2117	2123	2136	rBV	490672	710458	69.55%	8.270%
38	15.621	2143	2148	2164	rBV	136608	227854	22.31%	2.652%
39	15.862	2184	2189	2194	rVB3	2977	5084	0.50%	0.059%
40	16.192	2240	2245	2249	rBV4	1876	3018	0.30%	0.035%
41	16.509	2293	2299	2301	rBV3	953	1166	0.11%	0.014%
42	16.809	2348	2350	2354	rVB3	1020	1210	0.12%	0.014%
43	16.892	2363	2364	2367	rVV2	1225	1449	0.14%	0.017%
44	17.233	2415	2422	2433	rBV	304373	439095	42.98%	5.111%
45	17.333	2433	2439	2458	rVB	333679	522808	51.18%	6.086%
46	17.498	2465	2467	2468	rVB2	2166	1042	0.10%	0.012%
47	18.092	2562	2568	2574	rBV4	12788	24395	2.39%	0.284%
48	18.186	2581	2584	2587	rVB2	1535	2111	0.21%	0.025%
49	18.227	2590	2591	2594	rVB3	1693	1225	0.12%	0.014%
50	18.650	2658	2663	2670	rVV4	13893	26516	2.60%	0.309%
51	18.733	2674	2677	2678	rVV3	1903	2110	0.21%	0.025%
52	18.762	2681	2682	2687	rVB5	1436	2022	0.20%	0.024%
53	18.992	2719	2721	2723	rVB2	1984	1272	0.12%	0.015%
54	19.192	2752	2755	2761	rVB5	6341	8294	0.81%	0.097%
55	19.239	2761	2763	2764	rBV2	1392	1276	0.12%	0.015%
56	19.262	2764	2767	2773	rBV3	6126	8121	0.79%	0.095%
57	19.374	2784	2786	2790	rBV4	4087	5378	0.53%	0.063%
58	19.509	2806	2809	2811	rBV4	2816	3529	0.35%	0.041%
59	19.627	2824	2829	2841	rBV	704715	920173	90.08%	10.711%
60	19.903	2874	2876	2879	rBV3	2429	1908	0.19%	0.022%
61	20.009	2890	2894	2895	rBV3	3042	3153	0.31%	0.037%
62	20.103	2906	2910	2911	rBV4	2842	3716	0.36%	0.043%
63	20.397	2958	2960	2966	rBV7	2402	3845	0.38%	0.045%
64	21.415	3128	3133	3146	rBV	341865	517448	50.65%	6.023%
65	23.621	3502	3508	3524	rBV	509893	1021534	100.00%	11.891%
66	23.780	3528	3535	3545	rVV	272979	576118	56.40%	6.706%




Sum of corrected areas: 8590961

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042795.D
Acq On : 16 Nov 2023 07:43
Operator : MA/JU
Sample : 05105-09
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0011

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

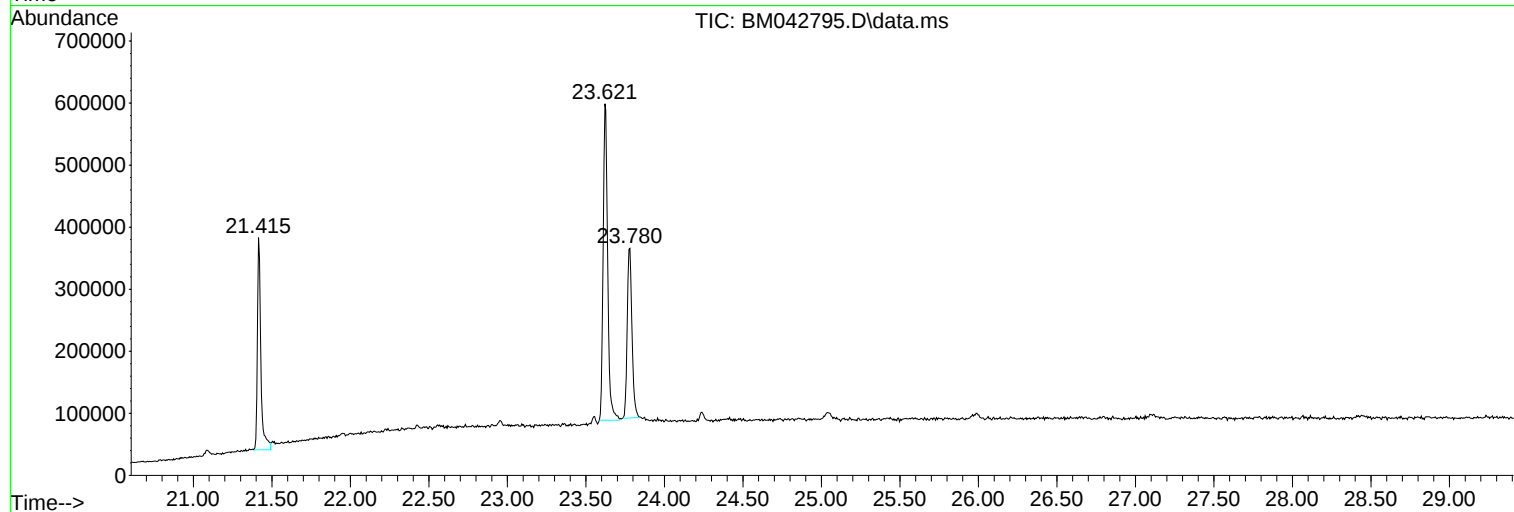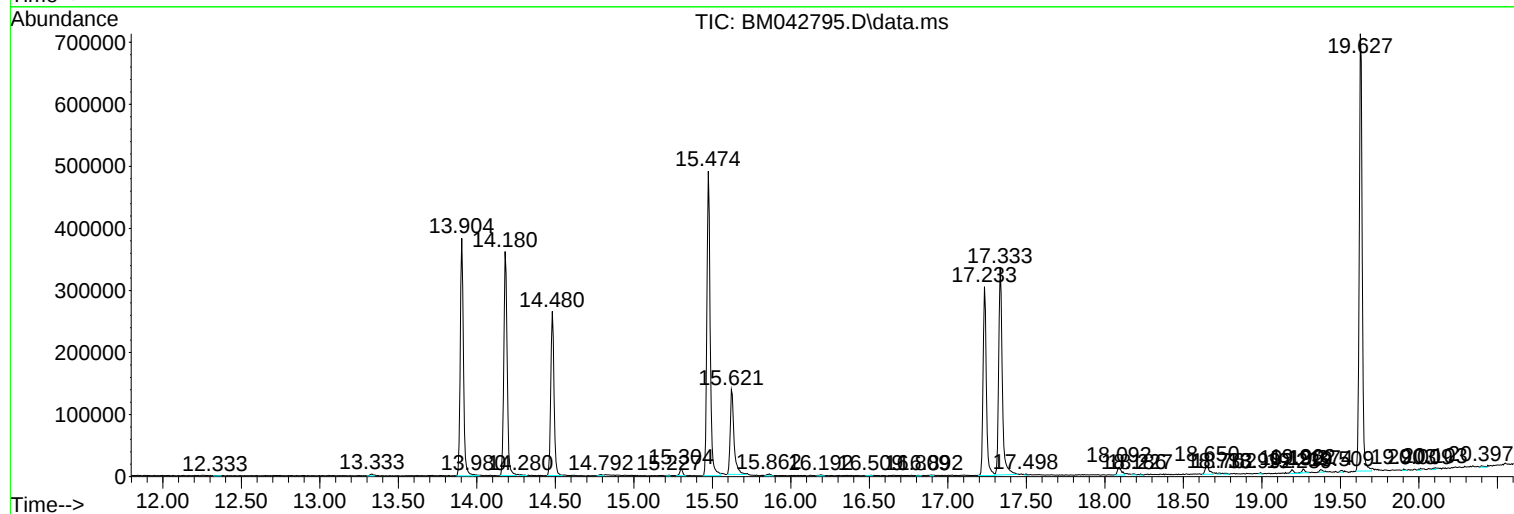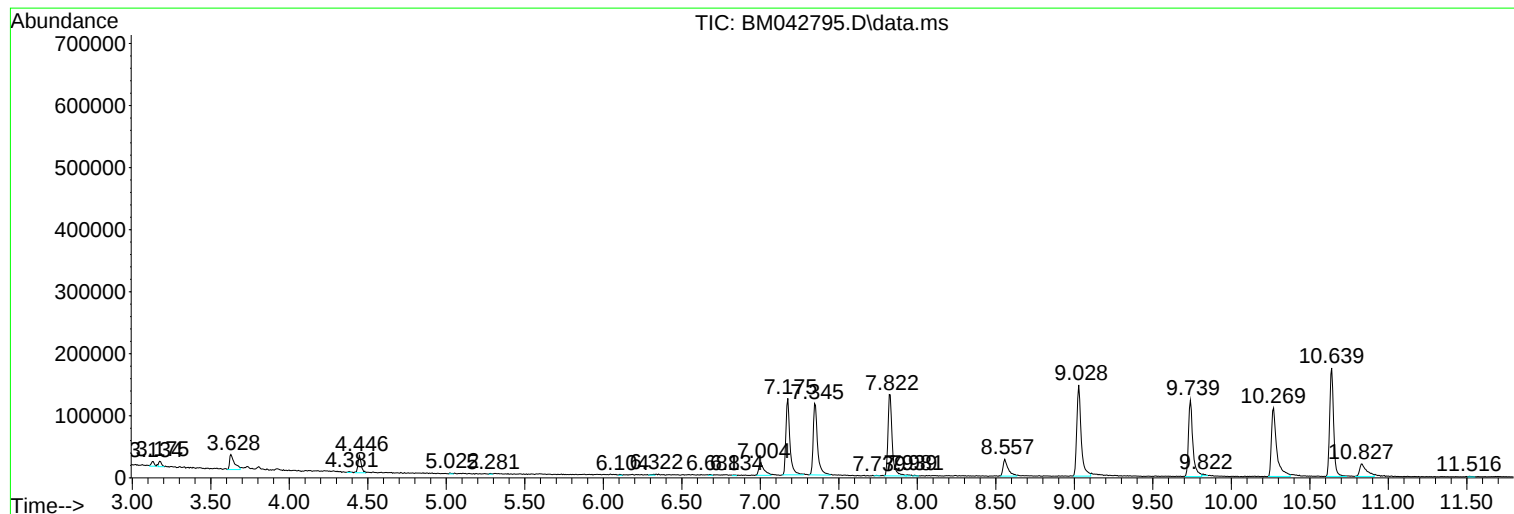

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042795.D
Acq On : 16 Nov 2023 07:43
Operator : MA/JU
Sample : 05105-09
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0011

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042795.D
Acq On : 16 Nov 2023 07:43
Operator : MA/JU
Sample : 05105-09
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0011

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc