

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
 Data File : BM042796.D
 Acq On : 16 Nov 2023 08:19
 Operator : MA/JU
 Sample : 05105-16
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0012

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM042796.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.128	20	24	29	rBV	36789	45919	3.77%	0.470%
2	3.628	106	109	117	rBV	26008	49111	4.03%	0.503%
3	3.810	135	140	144	rVB6	4344	7765	0.64%	0.079%
4	4.446	244	248	255	rVB2	18315	27308	2.24%	0.279%
5	4.916	327	328	330	rBV2	1660	1284	0.11%	0.013%
6	6.863	656	659	661	rBV4	829	1303	0.11%	0.013%
7	6.998	677	682	694	rBV2	23677	55576	4.56%	0.569%
8	7.175	706	712	725	rBV	123617	223166	18.32%	2.284%
9	7.346	735	741	756	rBV	126851	238780	19.60%	2.444%
10	7.481	762	764	767	rVB2	1675	1323	0.11%	0.014%
11	7.822	817	822	834	rBV	133526	241540	19.83%	2.472%
12	8.551	940	946	962	rBV2	64218	142780	11.72%	1.461%
13	9.028	1021	1027	1046	rBV	152279	305101	25.05%	3.123%
14	9.204	1053	1057	1060	rBV5	1618	2296	0.19%	0.023%
15	9.739	1142	1148	1159	rBV	130642	241226	19.80%	2.469%
16	9.928	1178	1180	1185	rVB4	1395	1667	0.14%	0.017%
17	10.263	1231	1237	1253	rBV	137629	294942	24.21%	3.019%
18	10.639	1294	1301	1311	rBV	176281	312274	25.64%	3.196%
19	10.704	1311	1312	1319	rVB4	2010	2084	0.17%	0.021%
20	10.816	1325	1331	1347	rBV	72143	194540	15.97%	1.991%
21	13.333	1755	1759	1763	rVB4	2674	3852	0.32%	0.039%
22	13.904	1850	1856	1869	rBV	383393	526014	43.18%	5.384%
23	14.180	1896	1903	1919	rBV	378619	575654	47.26%	5.892%
24	14.480	1948	1954	1965	rBV	269774	396371	32.54%	4.057%
25	14.774	2001	2004	2007	rBV3	1802	2655	0.22%	0.027%
26	14.898	2024	2025	2032	rVB4	928	1328	0.11%	0.014%
27	15.174	2066	2072	2073	rBV3	647	1296	0.11%	0.013%
28	15.474	2117	2123	2135	rBV	499971	720686	59.16%	7.376%
29	15.621	2143	2148	2159	rBV	138375	227380	18.67%	2.327%
30	15.851	2182	2187	2194	rBV4	2232	5076	0.42%	0.052%
31	17.233	2416	2422	2433	rBV	335498	471554	38.71%	4.826%
32	17.333	2433	2439	2454	rVV	541662	791888	65.01%	8.105%
33	17.451	2458	2459	2461	rVV2	3169	2813	0.23%	0.029%
34	17.492	2464	2466	2469	rVV3	2170	2403	0.20%	0.025%
35	18.092	2564	2568	2576	rBV4	9273	16226	1.33%	0.166%
36	18.186	2582	2584	2588	rVB2	1492	1424	0.12%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
 Data File : BM042796.D
 Acq On : 16 Nov 2023 08:19
 Operator : MA/JU
 Sample : 05105-16
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0012

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

37	18.251	2592	2595	2596	rBV3	1080	1306	0.11%	0.013%
38	18.315	2604	2606	2609	rBV3	1253	1472	0.12%	0.015%
39	18.651	2661	2663	2668	rVB5	1692	1774	0.15%	0.018%
40	19.062	2729	2733	2736	rBV4	1758	2264	0.19%	0.023%
41	19.192	2751	2755	2761	rVB4	6256	7568	0.62%	0.077%
42	19.268	2763	2768	2772	rBV3	5675	9661	0.79%	0.099%
43	19.321	2776	2777	2780	rVB2	2889	2515	0.21%	0.026%
44	19.380	2780	2787	2791	rBV6	6307	13376	1.10%	0.137%
45	19.504	2805	2808	2812	rBV5	3065	3765	0.31%	0.039%
46	19.627	2824	2829	2844	rBV	803282	1075731	88.31%	11.010%
47	21.415	3129	3133	3149	rBV	396554	578551	47.50%	5.921%
48	23.621	3502	3508	3524	rBV	621718	1218121	100.00%	12.468%
49	23.780	3528	3535	3556	rVB	341238	717654	58.91%	7.345%




Sum of corrected areas: 9770363

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042796.D
Acq On : 16 Nov 2023 08:19
Operator : MA/JU
Sample : 05105-16
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0012

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

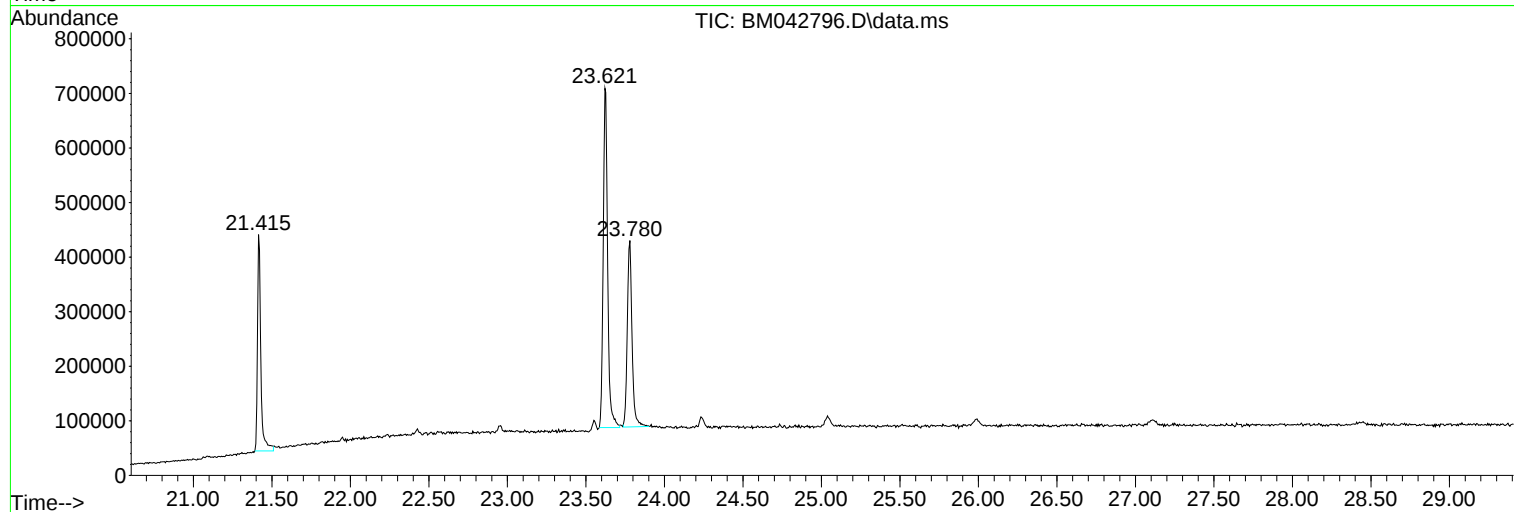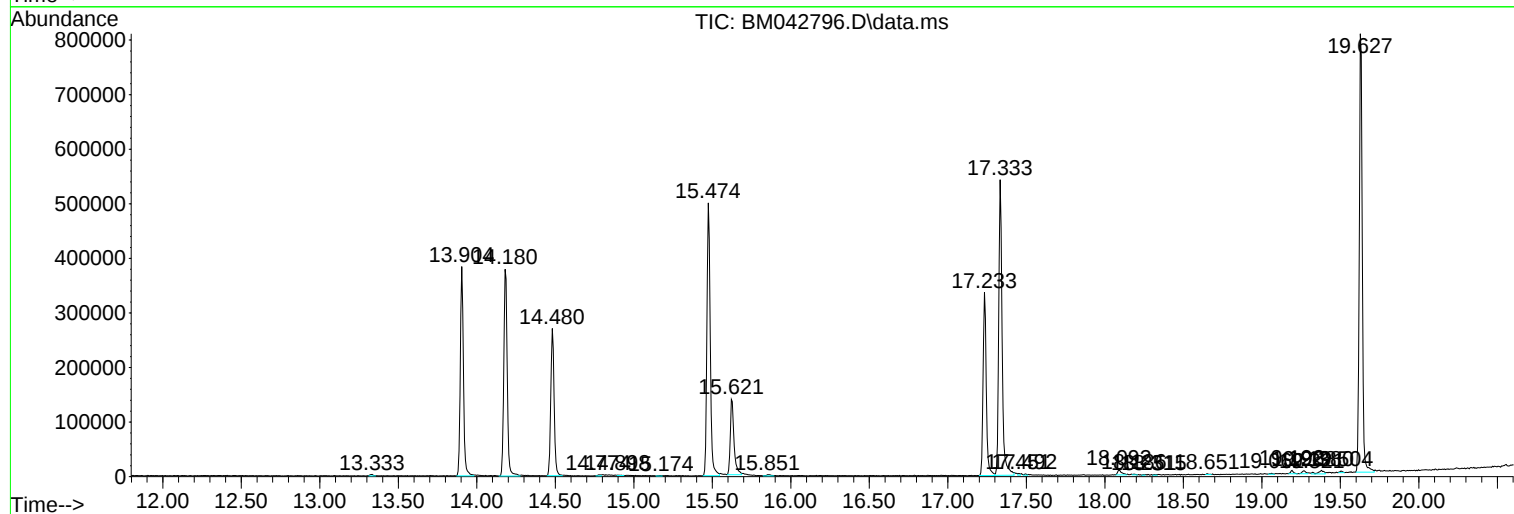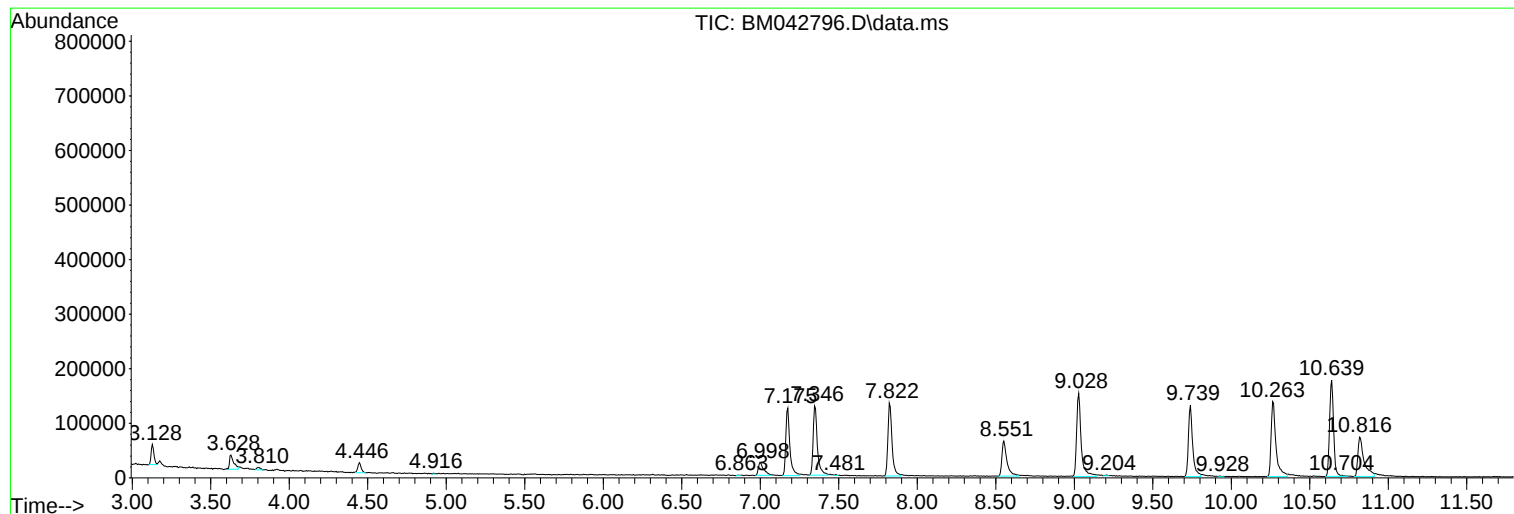

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042796.D
Acq On : 16 Nov 2023 08:19
Operator : MA/JU
Sample : 05105-16
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0012

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042796.D
Acq On : 16 Nov 2023 08:19
Operator : MA/JU
Sample : 05105-16
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0012

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------