

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
 Data File : BM042797.D
 Acq On : 16 Nov 2023 08:55
 Operator : MA/JU
 Sample : 05105-17
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0013

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM042797.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.128	20	24	29	rBV2	29731	40124	3.63%	0.462%
2	3.175	29	32	39	rVB5	9827	13851	1.25%	0.160%
3	3.628	106	109	118	rBV2	19184	38180	3.45%	0.440%
4	5.081	354	356	361	rBV5	1490	2343	0.21%	0.027%
5	5.775	471	474	475	rBV2	1197	1259	0.11%	0.015%
6	6.098	528	529	532	rVB2	1424	1226	0.11%	0.014%
7	6.998	677	682	691	rBV2	21678	51918	4.69%	0.598%
8	7.175	706	712	726	rBV	106438	193229	17.47%	2.226%
9	7.345	736	741	755	rBV	109538	204959	18.53%	2.361%
10	7.822	817	822	836	rBV	121906	226999	20.52%	2.615%
11	8.551	940	946	961	rBV2	61616	134075	12.12%	1.545%
12	9.028	1020	1027	1041	rBV	127481	250566	22.65%	2.887%
13	9.210	1057	1058	1061	rVB3	1992	1812	0.16%	0.021%
14	9.739	1141	1148	1162	rBV	107971	205982	18.62%	2.373%
15	9.892	1172	1174	1177	rVB3	1374	1281	0.12%	0.015%
16	10.045	1198	1200	1205	rVB5	1011	1393	0.13%	0.016%
17	10.269	1232	1238	1256	rBV2	114722	257182	23.25%	2.963%
18	10.386	1256	1258	1264	rVB5	2711	3960	0.36%	0.046%
19	10.639	1294	1301	1310	rBV	165536	291620	26.36%	3.360%
20	10.822	1326	1332	1348	rBV2	60937	171019	15.46%	1.970%
21	10.928	1348	1350	1354	rVB5	2971	3583	0.32%	0.041%
22	11.216	1395	1399	1402	rVB4	793	1380	0.12%	0.016%
23	11.704	1478	1482	1487	rVB4	3261	4954	0.45%	0.057%
24	12.269	1575	1578	1581	rVB3	1122	1138	0.10%	0.013%
25	13.333	1754	1759	1763	rBV3	3171	4639	0.42%	0.053%
26	13.710	1819	1823	1827	rVV4	1038	1505	0.14%	0.017%
27	13.904	1850	1856	1869	rBV	337890	476545	43.07%	5.490%
28	14.180	1897	1903	1916	rBV	345181	494591	44.70%	5.698%
29	14.480	1948	1954	1965	rBV	255647	362575	32.77%	4.177%
30	14.786	2001	2006	2010	rBV3	2591	5043	0.46%	0.058%
31	14.898	2022	2025	2028	rVB3	1050	1388	0.13%	0.016%
32	15.074	2052	2055	2060	rBV3	842	1394	0.13%	0.016%
33	15.474	2117	2123	2136	rBV	444356	648573	58.62%	7.472%
34	15.621	2142	2148	2162	rBV	122494	213540	19.30%	2.460%
35	15.857	2183	2188	2194	rBV3	7156	11095	1.00%	0.128%
36	15.974	2205	2208	2212	rVV3	795	1115	0.10%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
 Data File : BM042797.D
 Acq On : 16 Nov 2023 08:55
 Operator : MA/JU
 Sample : 05105-17
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0013

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

37	16.415	2277	2283	2287	rBV4	3943	6252	0.57%	0.072%
38	16.751	2332	2340	2343	rBV4	655	1462	0.13%	0.017%
39	16.880	2358	2362	2365	rBV3	1473	1754	0.16%	0.020%
40	17.033	2382	2388	2390	rVB3	1063	1510	0.14%	0.017%
41	17.139	2403	2406	2409	rVB2	954	1345	0.12%	0.015%
42	17.174	2409	2412	2416	rBV2	892	1668	0.15%	0.019%
43	17.233	2416	2422	2433	rBV	279333	419617	37.93%	4.834%
44	17.333	2433	2439	2454	rBV	485037	721518	65.22%	8.312%
45	18.086	2563	2567	2573	rBV5	12112	21239	1.92%	0.245%
46	18.192	2583	2585	2588	rVB4	1270	1246	0.11%	0.014%
47	18.662	2661	2665	2666	rVB4	1572	1591	0.14%	0.018%
48	18.680	2666	2668	2672	rBV3	1181	1199	0.11%	0.014%
49	18.821	2689	2692	2694	rBV4	1921	2067	0.19%	0.024%
50	19.056	2730	2732	2733	rBV2	1733	1341	0.12%	0.015%
51	19.186	2751	2754	2759	rVB5	4594	5723	0.52%	0.066%
52	19.262	2763	2767	2771	rBV3	5105	8284	0.75%	0.095%
53	19.374	2782	2786	2791	rBV7	4047	7730	0.70%	0.089%
54	19.503	2805	2808	2813	rBV4	2680	4109	0.37%	0.047%
55	19.627	2822	2829	2840	rBV	741618	983905	88.93%	11.335%
56	20.221	2928	2930	2931	rBV2	2056	1340	0.12%	0.015%
57	20.639	2999	3001	3006	rBV4	3105	2509	0.23%	0.029%
58	21.086	3074	3077	3081	rBV4	9711	14021	1.27%	0.162%
59	21.415	3129	3133	3145	rBV	325852	483825	43.73%	5.574%
60	23.621	3501	3508	3523	rBV2	547851	1106350	100.00%	12.746%
61	23.780	3528	3535	3544	rVV	268897	552393	49.93%	6.364%




Sum of corrected areas: 8680034

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042797.D
Acq On : 16 Nov 2023 08:55
Operator : MA/JU
Sample : 05105-17
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0013

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

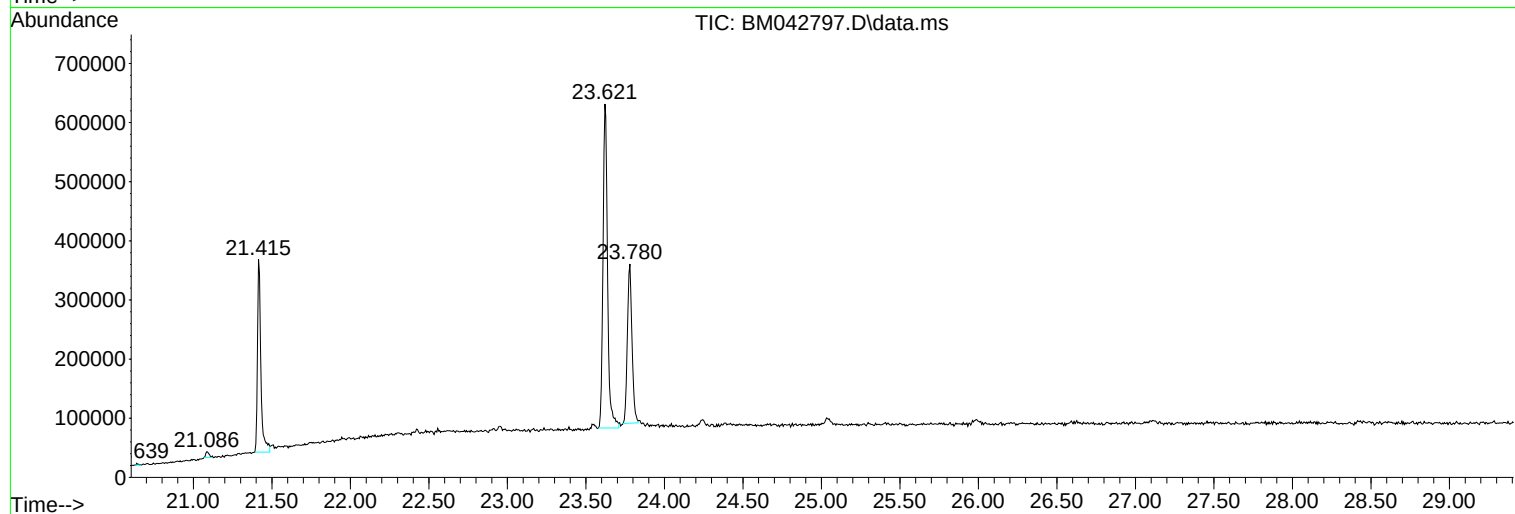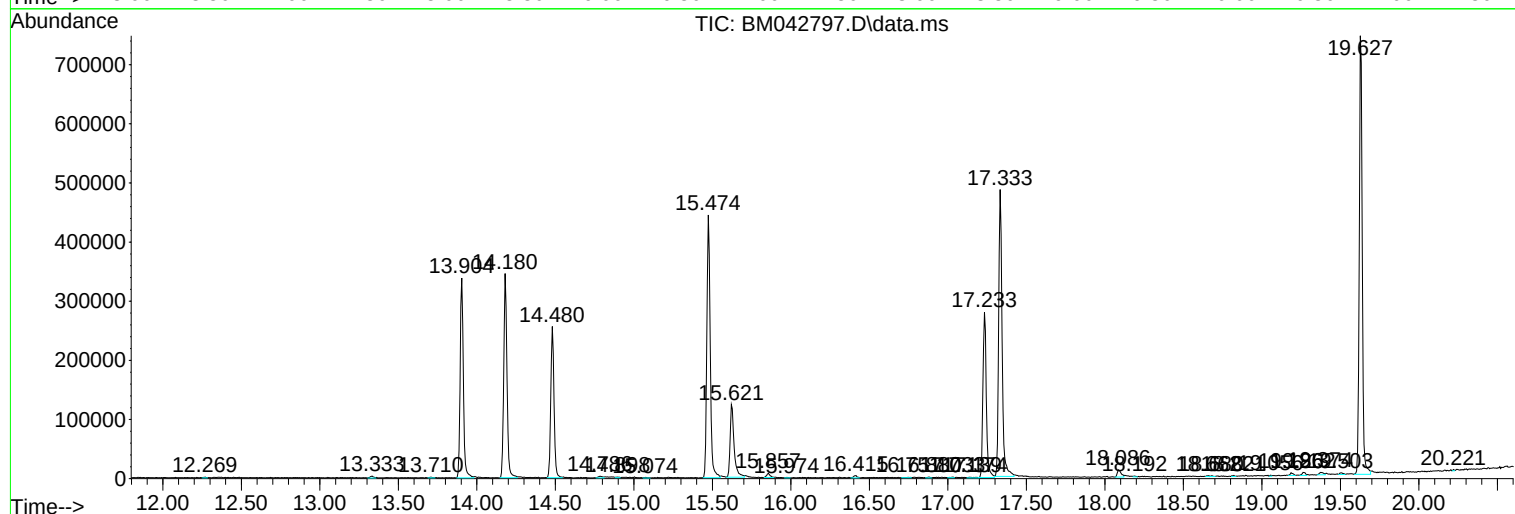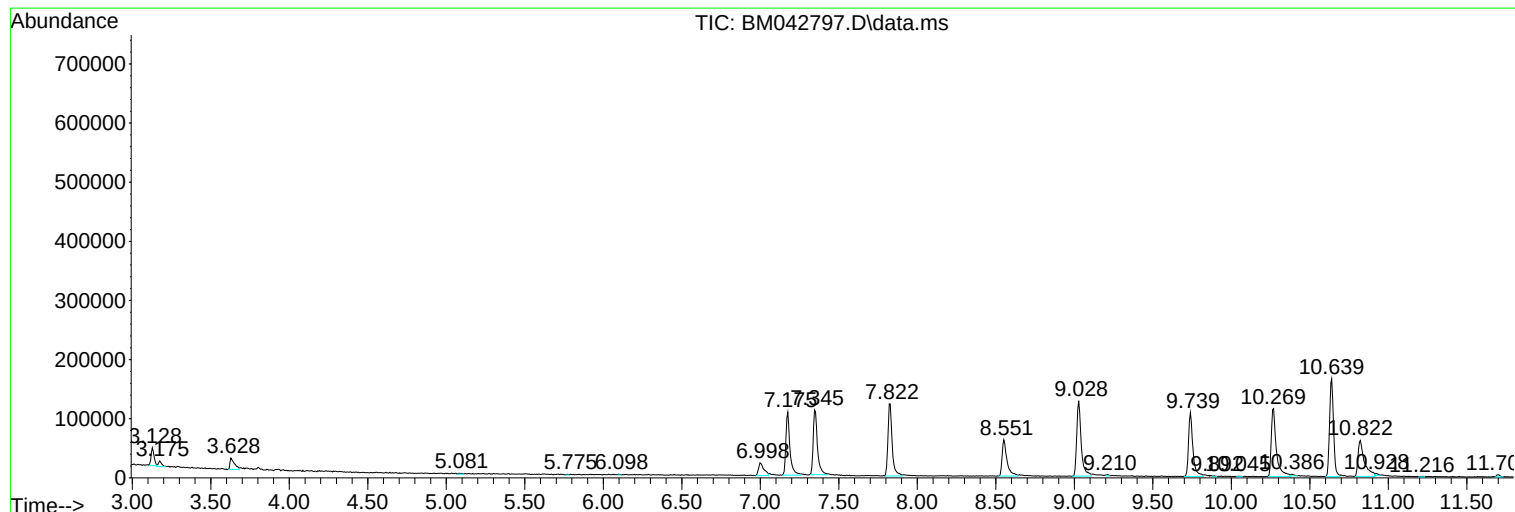

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042797.D
Acq On : 16 Nov 2023 08:55
Operator : MA/JU
Sample : 05105-17
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0013

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042797.D
Acq On : 16 Nov 2023 08:55
Operator : MA/JU
Sample : 05105-17
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0013

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc