

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
 Data File : BM042798.D
 Acq On : 16 Nov 2023 09:31
 Operator : MA/JU
 Sample : 05259-01
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YCGA9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM042798.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	29	32	40	rVB4	8270	13776	1.48%	0.168%
2	3.622	105	108	122	rBV	30600	59833	6.42%	0.729%
3	3.922	157	159	164	rVB4	3652	3821	0.41%	0.047%
4	4.463	250	251	253	rBV	1506	1360	0.15%	0.017%
5	4.828	311	313	315	rBV3	1173	959	0.10%	0.012%
6	5.457	418	420	422	rVB3	1263	1014	0.11%	0.012%
7	5.534	431	433	434	rBV2	1513	1021	0.11%	0.012%
8	6.163	536	540	542	rVB4	973	1054	0.11%	0.013%
9	6.593	611	613	617	rVB4	878	991	0.11%	0.012%
10	6.710	630	633	636	rVB3	977	1015	0.11%	0.012%
11	7.004	678	683	695	rVV4	15525	42202	4.53%	0.514%
12	7.104	697	700	703	rVB5	972	1255	0.13%	0.015%
13	7.175	706	712	725	rBV	110708	202802	21.75%	2.472%
14	7.345	736	741	757	rBV	111316	208342	22.35%	2.539%
15	7.498	764	767	769	rVB4	1528	1787	0.19%	0.022%
16	7.516	769	770	772	rBV2	1777	1055	0.11%	0.013%
17	7.604	783	785	788	rBV3	670	1008	0.11%	0.012%
18	7.769	809	813	816	rBV4	610	1186	0.13%	0.014%
19	7.822	816	822	835	rBV	112059	205974	22.09%	2.511%
20	8.551	940	946	960	rBV2	56108	122639	13.15%	1.495%
21	8.763	980	982	986	rVB3	869	1209	0.13%	0.015%
22	8.845	992	996	999	rBV4	734	980	0.11%	0.012%
23	9.028	1020	1027	1038	rBV	138309	261302	28.03%	3.185%
24	9.322	1075	1077	1079	rVB2	1052	996	0.11%	0.012%
25	9.528	1109	1112	1117	rVB4	733	1187	0.13%	0.014%
26	9.739	1142	1148	1160	rBV	116099	214910	23.05%	2.619%
27	9.863	1168	1169	1172	rVB3	1854	1537	0.16%	0.019%
28	9.892	1172	1174	1179	rVB4	1144	1660	0.18%	0.020%
29	10.157	1215	1219	1221	rBV2	698	934	0.10%	0.011%
30	10.263	1231	1237	1261	rBV2	121864	273296	29.31%	3.331%
31	10.475	1271	1273	1276	rVB4	1297	1139	0.12%	0.014%
32	10.639	1294	1301	1310	rBV	150409	263242	28.24%	3.209%
33	10.816	1325	1331	1350	rBV2	82640	222637	23.88%	2.714%
34	11.698	1478	1481	1487	rVB2	3236	4875	0.52%	0.059%
35	11.969	1525	1527	1532	rVB3	794	1052	0.11%	0.013%
36	13.057	1710	1712	1718	rVB3	1076	1459	0.16%	0.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
 Data File : BM042798.D
 Acq On : 16 Nov 2023 09:31
 Operator : MA/JU
 Sample : 05259-01
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YCGA9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

37	13.322	1754	1757	1759	rBV4	1578	1432	0.15%	0.017%
38	13.674	1813	1817	1820	rBV2	753	976	0.10%	0.012%
39	13.704	1820	1822	1826	rVB5	1550	2027	0.22%	0.025%
40	13.904	1850	1856	1867	rVV	327995	474671	50.91%	5.786%
41	14.004	1871	1873	1878	rVB3	1078	1183	0.13%	0.014%
42	14.180	1897	1903	1919	rBV	349151	511768	54.89%	6.238%
43	14.480	1948	1954	1968	rBV2	229174	333619	35.78%	4.066%
44	15.216	2077	2079	2083	rVB3	1488	1594	0.17%	0.019%
45	15.304	2092	2094	2098	rVB5	1410	1502	0.16%	0.018%
46	15.392	2106	2109	2111	rBV2	912	1062	0.11%	0.013%
47	15.474	2117	2123	2143	rBV	439717	649262	69.64%	7.914%
48	15.621	2143	2148	2164	rVV	96155	185455	19.89%	2.260%
49	15.721	2164	2165	2168	rVV	3330	2724	0.29%	0.033%
50	15.757	2168	2171	2178	rVB2	2460	3995	0.43%	0.049%
51	15.804	2178	2179	2181	rBV	1187	976	0.10%	0.012%
52	16.104	2224	2230	2232	rVB2	626	977	0.10%	0.012%
53	16.345	2268	2271	2276	rVB5	2411	3580	0.38%	0.044%
54	16.715	2331	2334	2337	rBV3	863	1205	0.13%	0.015%
55	17.104	2397	2400	2403	rBV2	1109	1132	0.12%	0.014%
56	17.233	2416	2422	2433	rBV	274625	387599	41.57%	4.724%
57	17.333	2433	2439	2458	rVV	469772	701306	75.22%	8.548%
58	17.457	2458	2460	2465	rVB4	1982	2276	0.24%	0.028%
59	17.674	2491	2497	2499	rBV3	751	1657	0.18%	0.020%
60	18.098	2563	2569	2570	rBV4	4544	5605	0.60%	0.068%
61	18.180	2578	2583	2587	rVB5	2692	4108	0.44%	0.050%
62	18.327	2605	2608	2610	rBV3	1219	1310	0.14%	0.016%
63	18.351	2610	2612	2614	rBV2	1277	1374	0.15%	0.017%
64	18.609	2653	2656	2659	rBV3	1097	1016	0.11%	0.012%
65	18.727	2675	2676	2679	rBV3	947	939	0.10%	0.011%
66	18.821	2689	2692	2695	rVV4	675	1053	0.11%	0.013%
67	18.851	2695	2697	2701	rBV4	940	1225	0.13%	0.015%
68	19.009	2720	2724	2725	rBV3	1375	1325	0.14%	0.016%
69	19.074	2733	2735	2737	rBV2	1283	1318	0.14%	0.016%
70	19.168	2748	2751	2752	rBV2	1870	2033	0.22%	0.025%
71	19.192	2752	2755	2759	rVV3	5228	6844	0.73%	0.083%
72	19.262	2763	2767	2771	rVV5	5089	6990	0.75%	0.085%
73	19.374	2783	2786	2789	rBV5	3865	4837	0.52%	0.059%
74	19.509	2806	2809	2811	rBV3	3126	3185	0.34%	0.039%
75	19.627	2824	2829	2843	rBV	661747	880697	94.46%	10.735%
76	19.851	2863	2867	2869	rBV4	1857	2578	0.28%	0.031%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042798.D
Acq On : 16 Nov 2023 09:31
Operator : MA/JU
Sample : 05259-01
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YCGA9

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Title : SVOA CALIBRATION

77	19.886	2872	2873	2875	rBV2	2002	1049	0.11%	0.013%
78	19.992	2889	2891	2892	rBV2	1815	1670	0.18%	0.020%
79	20.180	2921	2923	2924	rBV2	2259	1641	0.18%	0.020%
80	20.545	2984	2985	2986	rBV	3557	1987	0.21%	0.024%
81	21.415	3129	3133	3145	rBV	294227	442831	47.50%	5.398%
82	23.621	3502	3508	3522	rBV2	467423	932303	100.00%	11.364%
83	23.780	3529	3535	3545	rVB	242755	498903	53.51%	6.081%




Sum of corrected areas: 8204308

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042798.D
Acq On : 16 Nov 2023 09:31
Operator : MA/JU
Sample : 05259-01
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YCGA9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

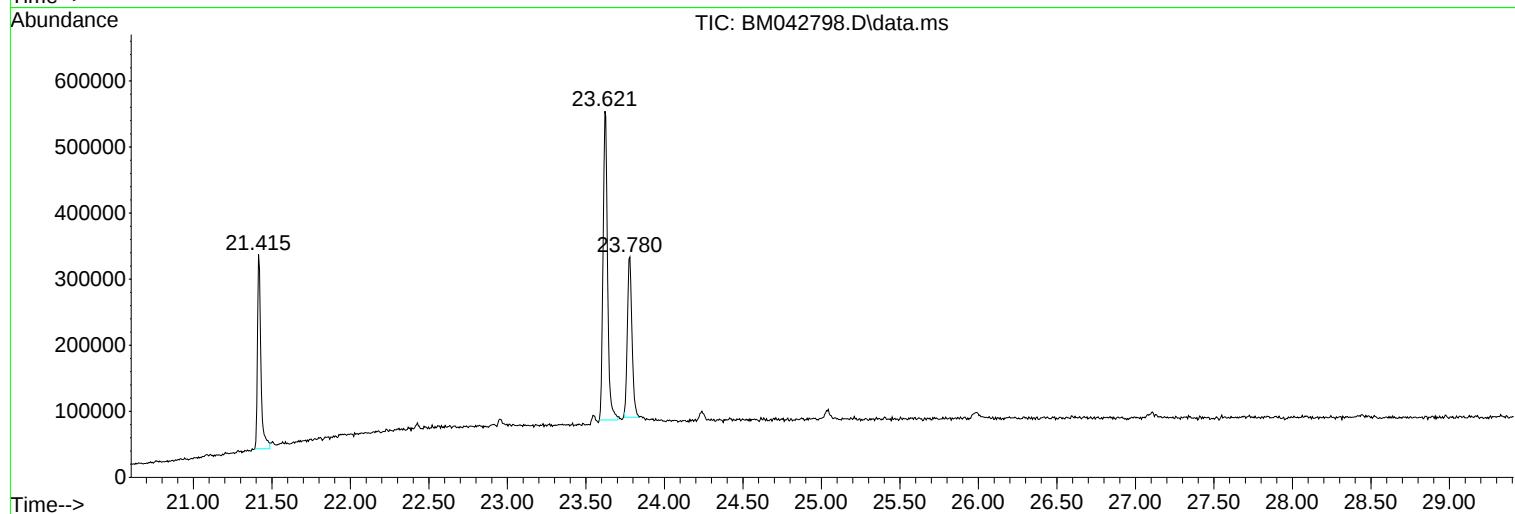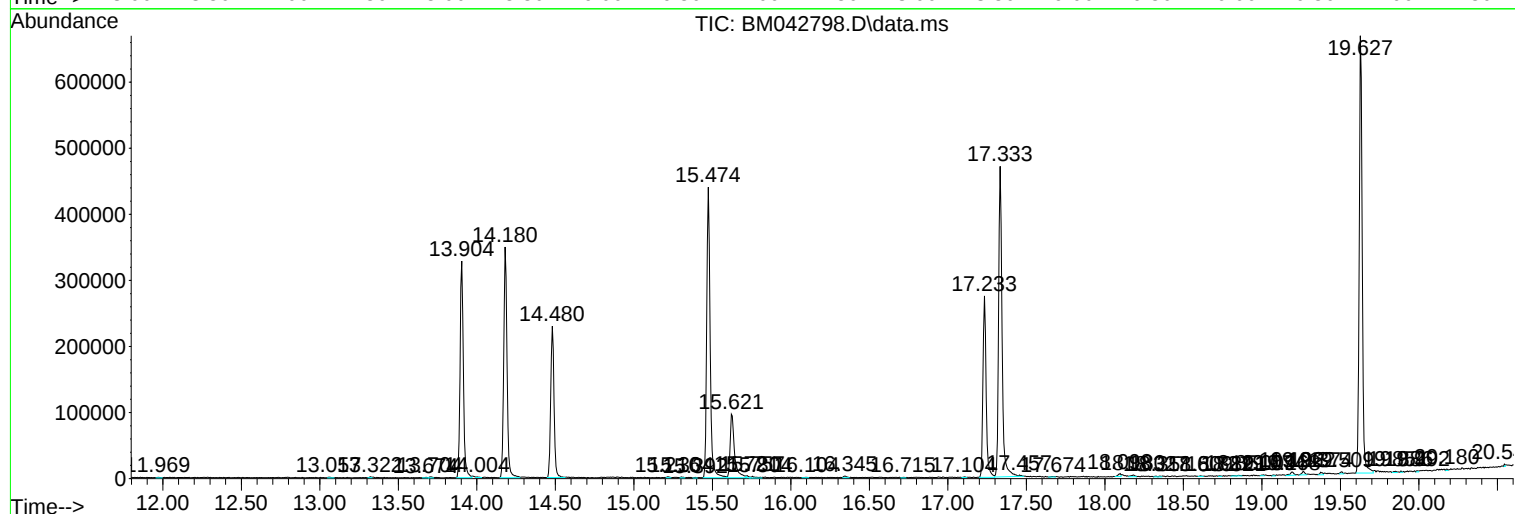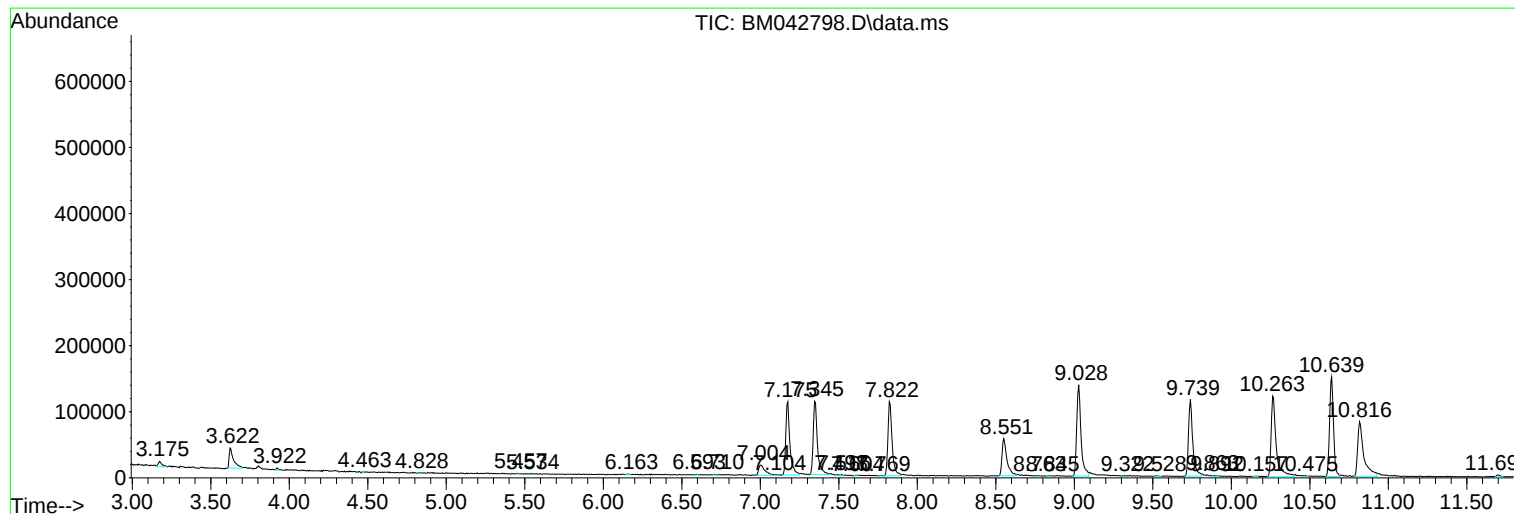

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042798.D
Acq On : 16 Nov 2023 09:31
Operator : MA/JU
Sample : 05259-01
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YCGA9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042798.D
Acq On : 16 Nov 2023 09:31
Operator : MA/JU
Sample : 05259-01
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YCGA9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc