

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
 Data File : BM042805.D
 Acq On : 16 Nov 2023 13:43
 Operator : MA/JU
 Sample : PB156780BL
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK780

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM042805.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	29	32	38	rVB	15115	20650	2.24%	0.206%
2	3.616	103	107	123	rBV	146674	253949	27.52%	2.534%
3	4.546	263	265	268	rVB4	1704	1402	0.15%	0.014%
4	4.758	299	301	302	rBV2	1279	1005	0.11%	0.010%
5	5.675	455	457	459	rBV2	1405	1263	0.14%	0.013%
6	6.134	533	535	539	rVV3	991	1350	0.15%	0.013%
7	6.410	580	582	586	rBV4	729	1181	0.13%	0.012%
8	6.563	605	608	610	rBV3	1041	1412	0.15%	0.014%
9	6.681	627	628	633	rVB3	1750	1717	0.19%	0.017%
10	6.881	658	662	665	rBV4	678	1104	0.12%	0.011%
11	6.993	675	681	701	rBV	158007	321275	34.81%	3.206%
12	7.175	706	712	728	rVB	132352	236287	25.60%	2.358%
13	7.346	735	741	756	rBV	182684	318062	34.46%	3.174%
14	7.516	769	770	776	rVB5	1097	1296	0.14%	0.013%
15	7.822	816	822	839	rBV	146516	264221	28.63%	2.636%
16	8.546	937	945	966	rBV	171531	346290	37.52%	3.455%
17	8.710	971	973	974	rVV2	1895	1418	0.15%	0.014%
18	8.834	992	994	996	rBV3	937	969	0.10%	0.010%
19	8.951	1012	1014	1017	rVB3	1525	1545	0.17%	0.015%
20	8.975	1017	1018	1020	rBV2	1005	986	0.11%	0.010%
21	9.028	1020	1027	1038	rBV	158399	298750	32.37%	2.981%
22	9.493	1105	1106	1110	rBV2	1020	951	0.10%	0.009%
23	9.740	1141	1148	1167	rBV	133882	264256	28.63%	2.637%
24	9.857	1167	1168	1174	rVV6	1642	2376	0.26%	0.024%
25	9.928	1178	1180	1183	rVB3	1509	1069	0.12%	0.011%
26	10.075	1201	1205	1208	rVB4	760	1132	0.12%	0.011%
27	10.263	1231	1237	1255	rBV2	164842	337048	36.52%	3.363%
28	10.416	1260	1263	1266	rVB4	1282	1868	0.20%	0.019%
29	10.504	1276	1278	1281	rVB4	951	1030	0.11%	0.010%
30	10.634	1293	1300	1317	rBV	191659	338565	36.68%	3.378%
31	10.816	1323	1331	1359	rBV	121958	326337	35.36%	3.256%
32	11.410	1430	1432	1435	rVB2	1002	1023	0.11%	0.010%
33	11.451	1435	1439	1442	rBV3	958	1564	0.17%	0.016%
34	11.645	1471	1472	1475	rBV3	986	933	0.10%	0.009%
35	11.951	1518	1524	1526	rBV3	656	1054	0.11%	0.011%
36	12.657	1640	1644	1647	rBV3	617	959	0.10%	0.010%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042805.D
Acq On : 16 Nov 2023 13:43
Operator : MA/JU
Sample : PB156780BL
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK780

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Title : SVOA CALIBRATION

37	12.686	1647	1649	1654	rVB3	681	1043	0.11%	0.010%
38	13.333	1755	1759	1766	rVB4	1949	3289	0.36%	0.033%
39	13.904	1850	1856	1867	rBV	354921	513695	55.66%	5.126%
40	14.180	1897	1903	1918	rBV	399275	578655	62.70%	5.774%
41	14.280	1918	1920	1922	rVV3	1329	1044	0.11%	0.010%
42	14.480	1948	1954	1964	rBV	290676	418003	45.29%	4.171%
43	14.551	1964	1966	1970	rVB3	853	1164	0.13%	0.012%
44	14.751	1994	2000	2015	rBV4	28069	112297	12.17%	1.120%
45	14.963	2034	2036	2039	rVV4	1335	1374	0.15%	0.014%
46	14.986	2039	2040	2044	rVV4	1499	1454	0.16%	0.015%
47	15.269	2085	2088	2091	rBV2	1066	1215	0.13%	0.012%
48	15.475	2117	2123	2139	rBV	476367	702187	76.08%	7.006%
49	15.622	2143	2148	2163	rBV	105512	191162	20.71%	1.907%
50	15.775	2172	2174	2177	rVB3	1030	1049	0.11%	0.010%
51	15.845	2182	2186	2189	rVB3	782	949	0.10%	0.009%
52	15.880	2189	2192	2195	rBV3	792	945	0.10%	0.009%
53	16.057	2219	2222	2226	rVV3	1049	1462	0.16%	0.015%
54	16.092	2226	2228	2232	rVV2	892	924	0.10%	0.009%
55	16.357	2270	2273	2276	rBV3	611	959	0.10%	0.010%
56	16.516	2298	2300	2303	rBV3	674	1004	0.11%	0.010%
57	17.233	2416	2422	2433	rBV	323670	468320	50.74%	4.673%
58	17.333	2433	2439	2461	rVV	492341	735128	79.65%	7.335%
59	17.469	2461	2462	2466	rVB2	1636	1295	0.14%	0.013%
60	17.569	2478	2479	2484	rVB3	1133	1202	0.13%	0.012%
61	17.610	2484	2486	2491	rBV4	653	931	0.10%	0.009%
62	17.774	2512	2514	2520	rVB5	999	1431	0.16%	0.014%
63	17.921	2538	2539	2542	rBV3	1508	1190	0.13%	0.012%
64	18.027	2552	2557	2560	rBV3	1293	2199	0.24%	0.022%
65	18.257	2595	2596	2600	rVB4	1121	975	0.11%	0.010%
66	18.316	2603	2606	2607	rBV	1129	1026	0.11%	0.010%
67	18.463	2630	2631	2635	rBV2	1311	1333	0.14%	0.013%
68	18.704	2669	2672	2673	rBV2	1073	1235	0.13%	0.012%
69	18.733	2675	2677	2680	rBV3	1244	1608	0.17%	0.016%
70	18.815	2686	2691	2692	rBV5	1073	1691	0.18%	0.017%
71	18.839	2692	2695	2698	rBV4	1010	1433	0.16%	0.014%
72	18.874	2699	2701	2704	rVV3	1198	1052	0.11%	0.010%
73	18.921	2708	2709	2712	rBV3	1145	1186	0.13%	0.012%
74	19.133	2743	2745	2748	rVV4	1106	1136	0.12%	0.011%
75	19.198	2751	2756	2762	rVV6	4266	6950	0.75%	0.069%
76	19.268	2765	2768	2772	rBV3	4056	4461	0.48%	0.045%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042805.D
Acq On : 16 Nov 2023 13:43
Operator : MA/JU
Sample : PB156780BL
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK780

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Title : SVOA CALIBRATION

77	19.392	2784	2789	2791	rVV5	1388	2244	0.24%	0.022%
78	19.627	2824	2829	2841	rBV	614004	870786	94.35%	8.689%
79	20.151	2916	2918	2919	rBV2	2038	1372	0.15%	0.014%
80	21.421	3129	3134	3146	rBV	324995	503037	54.50%	5.019%
81	23.627	3502	3509	3521	rBV	451579	922935	100.00%	9.209%
82	23.780	3528	3535	3549	rBV	283635	595954	64.57%	5.946%




Sum of corrected areas: 10022281

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042805.D
Acq On : 16 Nov 2023 13:43
Operator : MA/JU
Sample : PB156780BL
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK780

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

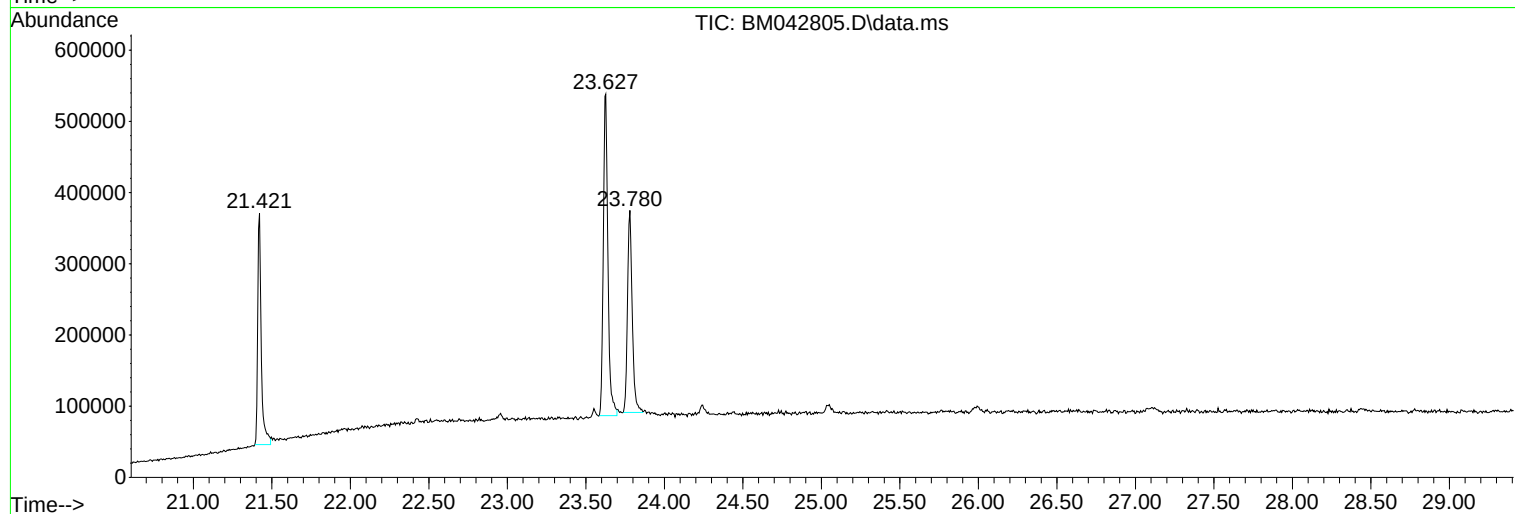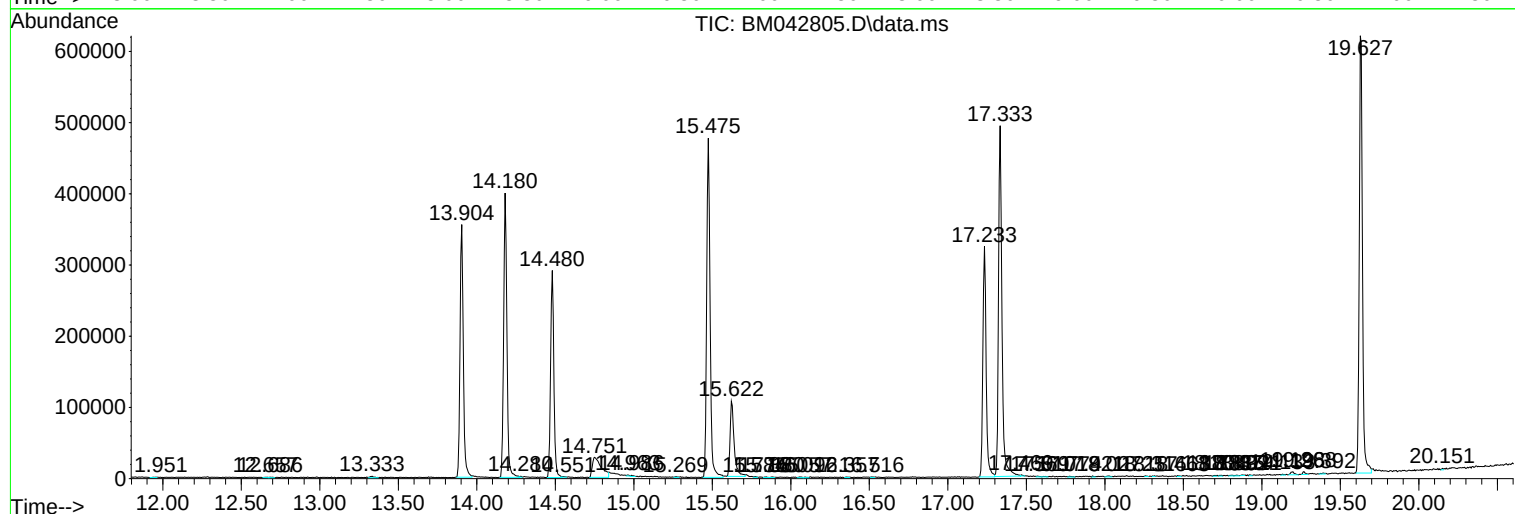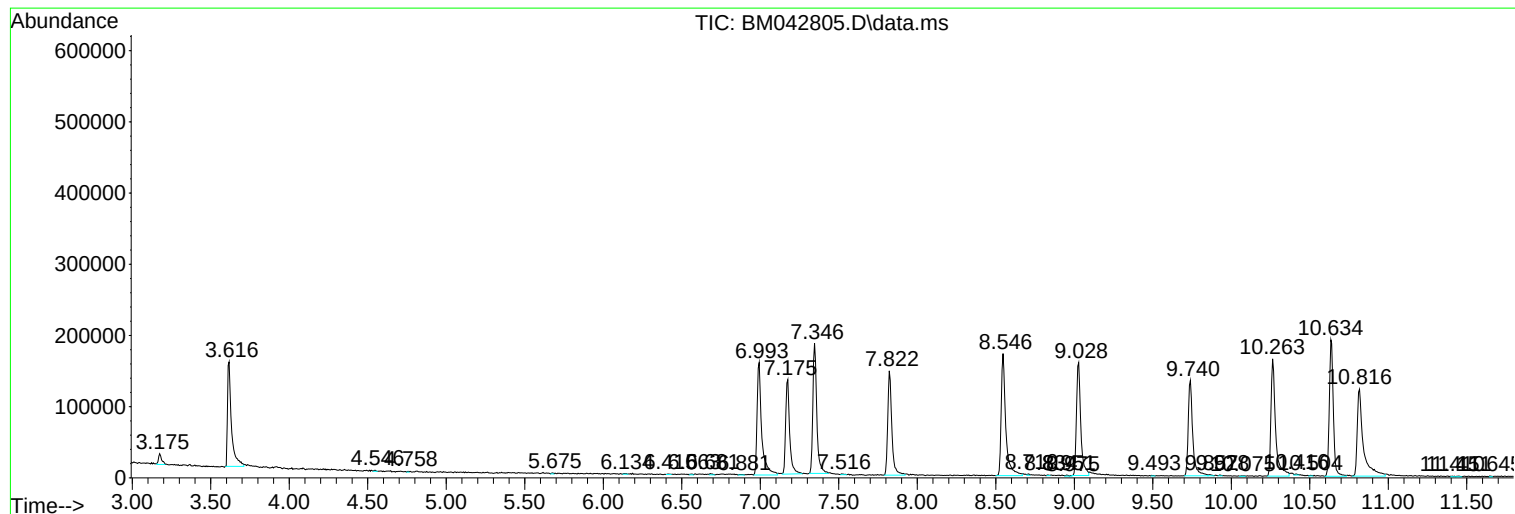

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042805.D
Acq On : 16 Nov 2023 13:43
Operator : MA/JU
Sample : PB156780BL
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK780

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042805.D
Acq On : 16 Nov 2023 13:43
Operator : MA/JU
Sample : PB156780BL
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK780

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc