

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
 Data File : BM042808.D
 Acq On : 16 Nov 2023 16:08
 Operator : MA/JU
 Sample : 05105-06
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0008

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM042808.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	30	32	37	rVB2	7869	9485	0.73%	0.094%
2	3.628	106	109	119	rBV	23443	48313	3.70%	0.481%
3	3.798	136	138	145	rVB5	4646	7210	0.55%	0.072%
4	3.922	157	159	163	rBV5	2393	2304	0.18%	0.023%
5	6.604	612	615	617	rBV3	1420	1753	0.13%	0.017%
6	6.739	636	638	641	rBV3	1190	1351	0.10%	0.013%
7	6.998	677	682	695	rBV2	31767	75651	5.79%	0.753%
8	7.175	706	712	727	rBV	127461	232501	17.80%	2.314%
9	7.345	735	741	756	rBV	138315	251344	19.24%	2.502%
10	7.528	771	772	777	rVB4	1671	1804	0.14%	0.018%
11	7.569	777	779	785	rVV3	1017	1365	0.10%	0.014%
12	7.822	816	822	836	rBV	137122	257802	19.73%	2.566%
13	7.910	836	837	841	rVV4	2871	3470	0.27%	0.035%
14	7.963	844	846	851	rVB4	1156	1796	0.14%	0.018%
15	8.545	940	945	960	rBV2	78518	172324	13.19%	1.715%
16	8.686	967	969	976	rVB6	2036	3824	0.29%	0.038%
17	8.933	1006	1011	1017	rBV2	11089	19118	1.46%	0.190%
18	9.028	1020	1027	1041	rBV	160364	309389	23.68%	3.080%
19	9.175	1051	1052	1056	rVB3	1655	1492	0.11%	0.015%
20	9.739	1142	1148	1160	rBV2	94811	181375	13.88%	1.805%
21	10.263	1231	1237	1257	rBV	142604	306724	23.48%	3.053%
22	10.639	1292	1301	1313	rBV	184009	327267	25.05%	3.258%
23	10.816	1325	1331	1346	rBV	104997	253949	19.44%	2.528%
24	11.604	1460	1465	1468	rBV3	872	1510	0.12%	0.015%
25	12.251	1573	1575	1580	rVB5	1103	1841	0.14%	0.018%
26	13.057	1709	1712	1715	rBV4	938	1369	0.10%	0.014%
27	13.327	1754	1758	1765	rVB2	4047	5476	0.42%	0.055%
28	13.904	1850	1856	1870	rBV	383269	541727	41.47%	5.393%
29	14.180	1897	1903	1914	rBV2	420311	584725	44.76%	5.821%
30	14.480	1945	1954	1970	rBV	288122	426122	32.62%	4.242%
31	14.804	2004	2009	2012	rBV4	1349	2699	0.21%	0.027%
32	15.151	2063	2068	2071	rBV3	1603	2910	0.22%	0.029%
33	15.292	2089	2092	2097	rVB5	888	1626	0.12%	0.016%
34	15.474	2117	2123	2139	rBV	527035	756207	57.89%	7.528%
35	15.586	2141	2142	2146	rVV2	1950	2669	0.20%	0.027%
36	15.633	2146	2150	2160	rVV5	15252	34414	2.63%	0.343%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
 Data File : BM042808.D
 Acq On : 16 Nov 2023 16:08
 Operator : MA/JU
 Sample : 05105-06
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0008

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

37	15.733	2163	2167	2170	rVB5	3770	5500	0.42%	0.055%
38	16.515	2294	2300	2303	rBV4	1047	1630	0.12%	0.016%
39	16.868	2354	2360	2361	rBV4	827	1359	0.10%	0.014%
40	17.233	2416	2422	2433	rBV	337530	482236	36.92%	4.800%
41	17.333	2433	2439	2458	rVV	628071	919158	70.36%	9.150%
42	17.480	2462	2464	2470	rVB5	1802	2958	0.23%	0.029%
43	17.862	2525	2529	2535	rVB2	31790	38160	2.92%	0.380%
44	18.350	2610	2612	2615	rVV4	1810	1743	0.13%	0.017%
45	18.603	2651	2655	2657	rVB4	1356	1818	0.14%	0.018%
46	19.145	2745	2747	2750	rBV3	1210	1623	0.12%	0.016%
47	19.192	2752	2755	2759	rBV3	5285	8128	0.62%	0.081%
48	19.262	2764	2767	2773	rVV4	4156	6479	0.50%	0.064%
49	19.627	2824	2829	2847	rBV	884627	1185754	90.77%	11.804%
50	19.880	2870	2872	2873	rBV2	2147	1456	0.11%	0.014%
51	20.056	2898	2902	2903	rBV3	2010	2532	0.19%	0.025%
52	21.415	3128	3133	3145	rBV	369513	573979	43.94%	5.714%
53	23.621	3502	3508	3527	rVB2	667539	1306340	100.00%	13.004%
54	23.780	3528	3535	3545	rBV	321844	670015	51.29%	6.670%




Sum of corrected areas: 10045774

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042808.D
Acq On : 16 Nov 2023 16:08
Operator : MA/JU
Sample : 05105-06
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0008

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

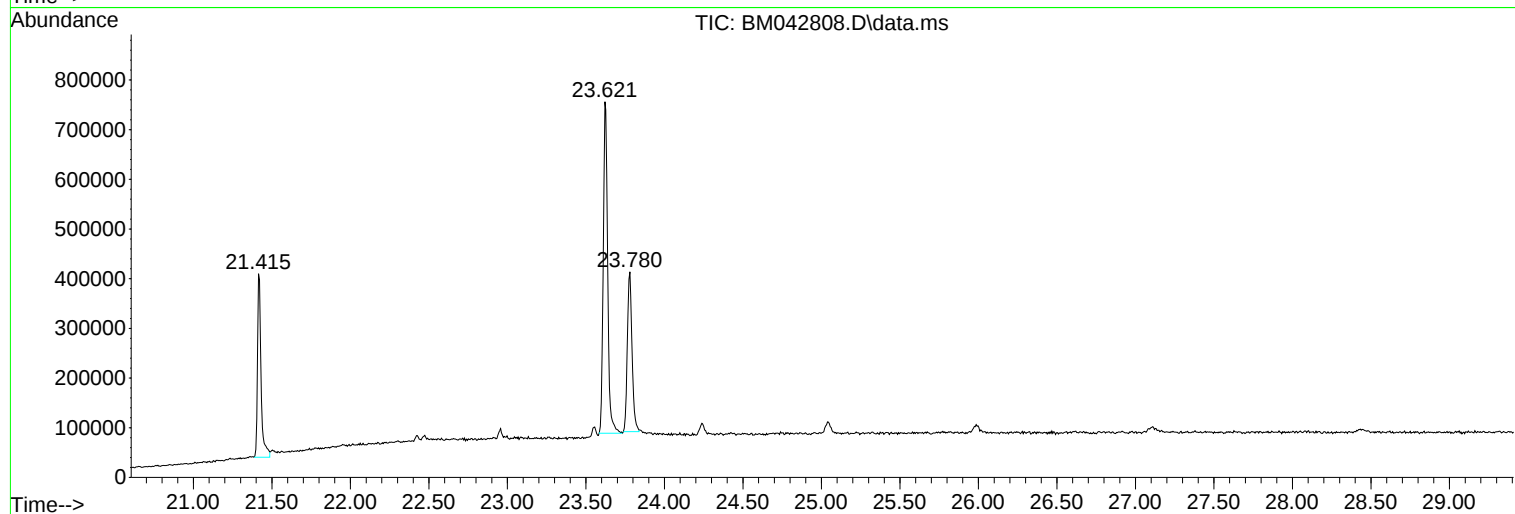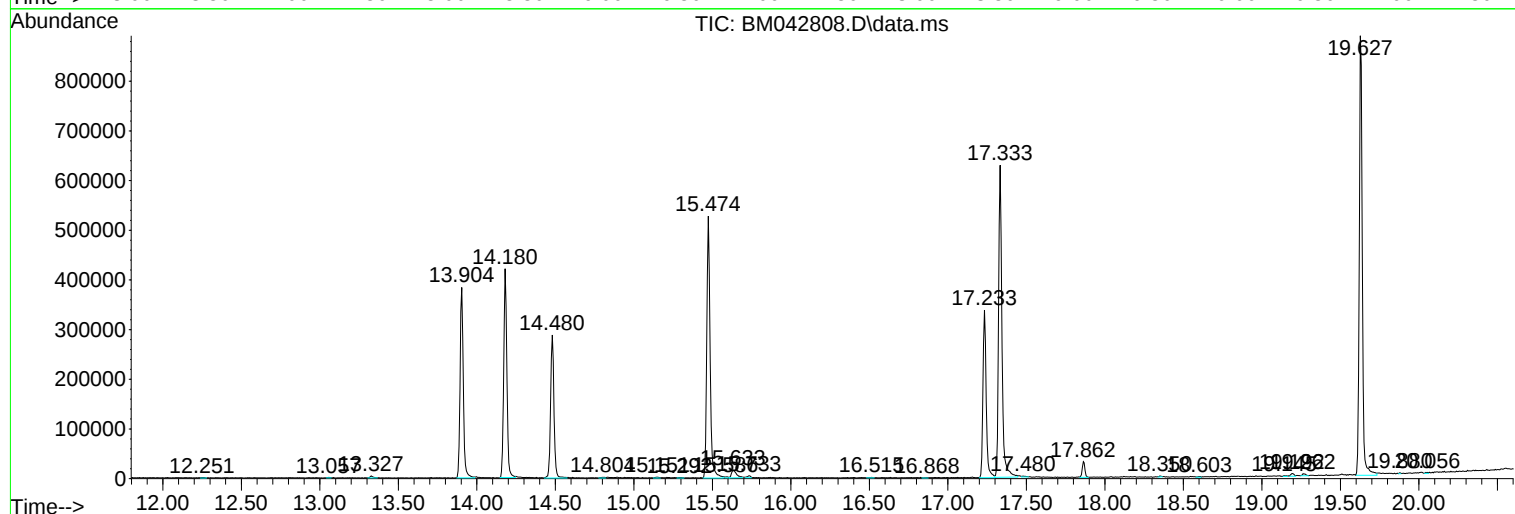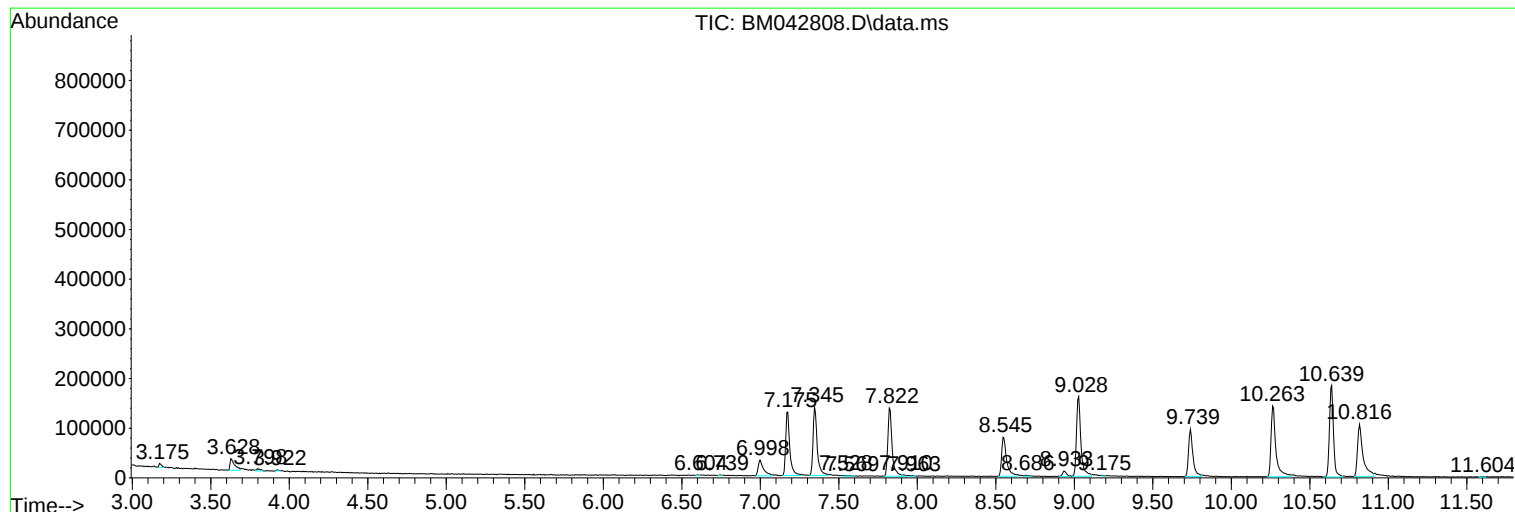

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042808.D
Acq On : 16 Nov 2023 16:08
Operator : MA/JU
Sample : 05105-06
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0008

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042808.D
Acq On : 16 Nov 2023 16:08
Operator : MA/JU
Sample : 05105-06
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0008

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc