

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
 Data File : BM042810.D
 Acq On : 16 Nov 2023 17:20
 Operator : MA/JU
 Sample : 05259-06
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YCG95

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM042810.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	29	32	37	rVB3	7341	10052	0.88%	0.108%
2	3.622	105	108	120	rBV	39835	74581	6.50%	0.800%
3	3.799	135	138	142	rVB5	3396	4677	0.41%	0.050%
4	3.922	155	159	164	rBV5	3369	5765	0.50%	0.062%
5	4.863	318	319	322	rBV2	1289	1258	0.11%	0.013%
6	4.928	328	330	333	rVB4	1263	1200	0.10%	0.013%
7	5.187	372	374	377	rBV4	1752	1570	0.14%	0.017%
8	5.687	457	459	462	rVB4	1693	1400	0.12%	0.015%
9	6.251	554	555	561	rBV5	914	1596	0.14%	0.017%
10	6.322	565	567	570	rVB4	1478	1442	0.13%	0.015%
11	6.769	640	643	646	rBV3	1553	1521	0.13%	0.016%
12	6.998	677	682	697	rBV2	18504	48964	4.27%	0.525%
13	7.175	706	712	723	rBV	121868	218900	19.07%	2.349%
14	7.346	735	741	762	rVB	127070	233045	20.30%	2.501%
15	7.822	816	822	839	rBV	126949	232508	20.26%	2.495%
16	8.551	940	946	966	rBV	63405	141551	12.33%	1.519%
17	9.028	1020	1027	1047	rBV	145984	299456	26.09%	3.213%
18	9.210	1056	1058	1064	rVB5	2137	3253	0.28%	0.035%
19	9.292	1070	1072	1078	rVB5	1288	1902	0.17%	0.020%
20	9.739	1141	1148	1158	rBV	126655	238267	20.76%	2.557%
21	9.881	1171	1172	1178	rVB5	1082	1354	0.12%	0.015%
22	10.116	1209	1212	1215	rBV3	720	1153	0.10%	0.012%
23	10.263	1232	1237	1253	rBV	137560	289917	25.26%	3.111%
24	10.634	1294	1300	1316	rBV	166834	291212	25.37%	3.125%
25	10.816	1325	1331	1351	rBV	96643	248372	21.64%	2.665%
26	11.704	1475	1482	1485	rBV2	5482	8766	0.76%	0.094%
27	12.269	1574	1578	1581	rBV4	849	1169	0.10%	0.013%
28	13.233	1737	1742	1748	rBV3	651	1472	0.13%	0.016%
29	13.328	1752	1758	1765	rVV2	3288	5348	0.47%	0.057%
30	13.586	1798	1802	1806	rBV4	772	1525	0.13%	0.016%
31	13.710	1817	1823	1825	rBV4	1962	2053	0.18%	0.022%
32	13.904	1850	1856	1867	rVV	362554	532906	46.43%	5.718%
33	13.980	1867	1869	1875	rVB4	1472	2251	0.20%	0.024%
34	14.180	1897	1903	1916	rBV	402081	581829	50.69%	6.243%
35	14.480	1948	1954	1967	rBV	249568	362405	31.57%	3.889%
36	14.792	2002	2007	2008	rBV4	1465	1697	0.15%	0.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
 Data File : BM042810.D
 Acq On : 16 Nov 2023 17:20
 Operator : MA/JU
 Sample : 05259-06
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YCG95

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

37	15.263	2085	2087	2091	rVV3	1253	1597	0.14%	0.017%
38	15.380	2103	2107	2111	rBV3	865	1947	0.17%	0.021%
39	15.474	2117	2123	2138	rBV	520034	752172	65.53%	8.071%
40	15.621	2143	2148	2162	rVV	129657	215117	18.74%	2.308%
41	16.398	2278	2280	2285	rBV3	863	1341	0.12%	0.014%
42	17.233	2416	2422	2433	rBV	284511	407142	35.47%	4.369%
43	17.333	2433	2439	2453	rVV	568067	833928	72.65%	8.949%
44	17.721	2502	2505	2507	rVB3	1355	1231	0.11%	0.013%
45	17.933	2539	2541	2545	rVB4	1226	1702	0.15%	0.018%
46	18.086	2563	2567	2570	rBV4	9127	13540	1.18%	0.145%
47	18.133	2574	2575	2578	rVV	2694	2221	0.19%	0.024%
48	18.162	2578	2580	2582	rVV2	1765	1812	0.16%	0.019%
49	18.180	2582	2583	2585	rVV2	1754	1195	0.10%	0.013%
50	18.345	2610	2611	2615	rVV3	1127	1184	0.10%	0.013%
51	18.386	2615	2618	2622	rVB4	1331	1816	0.16%	0.019%
52	18.521	2637	2641	2644	rBV4	932	1457	0.13%	0.016%
53	18.921	2706	2709	2711	rBV4	1228	1558	0.14%	0.017%
54	19.192	2751	2755	2759	rBV3	5979	7059	0.61%	0.076%
55	19.262	2763	2767	2773	rVV5	7228	10913	0.95%	0.117%
56	19.374	2782	2786	2790	rBV4	5871	9493	0.83%	0.102%
57	19.509	2806	2809	2813	rVB7	2520	3896	0.34%	0.042%
58	19.627	2823	2829	2844	rBV	810672	1062620	92.58%	11.403%
59	19.851	2865	2867	2870	rBV3	1955	2354	0.21%	0.025%
60	20.015	2893	2895	2899	rBV5	2932	3580	0.31%	0.038%
61	20.115	2910	2912	2914	rBV3	2140	1841	0.16%	0.020%
62	21.415	3128	3133	3143	rBV	300321	450162	39.22%	4.831%
63	23.621	3501	3508	3523	rBV	583668	1147834	100.00%	12.317%
64	23.780	3528	3535	3545	rVV	250692	521958	45.47%	5.601%



Sum of corrected areas: 9319007

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042810.D
Acq On : 16 Nov 2023 17:20
Operator : MA/JU
Sample : 05259-06
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YCG95

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

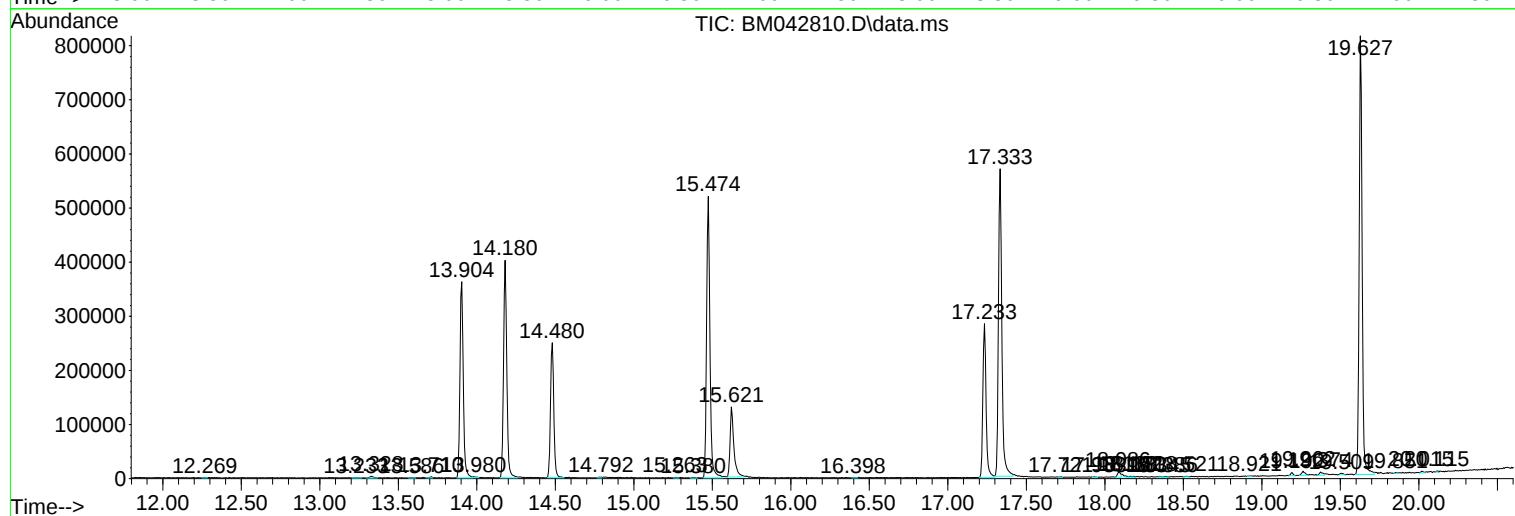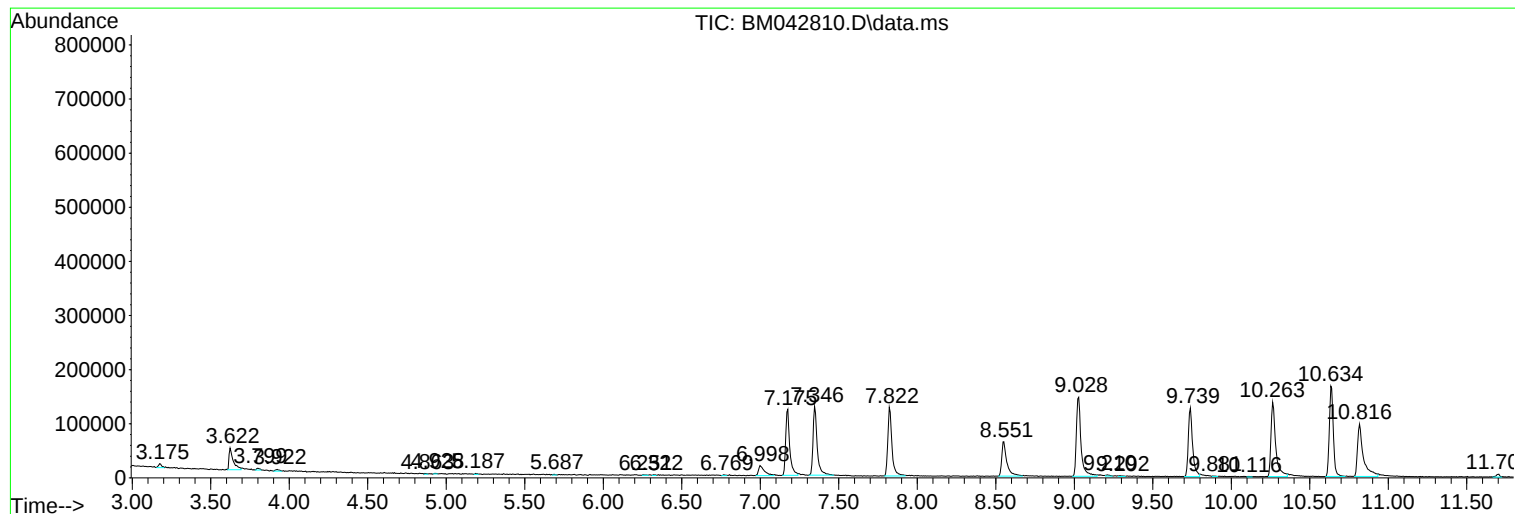

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042810.D
Acq On : 16 Nov 2023 17:20
Operator : MA/JU
Sample : 05259-06
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YCG95

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042810.D
Acq On : 16 Nov 2023 17:20
Operator : MA/JU
Sample : 05259-06
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YCG95

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------