

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
 Data File : BM042813.D
 Acq On : 16 Nov 2023 19:44
 Operator : MA/JU
 Sample : PB157007BL
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK007

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM042813.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	29	32	39	rVB2	14979	19691	2.20%	0.215%
2	3.611	103	106	126	rBV	132731	245867	27.50%	2.685%
3	4.463	249	251	252	rBV	1512	1061	0.12%	0.012%
4	4.757	299	301	302	rBV	1697	1052	0.12%	0.011%
5	5.134	364	365	368	rBV3	1247	940	0.11%	0.010%
6	5.234	380	382	385	rVB4	1292	909	0.10%	0.010%
7	5.769	471	473	477	rVB5	1336	1012	0.11%	0.011%
8	6.252	553	555	559	rVB4	1100	1217	0.14%	0.013%
9	6.281	559	560	565	rVB4	1159	1651	0.18%	0.018%
10	6.322	565	567	570	rBV4	1655	1814	0.20%	0.020%
11	6.634	617	620	621	rVB2	1314	981	0.11%	0.011%
12	6.704	630	632	637	rBV6	968	1728	0.19%	0.019%
13	6.740	637	638	641	rVB3	1558	1086	0.12%	0.012%
14	6.769	641	643	644	rBV	1282	1090	0.12%	0.012%
15	6.804	647	649	652	rVB2	1666	1496	0.17%	0.016%
16	6.851	655	657	661	rVB4	1250	1335	0.15%	0.015%
17	6.887	661	663	665	rBV3	1341	1079	0.12%	0.012%
18	6.987	675	680	698	rBV	138084	278238	31.12%	3.038%
19	7.169	706	711	727	rBV	119130	209883	23.48%	2.292%
20	7.346	734	741	759	rBV	165026	298051	33.34%	3.255%
21	7.822	816	822	831	rBV	118853	212474	23.77%	2.320%
22	8.457	929	930	934	rBV2	992	1349	0.15%	0.015%
23	8.545	939	945	967	rBV	151762	313136	35.03%	3.420%
24	8.857	995	998	1001	rBV4	949	1099	0.12%	0.012%
25	9.022	1020	1026	1043	rBV	140105	276592	30.94%	3.020%
26	9.687	1135	1139	1141	rBV4	1177	1536	0.17%	0.017%
27	9.740	1141	1148	1161	rBV	118787	237755	26.60%	2.596%
28	9.892	1170	1174	1176	rBV2	905	961	0.11%	0.010%
29	9.975	1184	1188	1190	rBV4	1102	1431	0.16%	0.016%
30	10.263	1231	1237	1254	rBV	141956	306956	34.34%	3.352%
31	10.634	1294	1300	1315	rBV	160401	285324	31.92%	3.116%
32	10.816	1324	1331	1344	rBV	107533	269491	30.15%	2.943%
33	11.086	1373	1377	1378	rVB4	826	1050	0.12%	0.011%
34	11.334	1415	1419	1420	rVB3	1303	1140	0.13%	0.012%
35	11.945	1519	1523	1524	rBV2	1064	930	0.10%	0.010%
36	12.257	1572	1576	1578	rBV3	835	1217	0.14%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
 Data File : BM042813.D
 Acq On : 16 Nov 2023 19:44
 Operator : MA/JU
 Sample : PB157007BL
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK007

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

37	12.386	1594	1598	1600	rBV3	818	983	0.11%	0.011%
38	12.669	1641	1646	1649	rVB3	426	1000	0.11%	0.011%
39	12.980	1696	1699	1704	rBV2	852	1011	0.11%	0.011%
40	13.322	1754	1757	1761	rBV5	1501	2107	0.24%	0.023%

41	13.486	1780	1785	1787	rBV3	678	988	0.11%	0.011%
42	13.533	1789	1793	1796	rVV3	654	1025	0.11%	0.011%
43	13.704	1818	1822	1829	rVB4	1176	2107	0.24%	0.023%
44	13.904	1850	1856	1867	rBV	312332	480733	53.78%	5.250%
45	13.998	1870	1872	1876	rVB3	1378	1613	0.18%	0.018%

46	14.180	1896	1903	1917	rBV	365875	538785	60.27%	5.884%
47	14.480	1948	1954	1964	rBV	244865	364340	40.76%	3.979%
48	14.551	1964	1966	1970	rVV5	1470	2132	0.24%	0.023%
49	14.704	1987	1992	1993	rBV2	804	1086	0.12%	0.012%
50	14.757	1993	2001	2014	rBV7	24268	100139	11.20%	1.094%

51	14.892	2022	2024	2030	rVB5	2372	3612	0.40%	0.039%
52	15.110	2057	2061	2066	rVB3	1138	1461	0.16%	0.016%
53	15.333	2096	2099	2102	rVV3	1011	1137	0.13%	0.012%
54	15.474	2117	2123	2142	rBV	441138	664823	74.37%	7.260%
55	15.621	2143	2148	2155	rBV	95314	157757	17.65%	1.723%

56	15.716	2162	2164	2168	rVB3	2192	2426	0.27%	0.026%
57	15.810	2178	2180	2184	rVB3	1039	1034	0.12%	0.011%
58	16.357	2272	2273	2277	rBV2	910	932	0.10%	0.010%
59	16.504	2297	2298	2302	rVB3	822	974	0.11%	0.011%
60	16.598	2312	2314	2317	rVB3	1116	968	0.11%	0.011%

61	17.039	2386	2389	2392	rBV2	819	1348	0.15%	0.015%
62	17.233	2416	2422	2433	rBV	283016	417159	46.66%	4.556%
63	17.333	2433	2439	2455	rVV	426183	675625	75.58%	7.378%
64	17.486	2463	2465	2467	rVB4	1327	1128	0.13%	0.012%
65	17.615	2485	2487	2490	rBV	792	1009	0.11%	0.011%

66	18.233	2590	2592	2596	rVB4	905	944	0.11%	0.010%
67	18.351	2609	2612	2614	rBV4	915	1223	0.14%	0.013%
68	18.427	2622	2625	2627	rBV3	969	1190	0.13%	0.013%
69	18.504	2636	2638	2640	rBV2	934	995	0.11%	0.011%
70	18.762	2679	2682	2684	rBV3	943	1220	0.14%	0.013%

71	18.933	2708	2711	2714	rVB3	835	950	0.11%	0.010%
72	19.033	2726	2728	2733	rVB5	1024	1355	0.15%	0.015%
73	19.192	2752	2755	2760	rVB3	3971	5073	0.57%	0.055%
74	19.239	2760	2763	2765	rBV3	1031	1082	0.12%	0.012%
75	19.268	2765	2768	2773	rBV5	3522	5780	0.65%	0.063%

76	19.433	2795	2796	2797	rBV	1777	896	0.10%	0.010%
----	--------	------	------	------	-----	------	-----	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042813.D
Acq On : 16 Nov 2023 19:44
Operator : MA/JU
Sample : PB157007BL
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK007

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Title : SVOA CALIBRATION

77	19.509	2807	2809	2810	rBV2	1387	1270	0.14%	0.014%
78	19.627	2824	2829	2844	rBV	635737	845030	94.53%	9.228%
79	19.945	2881	2883	2884	rBV2	1570	901	0.10%	0.010%
80	19.962	2884	2886	2887	rVB3	2153	1076	0.12%	0.012%
81	19.986	2887	2890	2893	rBV4	1720	2467	0.28%	0.027%
82	21.415	3129	3133	3144	rBV	279311	456398	51.05%	4.984%
83	23.621	3501	3508	3524	rBV2	423638	893958	100.00%	9.762%
84	23.774	3528	3534	3548	rVB	243450	523329	58.54%	5.715%




Sum of corrected areas: 9157201

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042813.D
Acq On : 16 Nov 2023 19:44
Operator : MA/JU
Sample : PB157007BL
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK007

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

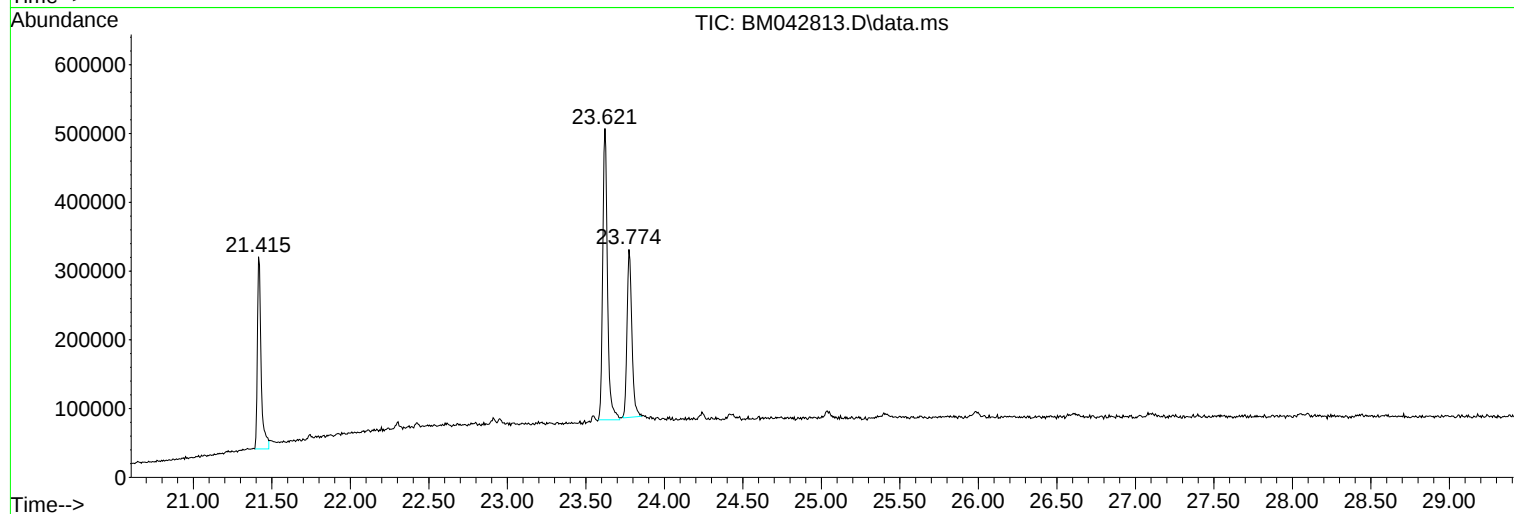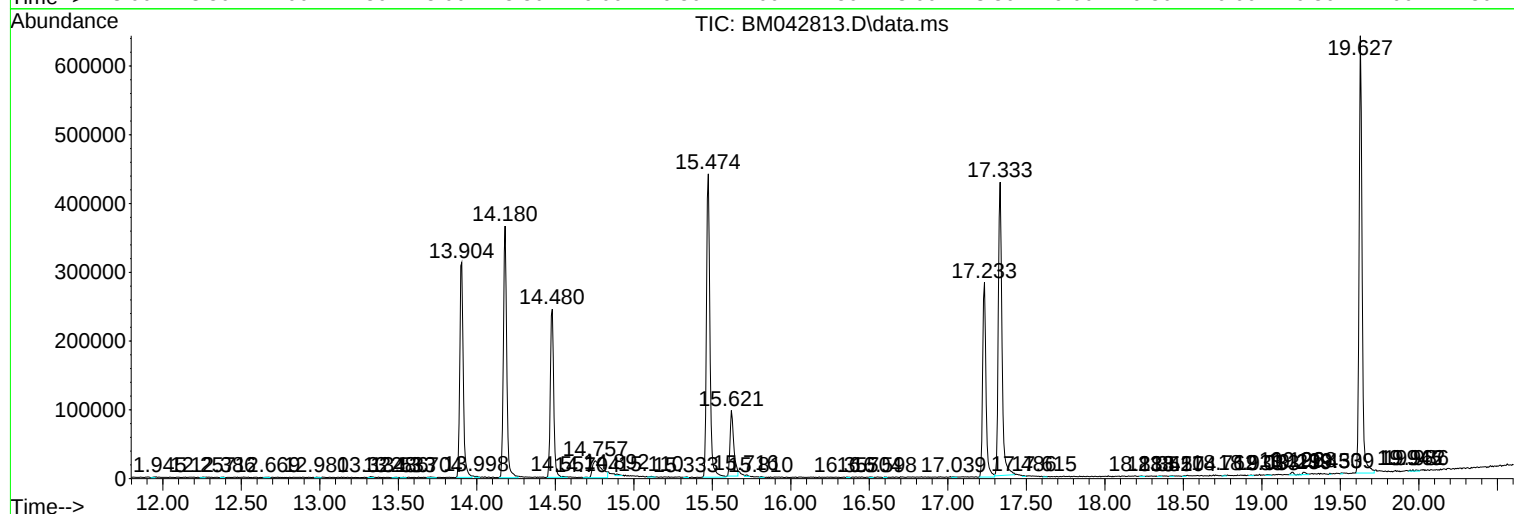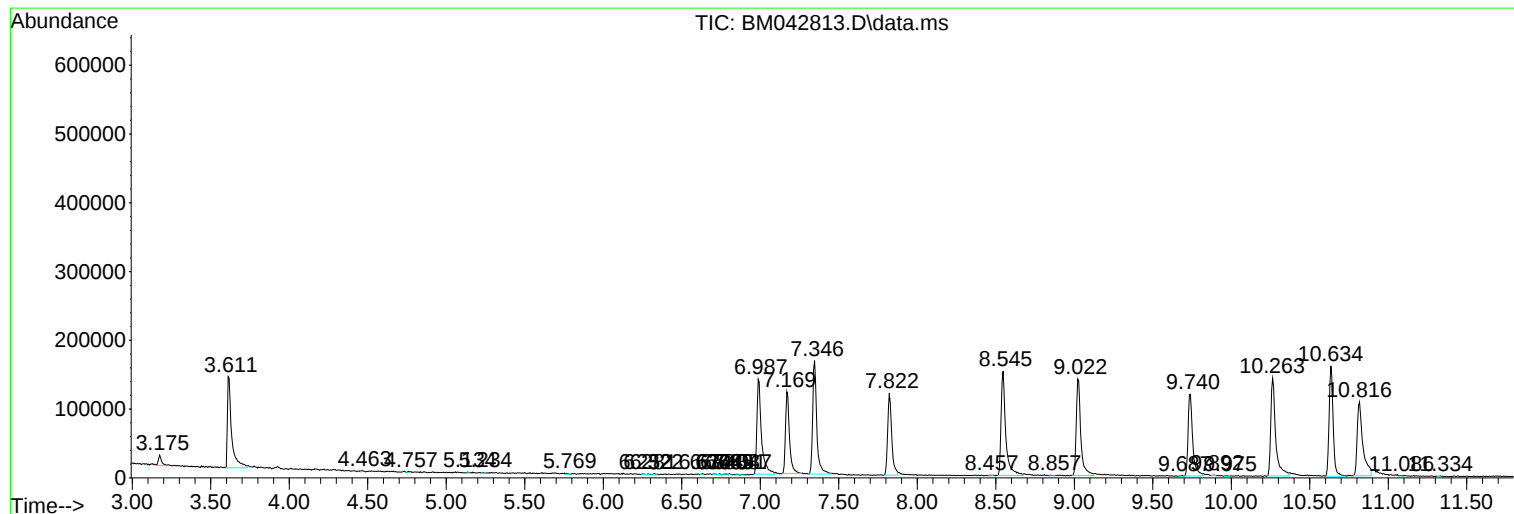

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042813.D
Acq On : 16 Nov 2023 19:44
Operator : MA/JU
Sample : PB157007BL
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK007

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042813.D
Acq On : 16 Nov 2023 19:44
Operator : MA/JU
Sample : PB157007BL
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK007

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------