

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
 Data File : BM042817.D
 Acq On : 16 Nov 2023 22:08
 Operator : MA/JU
 Sample : 05268-08
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCKD0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM042817.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.622	105	108	117	rBV	32559	61521	5.79%	0.754%
2	3.887	151	153	154	rBV2	2224	1745	0.16%	0.021%
3	4.546	263	265	267	rVB3	1526	1112	0.10%	0.014%
4	5.010	340	344	345	rBV3	1137	1534	0.14%	0.019%
5	5.675	455	457	461	rBV4	1057	1459	0.14%	0.018%
6	6.404	577	581	582	rVB3	1577	1565	0.15%	0.019%
7	6.998	678	682	692	rBV2	12632	33118	3.11%	0.406%
8	7.169	706	711	723	rBV	103421	190841	17.95%	2.338%
9	7.345	735	741	762	rBV	102551	198349	18.65%	2.430%
10	7.822	817	822	841	rVV	89571	166475	15.66%	2.039%
11	8.081	864	866	869	rBV3	821	1165	0.11%	0.014%
12	8.551	940	946	959	rBV2	48403	110877	10.43%	1.358%
13	8.704	970	972	975	rVB4	1151	1264	0.12%	0.015%
14	9.022	1020	1026	1043	rBV	127191	262833	24.72%	3.220%
15	9.622	1125	1128	1131	rBV4	794	1257	0.12%	0.015%
16	9.739	1142	1148	1163	rBV	103746	211001	19.84%	2.585%
17	9.851	1166	1167	1169	rVV	1606	1097	0.10%	0.013%
18	9.886	1172	1173	1177	rBV3	1232	1414	0.13%	0.017%
19	10.263	1231	1237	1257	rBV	115484	258144	24.28%	3.162%
20	10.634	1294	1300	1307	rBV	123524	211469	19.89%	2.590%
21	10.816	1324	1331	1357	rBV	79637	221605	20.84%	2.715%
22	11.022	1365	1366	1368	rBV2	1489	1156	0.11%	0.014%
23	11.375	1421	1426	1429	rBV2	856	1762	0.17%	0.022%
24	11.686	1475	1479	1480	rBV3	1487	1533	0.14%	0.019%
25	12.269	1575	1578	1584	rBV4	875	1384	0.13%	0.017%
26	12.886	1681	1683	1688	rBV3	1178	1486	0.14%	0.018%
27	13.327	1754	1758	1764	rVB3	2253	3478	0.33%	0.043%
28	13.704	1817	1822	1828	rBV5	1101	2216	0.21%	0.027%
29	13.898	1850	1855	1867	rBV	330447	499707	47.00%	6.121%
30	14.180	1896	1903	1917	rBV	354245	532374	50.07%	6.521%
31	14.480	1947	1954	1963	rVV	177680	276787	26.03%	3.390%
32	14.539	1963	1964	1969	rVB4	2565	2006	0.19%	0.025%
33	14.669	1983	1986	1988	rBV3	1143	1346	0.13%	0.016%
34	14.892	2021	2024	2030	rVB3	818	1312	0.12%	0.016%
35	15.474	2116	2123	2136	rBV	463678	697163	65.57%	8.540%
36	15.580	2139	2141	2143	rVB3	2027	1826	0.17%	0.022%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
 Data File : BM042817.D
 Acq On : 16 Nov 2023 22:08
 Operator : MA/JU
 Sample : 05268-08
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCKD0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

37	15.621	2143	2148	2161	rBV	119118	210188	19.77%	2.575%
38	15.710	2161	2163	2167	rVB4	2762	3405	0.32%	0.042%
39	16.521	2299	2301	2305	rVV2	951	1167	0.11%	0.014%
40	17.121	2401	2403	2406	rBV2	1091	1208	0.11%	0.015%
41	17.233	2415	2422	2433	rBV	211070	315074	29.63%	3.859%
42	17.333	2433	2439	2455	rVV	517154	791242	74.41%	9.692%
43	17.757	2508	2511	2516	rVB4	1202	1273	0.12%	0.016%
44	17.862	2523	2529	2533	rVB4	3118	3793	0.36%	0.046%
45	17.968	2544	2547	2548	rVB3	1490	1385	0.13%	0.017%
46	18.174	2580	2582	2585	rVB3	1138	1090	0.10%	0.013%
47	18.280	2599	2600	2603	rBV3	1063	1131	0.11%	0.014%
48	18.345	2606	2611	2614	rBV6	1160	1747	0.16%	0.021%
49	18.580	2647	2651	2654	rBV5	1114	1884	0.18%	0.023%
50	18.974	2715	2718	2721	rVV3	1935	2172	0.20%	0.027%
51	19.186	2751	2754	2759	rBV4	5452	7173	0.67%	0.088%
52	19.262	2764	2767	2771	rBV3	4114	5866	0.55%	0.072%
53	19.380	2784	2787	2788	rBV3	1057	1249	0.12%	0.015%
54	19.627	2823	2829	2846	rBV	768856	1004440	94.46%	12.304%
55	19.803	2857	2859	2861	rBV2	2593	3087	0.29%	0.038%
56	20.409	2960	2962	2963	rBV	2694	1880	0.18%	0.023%
57	21.415	3128	3133	3144	rBV2	235204	353354	33.23%	4.328%
58	23.621	3501	3508	3524	rBV2	528324	1063311	100.00%	13.025%
59	23.774	3528	3534	3550	rVB	190460	421132	39.61%	5.159%




Sum of corrected areas: 8163632

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042817.D
Acq On : 16 Nov 2023 22:08
Operator : MA/JU
Sample : 05268-08
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCKD0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

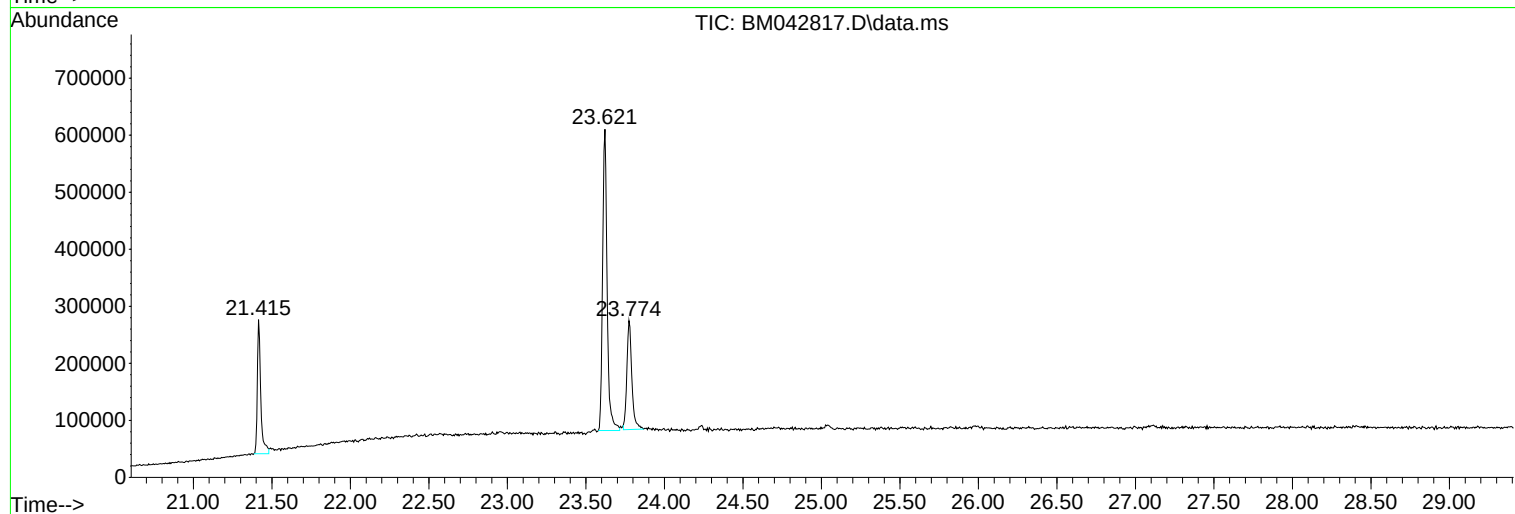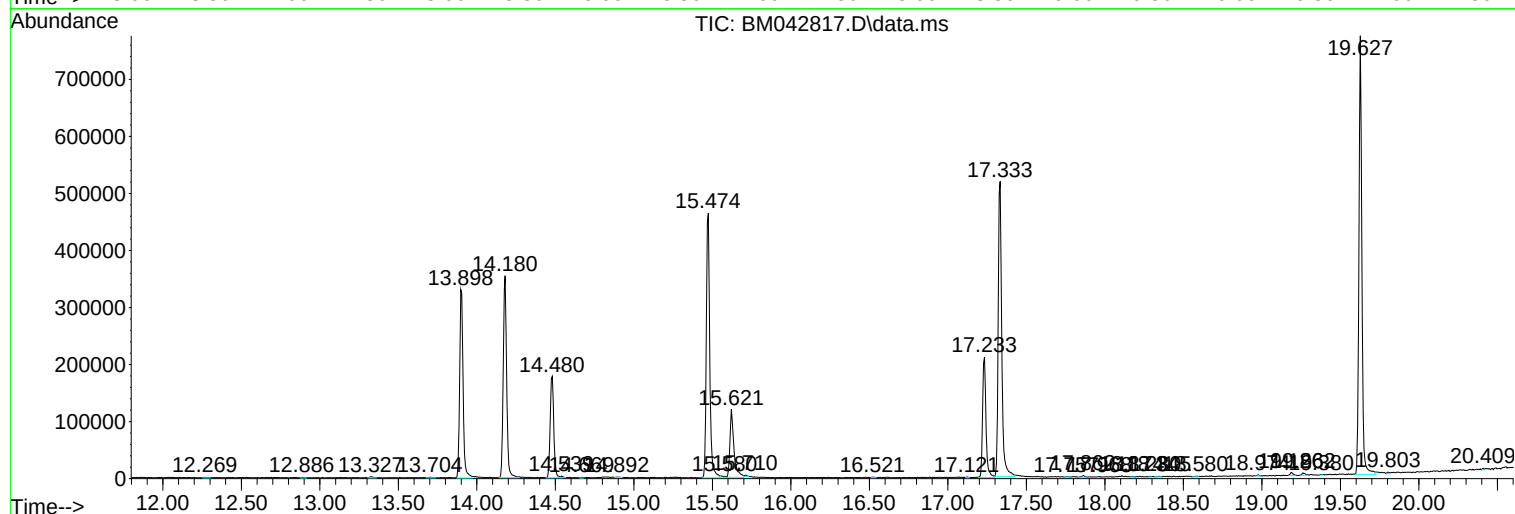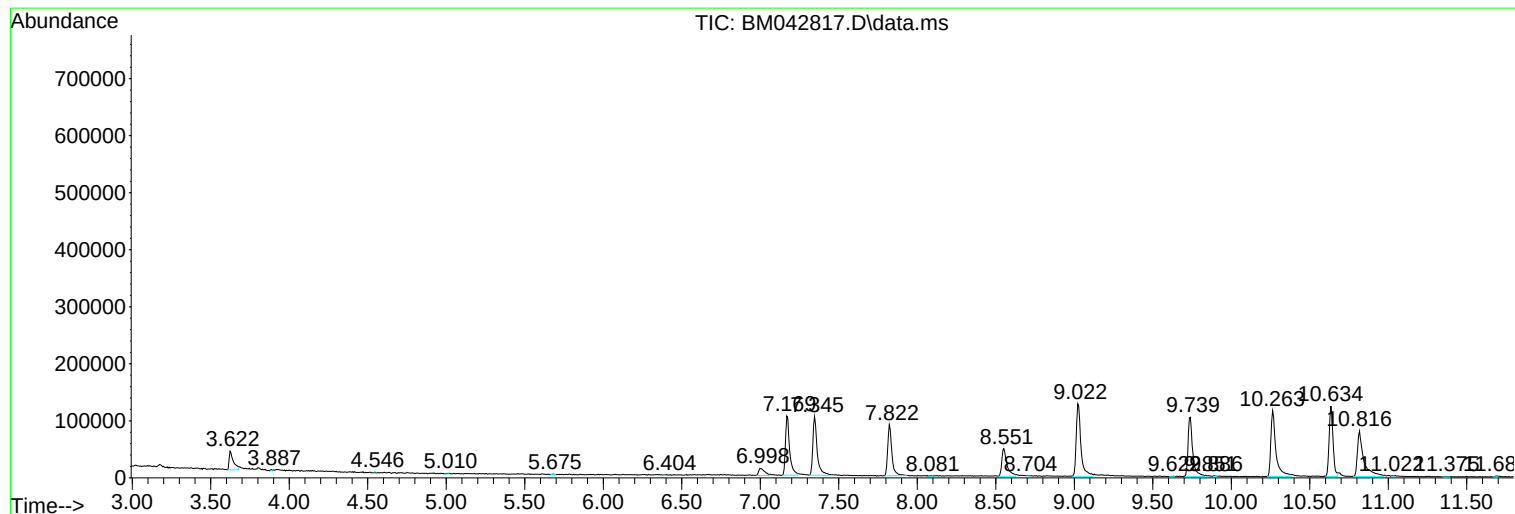

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042817.D
Acq On : 16 Nov 2023 22:08
Operator : MA/JU
Sample : 05268-08
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCKD0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042817.D
Acq On : 16 Nov 2023 22:08
Operator : MA/JU
Sample : 05268-08
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCKD0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc