

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
 Data File : BM042818.D
 Acq On : 16 Nov 2023 22:45
 Operator : MA/JU
 Sample : 05268-09
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCKD1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM042818.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.628	106	109	119	rBV2	21032	42559	3.89%	0.501%
2	4.940	328	332	336	rBV4	1179	1689	0.15%	0.020%
3	5.057	349	352	353	rBV3	3181	2797	0.26%	0.033%
4	5.604	444	445	447	rBV2	1285	1146	0.10%	0.013%
5	5.916	496	498	503	rVB3	1267	1228	0.11%	0.014%
6	6.069	520	524	525	rBV2	1071	1127	0.10%	0.013%
7	6.616	615	617	620	rVB4	1583	1273	0.12%	0.015%
8	6.646	620	622	624	rBV2	1299	1189	0.11%	0.014%
9	6.998	677	682	694	rBV	12428	33398	3.05%	0.393%
10	7.169	706	711	724	rBV	107470	195314	17.84%	2.298%
11	7.345	735	741	757	rBV	100288	188043	17.17%	2.212%
12	7.640	788	791	793	rBV3	921	1143	0.10%	0.013%
13	7.822	817	822	838	rBV	96938	179417	16.39%	2.111%
14	8.551	940	946	964	rBV2	48497	110093	10.05%	1.295%
15	8.704	969	972	978	rVB6	3930	7258	0.66%	0.085%
16	9.022	1020	1026	1040	rBV	130372	263277	24.04%	3.097%
17	9.734	1141	1147	1163	rBV	110707	218301	19.94%	2.568%
18	9.928	1177	1180	1182	rVB3	926	1145	0.10%	0.013%
19	10.263	1230	1237	1251	rBV	117189	256092	23.39%	3.013%
20	10.486	1273	1275	1279	rVB4	1288	1172	0.11%	0.014%
21	10.634	1292	1300	1312	rBV	132450	235541	21.51%	2.771%
22	10.816	1325	1331	1351	rBV2	62053	173005	15.80%	2.035%
23	11.281	1406	1410	1413	rBV3	951	1412	0.13%	0.017%
24	11.316	1413	1416	1419	rVB3	802	1195	0.11%	0.014%
25	11.698	1477	1481	1484	rVB3	1914	2431	0.22%	0.029%
26	13.327	1753	1758	1764	rVB2	3134	4895	0.45%	0.058%
27	13.710	1817	1823	1826	rVB3	982	1544	0.14%	0.018%
28	13.898	1850	1855	1870	rBV	352386	523415	47.80%	6.158%
29	14.180	1896	1903	1919	rBV	382302	557057	50.87%	6.553%
30	14.286	1919	1921	1923	rVV2	1611	1224	0.11%	0.014%
31	14.304	1923	1924	1931	rVB4	1063	1747	0.16%	0.021%
32	14.480	1947	1954	1962	rBV2	193116	293931	26.84%	3.458%
33	14.545	1962	1965	1971	rVB4	1015	1510	0.14%	0.018%
34	14.798	2003	2008	2011	rBV2	1234	2064	0.19%	0.024%
35	15.039	2044	2049	2052	rBV4	2972	4697	0.43%	0.055%
36	15.116	2058	2062	2069	rVB6	2316	4569	0.42%	0.054%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
 Data File : BM042818.D
 Acq On : 16 Nov 2023 22:45
 Operator : MA/JU
 Sample : 05268-09
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCKD1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

37	15.263	2083	2087	2091	rBV5	1055	1405	0.13%	0.017%
38	15.474	2117	2123	2139	rVV	481183	730091	66.68%	8.589%
39	15.621	2142	2148	2166	rVB	136216	234378	21.41%	2.757%
40	15.886	2190	2193	2197	rBV3	859	1287	0.12%	0.015%
41	16.051	2215	2221	2222	rBV3	933	1564	0.14%	0.018%
42	16.510	2293	2299	2304	rBV4	741	1388	0.13%	0.016%
43	16.880	2357	2362	2366	rBV4	1588	2857	0.26%	0.034%
44	17.233	2416	2422	2432	rBV	228248	336222	30.71%	3.955%
45	17.333	2432	2439	2457	rVV	539271	824293	75.28%	9.697%
46	17.486	2463	2465	2469	rVB3	1583	1854	0.17%	0.022%
47	17.780	2512	2515	2519	rBV4	972	1793	0.16%	0.021%
48	17.951	2541	2544	2547	rBV3	975	1350	0.12%	0.016%
49	18.045	2559	2560	2563	rBV3	1260	1383	0.13%	0.016%
50	18.086	2563	2567	2575	rVV5	8475	16249	1.48%	0.191%
51	18.174	2579	2582	2588	rVB3	1797	3280	0.30%	0.039%
52	18.492	2632	2636	2637	rBV3	1112	1255	0.11%	0.015%
53	18.768	2681	2683	2685	rBV	1195	1169	0.11%	0.014%
54	18.939	2710	2712	2715	rVB4	1215	1150	0.11%	0.014%
55	19.186	2748	2754	2758	rBV7	6055	9381	0.86%	0.110%
56	19.262	2764	2767	2772	rVB2	4076	5753	0.53%	0.068%
57	19.304	2772	2774	2776	rBV2	1097	1106	0.10%	0.013%
58	19.374	2783	2786	2788	rBV4	1962	2519	0.23%	0.030%
59	19.627	2823	2829	2839	rBV	861579	1067034	97.45%	12.553%
60	21.415	3128	3133	3144	rBV	272721	390127	35.63%	4.590%
61	23.621	3501	3508	3520	rBV	536445	1094967	100.00%	12.881%
62	23.774	3528	3534	3548	rVB	213220	448556	40.97%	5.277%




Sum of corrected areas: 8500309

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042818.D
Acq On : 16 Nov 2023 22:45
Operator : MA/JU
Sample : 05268-09
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCKD1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

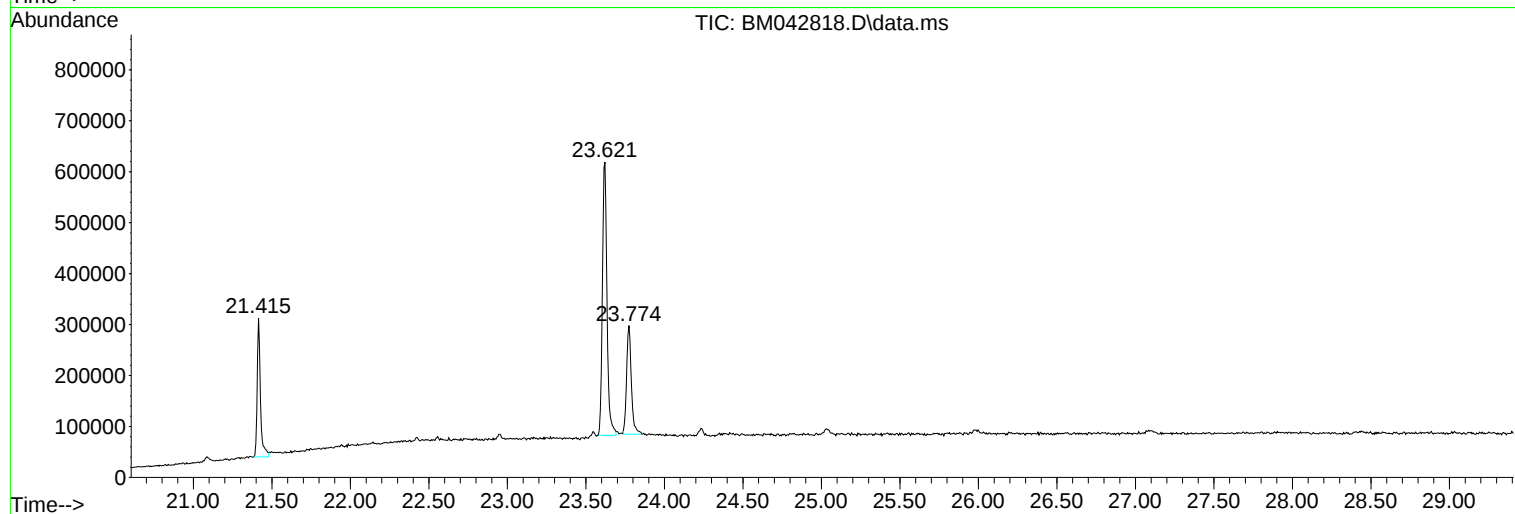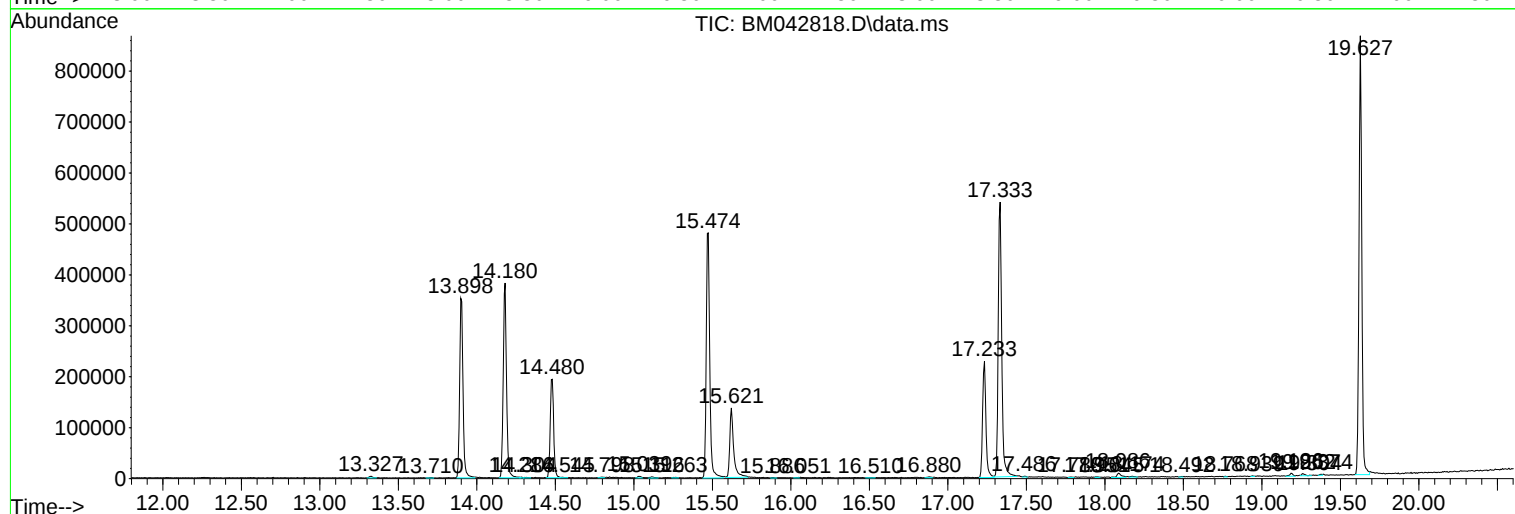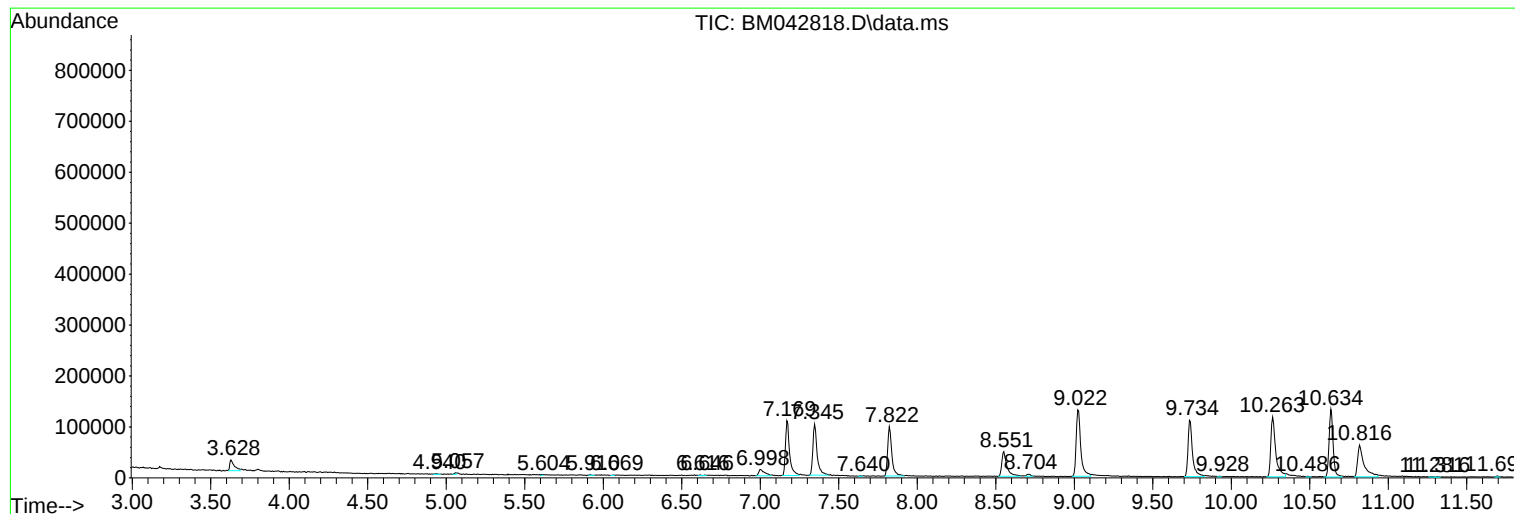

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042818.D
Acq On : 16 Nov 2023 22:45
Operator : MA/JU
Sample : 05268-09
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCKD1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042818.D
Acq On : 16 Nov 2023 22:45
Operator : MA/JU
Sample : 05268-09
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCKD1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc