

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
 Data File : BM042819.D
 Acq On : 16 Nov 2023 23:21
 Operator : MA/JU
 Sample : 05268-10
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCKD2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM042819.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.622	105	108	119	rBV	37642	72056	6.42%	0.757%
2	5.428	413	415	418	rBV3	1304	1164	0.10%	0.012%
3	5.463	420	421	423	rBV	1349	1160	0.10%	0.012%
4	5.510	426	429	430	rBV2	1544	1715	0.15%	0.018%
5	6.557	606	607	611	rVB4	1300	1383	0.12%	0.015%
6	6.998	677	682	696	rBV6	12733	34959	3.11%	0.367%
7	7.169	706	711	727	rBV	111553	202778	18.06%	2.130%
8	7.345	735	741	757	rBV	103151	195384	17.40%	2.052%
9	7.822	816	822	840	rBV	100736	192677	17.16%	2.024%
10	8.157	878	879	882	rVB3	1462	1134	0.10%	0.012%
11	8.181	882	883	886	rBV2	1297	1443	0.13%	0.015%
12	8.304	900	904	907	rVB3	758	1243	0.11%	0.013%
13	8.381	912	917	927	rVV7	5179	10679	0.95%	0.112%
14	8.551	941	946	964	rBV2	50173	109235	9.73%	1.147%
15	8.704	969	972	981	rVB3	9168	16439	1.46%	0.173%
16	9.022	1020	1026	1046	rBV	136928	274935	24.49%	2.887%
17	9.428	1092	1095	1097	rBV5	1210	1406	0.13%	0.015%
18	9.669	1134	1136	1139	rVB3	998	1150	0.10%	0.012%
19	9.733	1139	1147	1161	rBV	112704	227000	20.22%	2.384%
20	10.263	1230	1237	1249	rBV2	126036	266665	23.75%	2.801%
21	10.633	1294	1300	1306	rBV	142737	244768	21.80%	2.571%
22	10.686	1306	1309	1319	rVB2	22955	38489	3.43%	0.404%
23	10.816	1324	1331	1351	rBV2	105261	269912	24.04%	2.835%
24	11.263	1404	1407	1409	rBV3	939	1282	0.11%	0.013%
25	11.304	1412	1414	1417	rVB3	1354	1239	0.11%	0.013%
26	11.445	1434	1438	1440	rVV4	1122	1719	0.15%	0.018%
27	11.698	1475	1481	1484	rBV4	1962	3458	0.31%	0.036%
28	12.227	1568	1571	1573	rBV4	1337	1438	0.13%	0.015%
29	12.310	1578	1585	1599	rBV2	11170	25556	2.28%	0.268%
30	12.521	1616	1621	1627	rBV2	9190	17250	1.54%	0.181%
31	12.563	1627	1628	1631	rVB2	2101	1562	0.14%	0.016%
32	12.804	1666	1669	1673	rVV	1082	1267	0.11%	0.013%
33	13.016	1703	1705	1708	rVV3	1037	1263	0.11%	0.013%
34	13.321	1752	1757	1765	rBV2	12982	22413	2.00%	0.235%
35	13.698	1818	1821	1825	rBV4	1241	1757	0.16%	0.018%
36	13.792	1832	1837	1845	rBV6	4080	10300	0.92%	0.108%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
 Data File : BM042819.D
 Acq On : 16 Nov 2023 23:21
 Operator : MA/JU
 Sample : 05268-10
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCKD2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

37	13.898	1849	1855	1871	rVV	379005	535286	47.68%	5.622%
38	14.004	1871	1873	1876	rVV2	1599	2032	0.18%	0.021%
39	14.180	1896	1903	1913	rBV	388711	564249	50.26%	5.926%
40	14.480	1946	1954	1960	rBV	227836	323030	28.77%	3.393%
41	14.545	1960	1965	1971	rVB2	22740	38417	3.42%	0.403%
42	14.651	1978	1983	1988	rBV2	12263	20061	1.79%	0.211%
43	14.774	1998	2004	2009	rBV4	5402	10575	0.94%	0.111%
44	14.880	2017	2022	2031	rBV	35192	61116	5.44%	0.642%
45	14.939	2031	2032	2037	rVB3	1525	1397	0.12%	0.015%
46	15.027	2043	2047	2054	rVV4	9801	15587	1.39%	0.164%
47	15.115	2054	2062	2067	rVB4	4758	7571	0.67%	0.080%
48	15.474	2117	2123	2129	rBV	513468	739054	65.83%	7.762%
49	15.527	2129	2132	2141	rVB	32008	53363	4.75%	0.560%
50	15.621	2142	2148	2161	rVV	135986	230560	20.54%	2.421%
51	15.762	2171	2172	2177	rVB5	2014	1905	0.17%	0.020%
52	16.098	2225	2229	2230	rBV2	1078	1177	0.10%	0.012%
53	16.233	2247	2252	2258	rVB3	6462	11287	1.01%	0.119%
54	16.386	2275	2278	2280	rBV2	1055	1211	0.11%	0.013%
55	16.521	2296	2301	2310	rVV7	6406	14648	1.30%	0.154%
56	16.621	2317	2318	2323	rVB2	1272	1185	0.11%	0.012%
57	16.762	2338	2342	2343	rBV3	1354	1685	0.15%	0.018%
58	16.903	2356	2366	2373	rVV4	12248	28510	2.54%	0.299%
59	17.233	2413	2422	2427	rBV	260292	378748	33.74%	3.978%
60	17.268	2427	2428	2433	rVB2	18122	21403	1.91%	0.225%
61	17.333	2433	2439	2450	rBV	559518	819221	72.97%	8.604%
62	17.598	2481	2484	2486	rVB3	1171	1325	0.12%	0.014%
63	17.662	2490	2495	2504	rBV	55988	97627	8.70%	1.025%
64	17.833	2520	2524	2535	rBV6	6195	15670	1.40%	0.165%
65	17.962	2544	2546	2549	rBV3	1415	1673	0.15%	0.018%
66	18.092	2563	2568	2575	rBV4	9446	19745	1.76%	0.207%
67	18.180	2581	2583	2585	rVB2	2319	1477	0.13%	0.016%
68	18.268	2593	2598	2604	rVB5	1719	3150	0.28%	0.033%
69	18.509	2637	2639	2642	rVB3	1306	1252	0.11%	0.013%
70	18.568	2645	2649	2650	rBV3	1632	1676	0.15%	0.018%
71	18.650	2660	2663	2664	rBV3	1560	1567	0.14%	0.016%
72	18.686	2667	2669	2672	rVB3	2099	1862	0.17%	0.020%
73	18.786	2684	2686	2687	rBV2	1828	1247	0.11%	0.013%
74	19.109	2737	2741	2742	rBV3	1671	1910	0.17%	0.020%
75	19.186	2750	2754	2758	rBV5	7011	9680	0.86%	0.102%
76	19.227	2758	2761	2762	rBV2	17000	16654	1.48%	0.175%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042819.D
Acq On : 16 Nov 2023 23:21
Operator : MA/JU
Sample : 05268-10
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCKD2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Title : SVOA CALIBRATION

77	19.250	2762	2765	2773	rVB2	36152	60849	5.42%	0.639%
78	19.374	2782	2786	2793	rBV5	8076	15802	1.41%	0.166%
79	19.539	2812	2814	2816	rBV3	1384	1400	0.12%	0.015%
80	19.627	2823	2829	2844	rBV	863376	1084108	96.57%	11.386%
81	20.056	2900	2902	2904	rBV2	2046	1540	0.14%	0.016%
82	21.080	3074	3076	3077	rBV2	7314	5151	0.46%	0.054%
83	21.415	3128	3133	3141	rBV	310895	431961	38.48%	4.537%
84	23.615	3501	3507	3520	rBV2	556060	1122622	100.00%	11.790%
85	23.774	3528	3534	3546	rVB	235621	480087	42.76%	5.042%




Sum of corrected areas: 9521591

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042819.D
Acq On : 16 Nov 2023 23:21
Operator : MA/JU
Sample : 05268-10
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCKD2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

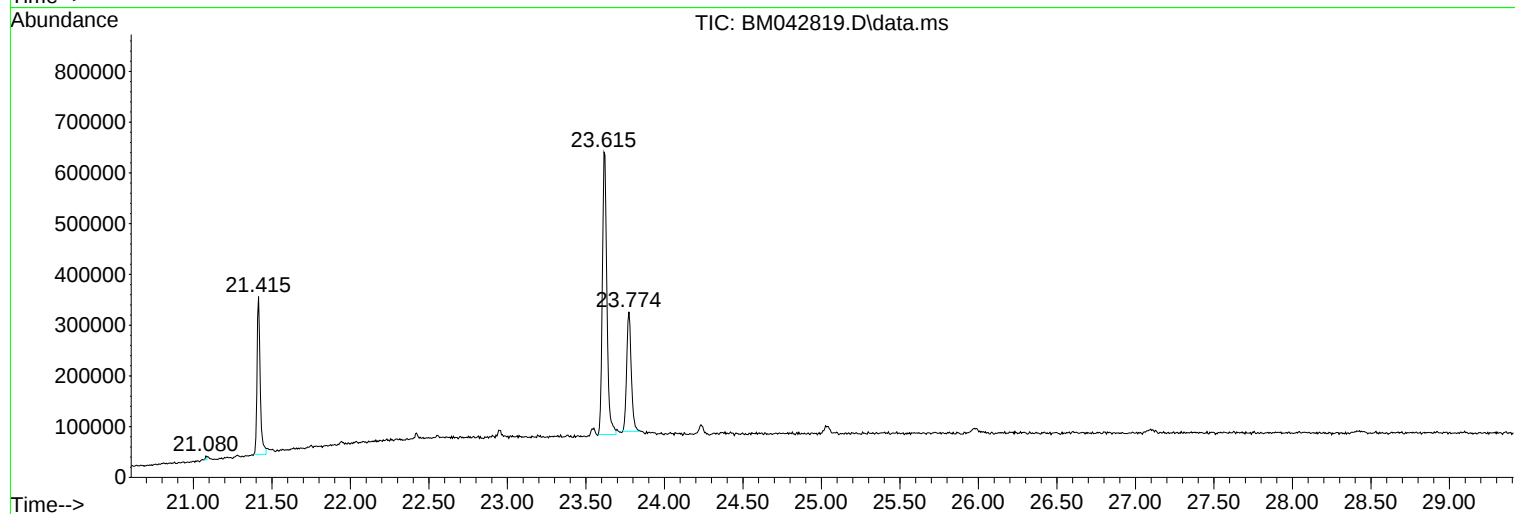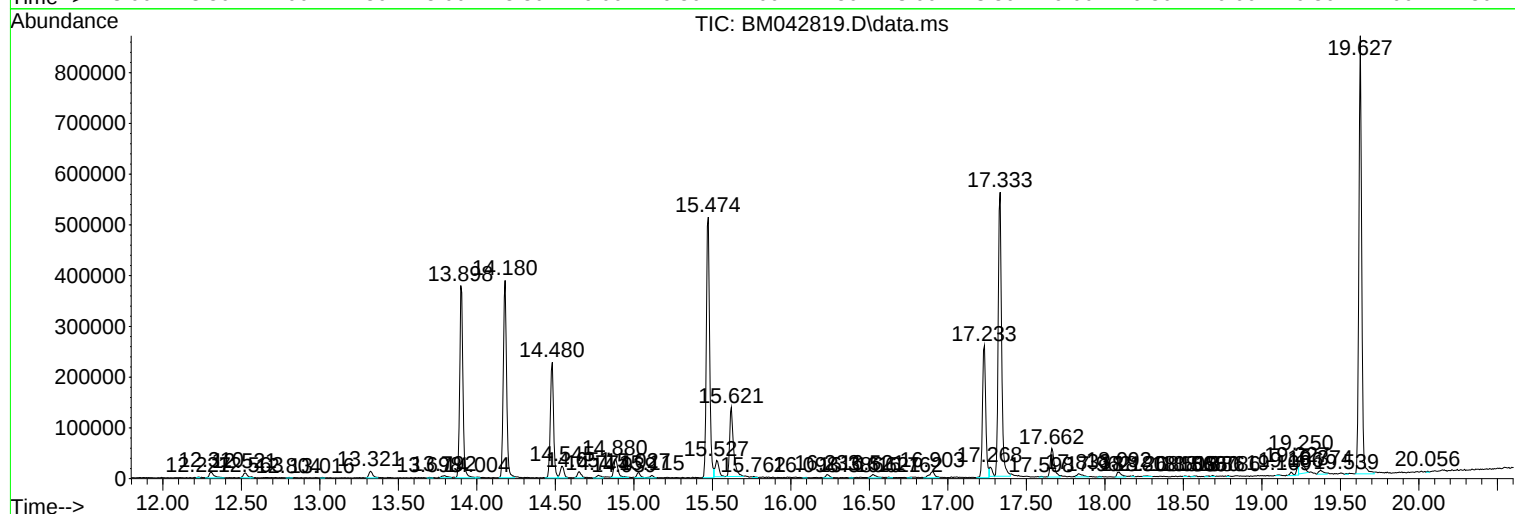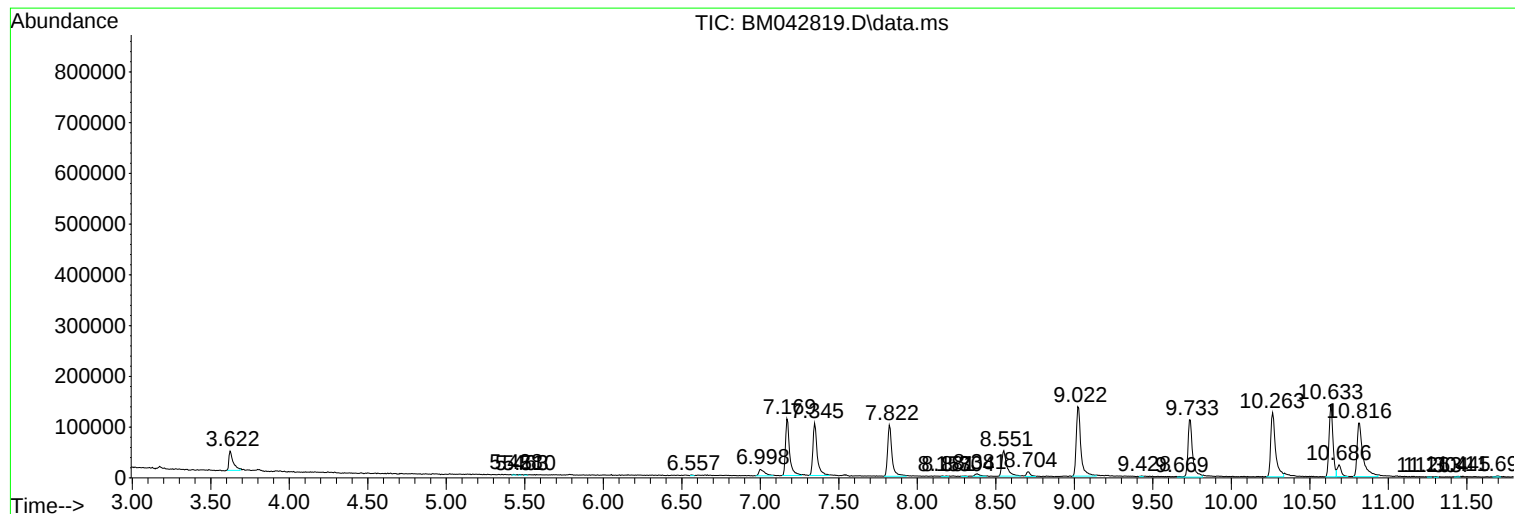

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042819.D
Acq On : 16 Nov 2023 23:21
Operator : MA/JU
Sample : 05268-10
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCKD2










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Cyclic19.250 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
19.250	3.21 ng/ul	60849	Phenanthrene-d10	17.233

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Cyclopentadecane	210	C15H30	000295-48-7	70
2			1-Pentadecene	210	C15H30	013360-61-7	70
3			1-Pentadecene	210	C15H30	013360-61-7	70
4			1-Dodecanol	186	C12H26O	000112-53-8	68
5			3-Hexadecene, (Z)-	224	C16H32	034303-81-6	52

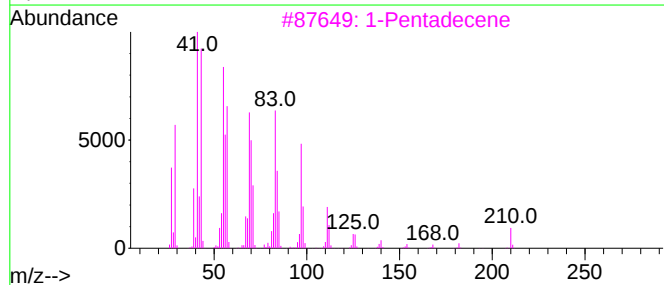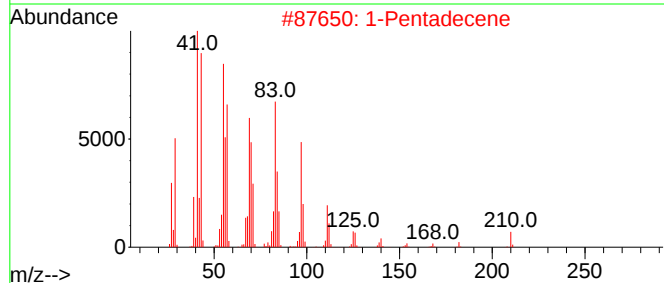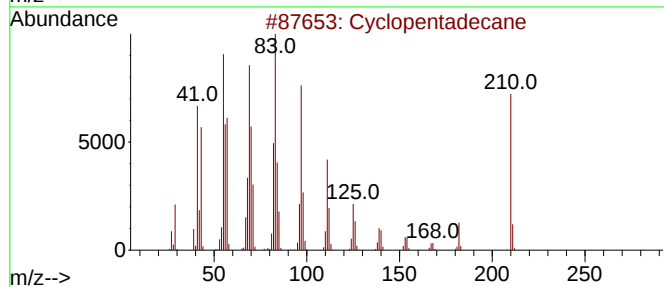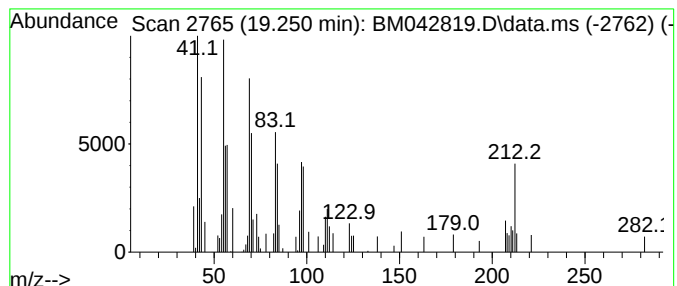

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042819.D
Acq On : 16 Nov 2023 23:21
Operator : MA/JU
Sample : 05268-10
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCKD2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: C...	19.250	3.2	ng/u1	60849	4	17.233	378748	20.0