

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
 Data File : BM042820.D
 Acq On : 16 Nov 2023 23:57
 Operator : MA/JU
 Sample : 05268-11
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCKD3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM042820.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	29	33	36	rBV4	5182	6534	0.64%	0.081%
2	3.628	105	109	120	rBV	26400	56898	5.56%	0.706%
3	4.616	276	277	279	rBV2	1236	1129	0.11%	0.014%
4	4.869	318	320	323	rBV3	978	1110	0.11%	0.014%
5	6.028	513	517	520	rBV5	1068	1252	0.12%	0.016%
6	6.481	592	594	597	rVB3	1244	1075	0.11%	0.013%
7	7.004	678	683	695	rBV3	12644	36137	3.53%	0.449%
8	7.169	705	711	722	rBV	104004	192640	18.83%	2.391%
9	7.345	735	741	761	rBV2	99485	192015	18.77%	2.384%
10	7.528	770	772	775	rVB4	1229	1239	0.12%	0.015%
11	7.822	816	822	834	rBV	92877	169375	16.55%	2.103%
12	8.145	875	877	880	rBV2	880	1198	0.12%	0.015%
13	8.516	937	940	941	rBV3	994	1189	0.12%	0.015%
14	8.551	941	946	961	rVV	50083	110222	10.77%	1.368%
15	8.651	961	963	965	rVB3	1200	1073	0.10%	0.013%
16	9.022	1020	1026	1047	rVV	130013	264763	25.88%	3.287%
17	9.204	1055	1057	1061	rVB5	1434	1967	0.19%	0.024%
18	9.498	1104	1107	1114	rBV4	716	1826	0.18%	0.023%
19	9.733	1140	1147	1162	rBV	101610	211268	20.65%	2.623%
20	9.875	1169	1171	1175	rVB4	1140	1228	0.12%	0.015%
21	10.263	1231	1237	1255	rBV	114970	250510	24.48%	3.110%
22	10.380	1255	1257	1262	rVB5	1937	2506	0.24%	0.031%
23	10.633	1293	1300	1310	rBV	132612	223910	21.88%	2.780%
24	10.816	1325	1331	1353	rVV2	78454	218721	21.38%	2.715%
25	10.986	1357	1360	1362	rVB3	993	1172	0.11%	0.015%
26	11.280	1406	1410	1411	rVB3	1009	1168	0.11%	0.014%
27	13.016	1702	1705	1710	rVB4	755	1148	0.11%	0.014%
28	13.057	1710	1712	1715	rBV2	945	1132	0.11%	0.014%
29	13.321	1753	1757	1761	rBV3	2686	4414	0.43%	0.055%
30	13.704	1819	1822	1828	rVB4	1154	1819	0.18%	0.023%
31	13.898	1850	1855	1870	rBV	321611	484360	47.34%	6.013%
32	14.180	1897	1903	1919	rBV	350020	513797	50.22%	6.378%
33	14.480	1947	1954	1962	rBV	188679	285959	27.95%	3.550%
34	14.539	1962	1964	1969	rVB2	1106	1356	0.13%	0.017%
35	15.115	2058	2062	2064	rBV2	1148	1596	0.16%	0.020%
36	15.268	2084	2088	2093	rVB4	850	1564	0.15%	0.019%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
 Data File : BM042820.D
 Acq On : 16 Nov 2023 23:57
 Operator : MA/JU
 Sample : 05268-11
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCKD3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

37	15.421	2109	2114	2117	rBV3	875	1260	0.12%	0.016%
38	15.474	2117	2123	2139	rBV	445230	671697	65.65%	8.338%
39	15.621	2143	2148	2162	rBV2	105639	187452	18.32%	2.327%
40	16.051	2219	2221	2224	rBV2	1169	1305	0.13%	0.016%
41	16.292	2257	2262	2265	rVB3	1082	1728	0.17%	0.021%
42	16.321	2265	2267	2269	rBV2	1260	1073	0.10%	0.013%
43	16.498	2293	2297	2298	rBV2	758	1026	0.10%	0.013%
44	16.892	2359	2364	2365	rBV3	902	1058	0.10%	0.013%
45	17.233	2416	2422	2432	rBV	216147	320325	31.31%	3.976%
46	17.333	2433	2439	2458	rVV	511938	771754	75.43%	9.580%
47	17.704	2499	2502	2504	rBV4	905	1062	0.10%	0.013%
48	17.962	2543	2546	2547	rBV2	1458	1575	0.15%	0.020%
49	17.974	2547	2548	2551	rVB3	1490	1185	0.12%	0.015%
50	18.092	2564	2568	2576	rBV6	5007	11088	1.08%	0.138%
51	18.227	2588	2591	2594	rBV3	1074	1084	0.11%	0.013%
52	18.592	2650	2653	2654	rBV3	1010	1035	0.10%	0.013%
53	18.980	2718	2719	2721	rBV2	1709	1187	0.12%	0.015%
54	19.039	2725	2729	2731	rBV4	1139	1389	0.14%	0.017%
55	19.192	2751	2755	2758	rBV4	4998	6485	0.63%	0.081%
56	19.268	2764	2768	2772	rVB5	3532	6012	0.59%	0.075%
57	19.380	2784	2787	2791	rBV5	2091	3687	0.36%	0.046%
58	19.468	2800	2802	2804	rVB3	1342	1186	0.12%	0.015%
59	19.503	2804	2808	2812	rBV5	2425	4369	0.43%	0.054%
60	19.627	2823	2829	2846	rBV	738224	983791	96.15%	12.213%
61	20.168	2919	2921	2922	rVB2	2232	1186	0.12%	0.015%
62	21.415	3128	3133	3145	rBV	232433	367925	35.96%	4.567%
63	23.621	3501	3508	3520	rBV	527740	1023191	100.00%	12.702%
64	23.774	3527	3534	3545	rBV	199151	430113	42.04%	5.339%




Sum of corrected areas: 8055498

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042820.D
Acq On : 16 Nov 2023 23:57
Operator : MA/JU
Sample : 05268-11
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCKD3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

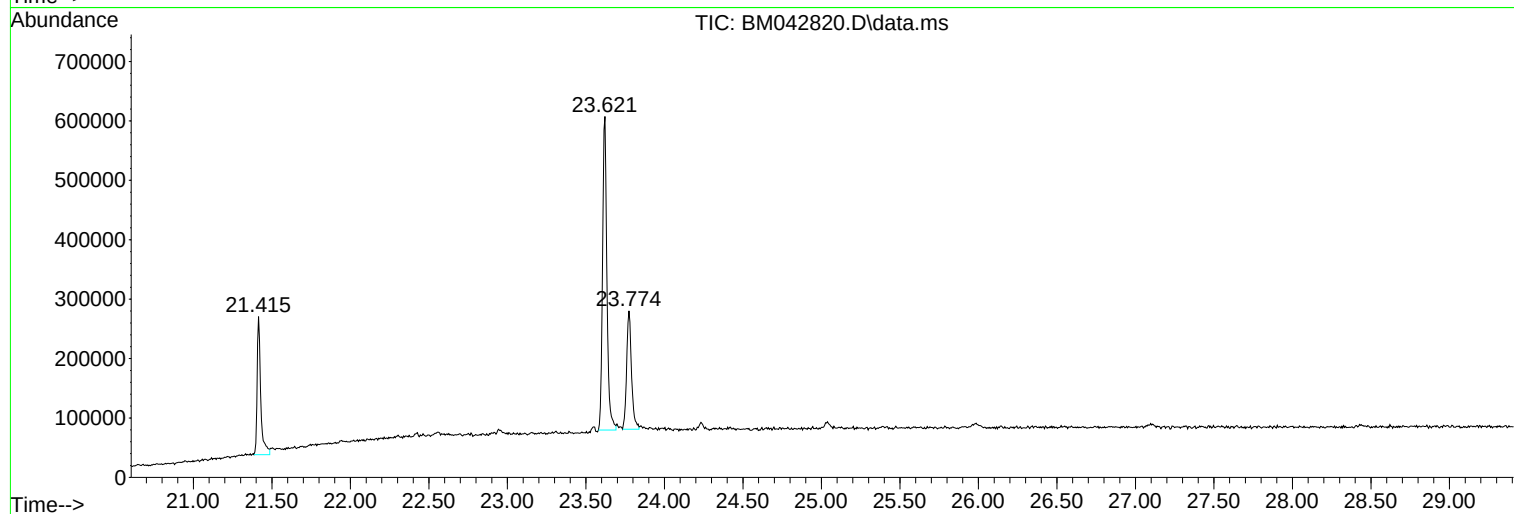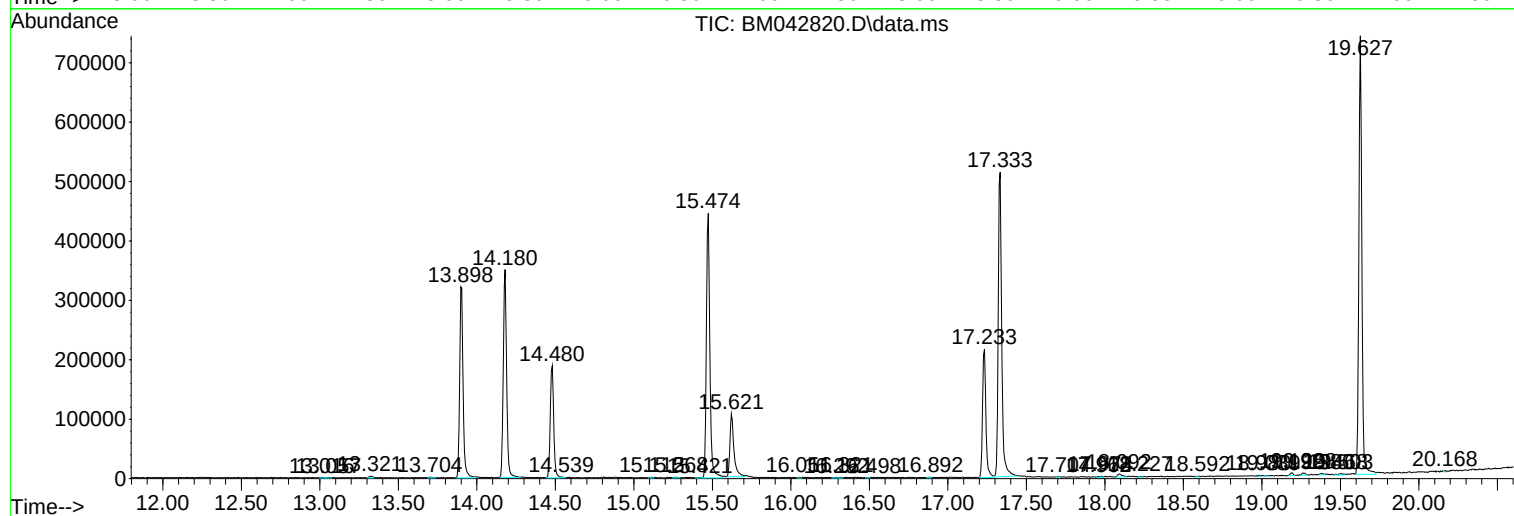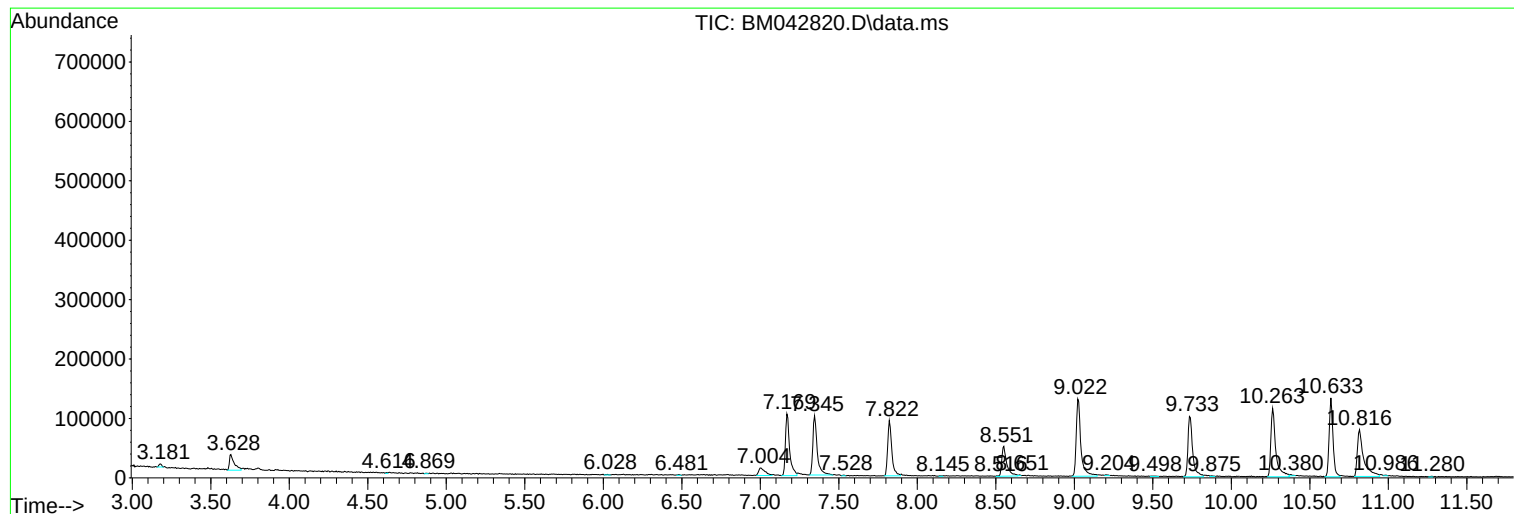

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042820.D
Acq On : 16 Nov 2023 23:57
Operator : MA/JU
Sample : 05268-11
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCKD3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042820.D
Acq On : 16 Nov 2023 23:57
Operator : MA/JU
Sample : 05268-11
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCKD3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc