

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
 Data File : BM042822.D
 Acq On : 17 Nov 2023 01:09
 Operator : MA/JU
 Sample : 05268-13
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCKD5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM042822.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.487	81	85	93	rBV5	5846	13385	1.29%	0.171%
2	3.628	107	109	116	rBV2	15972	28916	2.79%	0.370%
3	4.363	232	234	235	rVB2	2819	1601	0.15%	0.020%
4	4.640	279	281	284	rBV4	1397	1387	0.13%	0.018%
5	4.981	337	339	342	rBV4	1131	1159	0.11%	0.015%
6	6.216	547	549	552	rVB3	1402	1220	0.12%	0.016%
7	6.798	646	648	651	rVB3	1686	1451	0.14%	0.019%
8	6.828	651	653	657	rBV3	817	1286	0.12%	0.016%
9	7.004	678	683	693	rBV4	9019	26198	2.53%	0.335%
10	7.169	705	711	724	rBV	94560	176980	17.10%	2.265%
11	7.345	736	741	752	rBV	82881	155071	14.98%	1.984%
12	7.822	816	822	837	rVV	91754	171225	16.54%	2.191%
13	8.004	851	853	856	rVB3	1237	1040	0.10%	0.013%
14	8.045	858	860	865	rVB4	1004	1478	0.14%	0.019%
15	8.551	940	946	965	rBV	38429	91589	8.85%	1.172%
16	8.681	965	968	970	rVV4	1567	1996	0.19%	0.026%
17	8.704	970	972	976	rVB4	1353	1789	0.17%	0.023%
18	9.022	1019	1026	1039	rBV	111650	234443	22.65%	3.000%
19	9.733	1140	1147	1159	rBV	88408	182327	17.62%	2.333%
20	9.857	1167	1168	1175	rVB6	1250	1831	0.18%	0.023%
21	10.263	1231	1237	1254	rBV2	97499	218163	21.08%	2.792%
22	10.369	1254	1255	1259	rVV4	3775	4470	0.43%	0.057%
23	10.563	1285	1288	1292	rBV3	1026	1363	0.13%	0.017%
24	10.633	1294	1300	1313	rVV	131790	226641	21.90%	2.900%
25	10.816	1323	1331	1343	rBV2	70994	180998	17.49%	2.316%
26	11.698	1478	1481	1486	rVB2	1559	2038	0.20%	0.026%
27	13.322	1751	1757	1765	rVB3	1994	3939	0.38%	0.050%
28	13.669	1813	1816	1818	rBV2	1121	1127	0.11%	0.014%
29	13.898	1850	1855	1872	rBV	303959	461732	44.61%	5.909%
30	14.180	1896	1903	1916	rBV	322871	486668	47.02%	6.228%
31	14.480	1948	1954	1967	rBV	193509	295365	28.54%	3.780%
32	14.580	1969	1971	1974	rVB2	1672	1492	0.14%	0.019%
33	14.916	2027	2028	2033	rVB3	1149	1342	0.13%	0.017%
34	15.121	2060	2063	2067	rVB3	795	1089	0.11%	0.014%
35	15.474	2117	2123	2137	rBV	413055	637418	61.59%	8.157%
36	15.621	2143	2148	2166	rBV	104573	185816	17.95%	2.378%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
 Data File : BM042822.D
 Acq On : 17 Nov 2023 01:09
 Operator : MA/JU
 Sample : 05268-13
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCKD5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

37	17.233	2416	2422	2431	rBV	228528	332798	32.16%	4.259%
38	17.333	2433	2439	2457	rVV	491090	755477	73.00%	9.668%
39	17.474	2461	2463	2469	rVV6	2297	4252	0.41%	0.054%
40	17.921	2537	2539	2541	rBV	1318	1134	0.11%	0.015%
41	17.951	2541	2544	2546	rVB2	971	1071	0.10%	0.014%
42	17.974	2546	2548	2550	rBV3	1122	1201	0.12%	0.015%
43	18.009	2553	2554	2556	rBV2	1145	1130	0.11%	0.014%
44	18.086	2561	2567	2580	rBV4	16072	34062	3.29%	0.436%
45	18.180	2580	2583	2585	rVB3	1519	1796	0.17%	0.023%
46	18.462	2628	2631	2635	rBV4	1237	1801	0.17%	0.023%
47	18.827	2689	2693	2695	rBV3	993	1083	0.10%	0.014%
48	19.003	2721	2723	2726	rVB3	1211	1077	0.10%	0.014%
49	19.074	2730	2735	2736	rBV3	1427	1580	0.15%	0.020%
50	19.192	2751	2755	2757	rBV3	4399	4827	0.47%	0.062%
51	19.268	2763	2768	2773	rBV2	4164	7004	0.68%	0.090%
52	19.362	2781	2784	2791	rBV5	15126	26672	2.58%	0.341%
53	19.627	2823	2829	2840	rBV	754322	956945	92.46%	12.246%
54	19.762	2851	2852	2854	rBV2	1917	1105	0.11%	0.014%
55	19.921	2877	2879	2881	rBV3	1943	1415	0.14%	0.018%
56	19.998	2890	2892	2893	rBV2	1495	1262	0.12%	0.016%
57	20.392	2957	2959	2961	rBV2	2231	2325	0.22%	0.030%
58	21.415	3128	3133	3144	rBV	264220	395589	38.22%	5.062%
59	23.621	3501	3508	3522	rBV2	509942	1034961	100.00%	13.244%
60	23.774	3528	3534	3546	rVB	206505	437761	42.30%	5.602%




Sum of corrected areas: 7814361

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042822.D
Acq On : 17 Nov 2023 01:09
Operator : MA/JU
Sample : 05268-13
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCKD5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

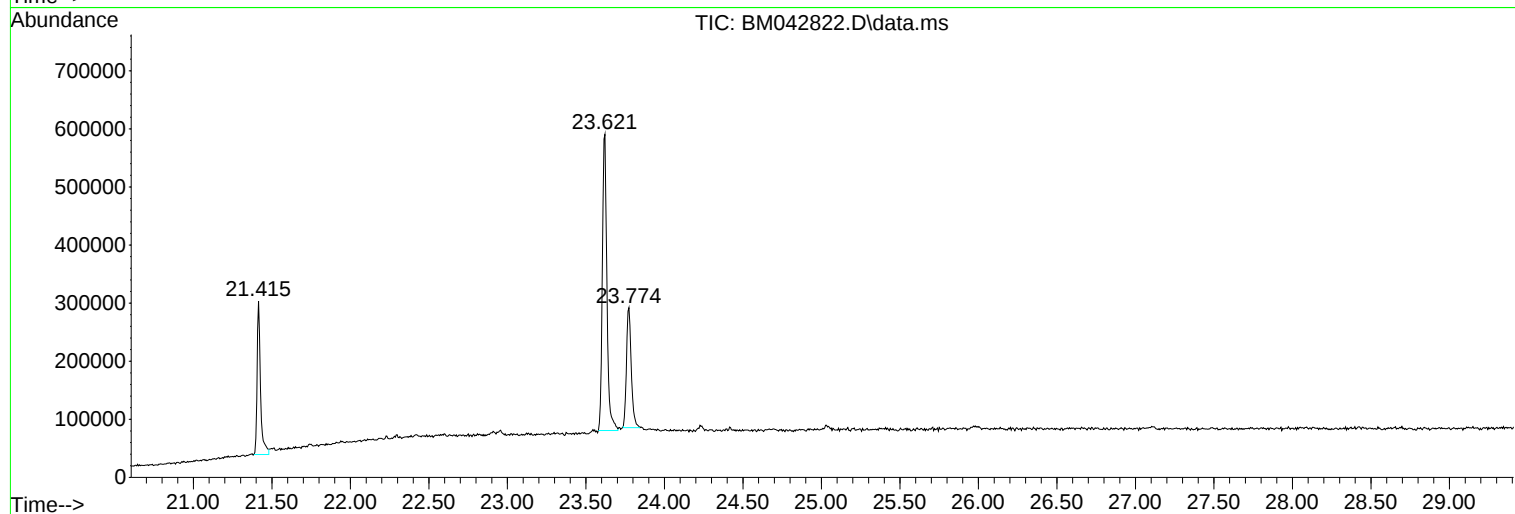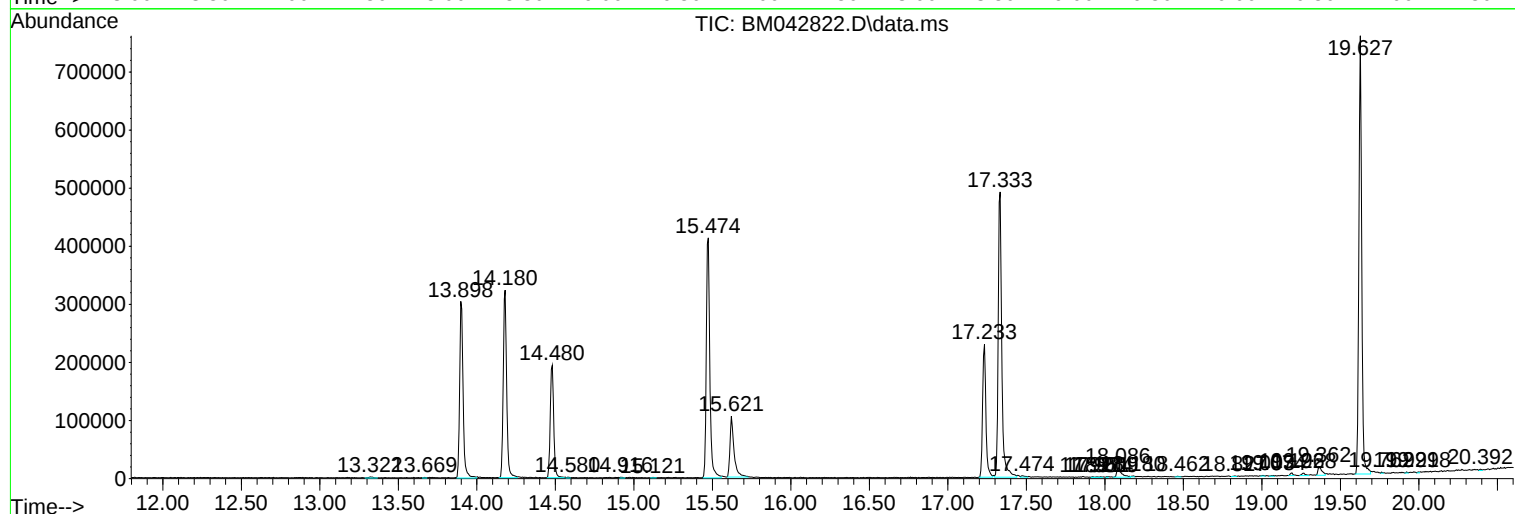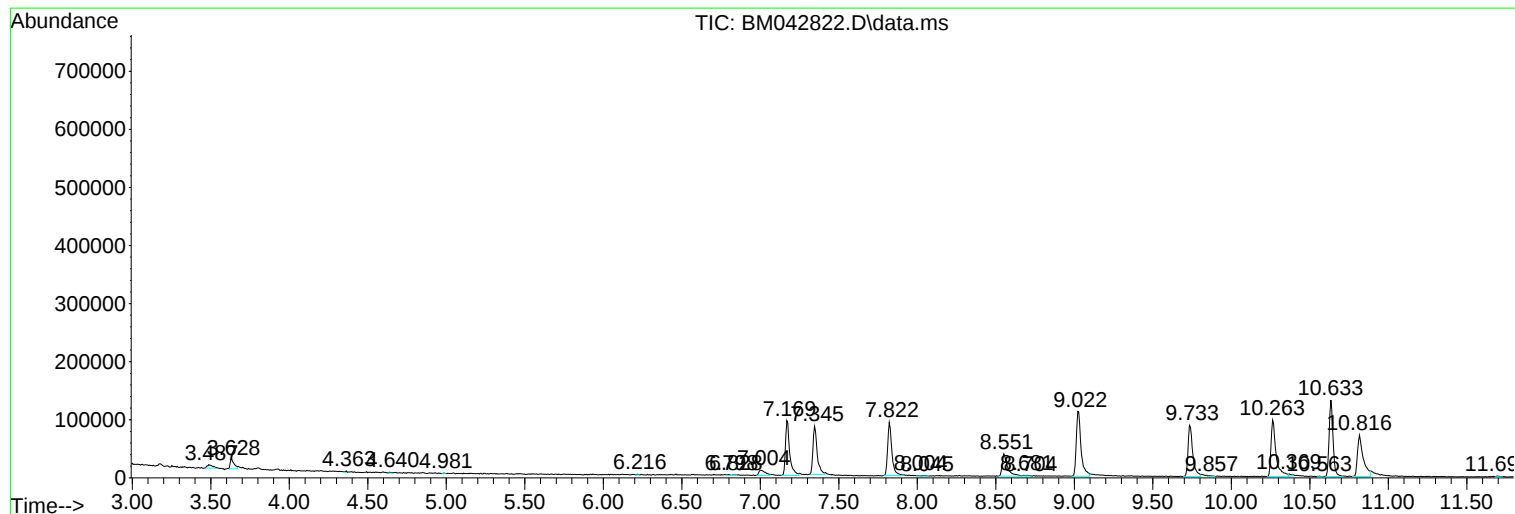

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042822.D
Acq On : 17 Nov 2023 01:09
Operator : MA/JU
Sample : 05268-13
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCKD5










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Dodecanoic acid Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
18.086	2.05 ng/ul	34062	Phenanthrene-d10	17.233

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Dodecanoic acid	200	C12H24O2	000143-07-7	50
2			n-Decanoic acid	172	C10H20O2	000334-48-5	43
3			9-Oxononanoic acid	172	C9H16O3	002553-17-5	43
4			Dodecanoic acid	200	C12H24O2	000143-07-7	43
5			Methyl isopropylidene-.beta.-d-a...	204	C9H16O5	1000129-88-1	43

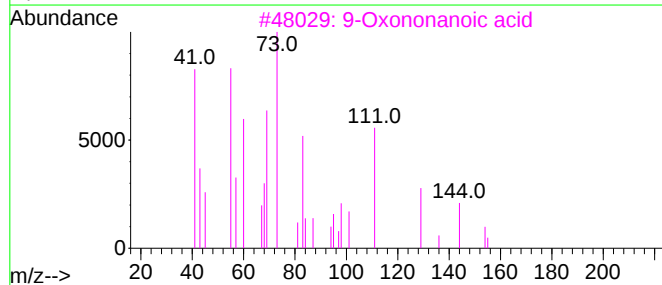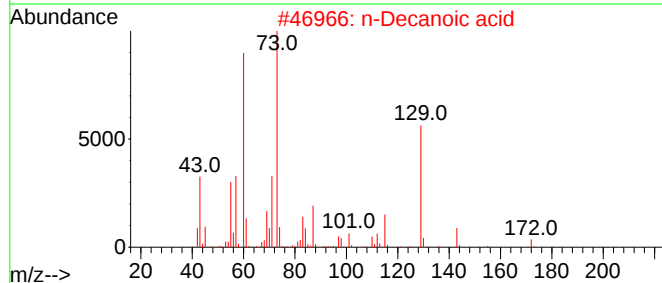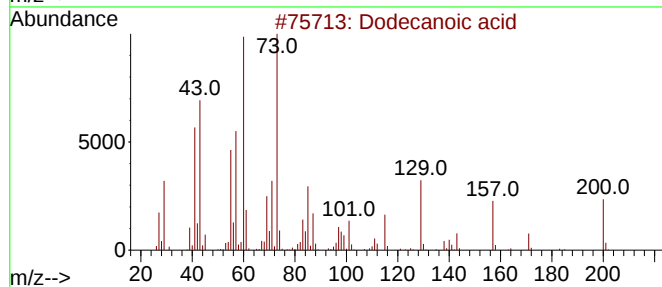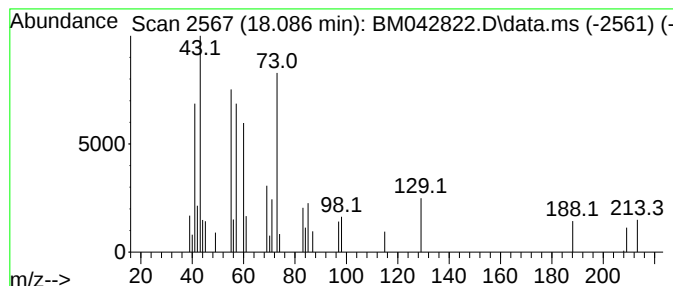

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042822.D
Acq On : 17 Nov 2023 01:09
Operator : MA/JU
Sample : 05268-13
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCKD5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Dodecanoic acid	18.086	2.0	ng/ul	34062	4	17.233	332798	20.0