

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
 Data File : BM042823.D
 Acq On : 17 Nov 2023 01:45
 Operator : MA/JU
 Sample : 05268-14
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCKD6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM042823.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	29	32	37	rVB5	5256	7118	0.83%	0.107%
2	3.628	106	109	116	rBV	24439	46994	5.50%	0.708%
3	4.716	292	294	297	rBV3	1413	1405	0.16%	0.021%
4	4.899	324	325	329	rVV3	1978	1303	0.15%	0.020%
5	4.952	331	334	336	rBV3	1086	1333	0.16%	0.020%
6	5.022	344	346	349	rBV3	1742	1689	0.20%	0.025%
7	5.375	404	406	407	rBV2	1110	988	0.12%	0.015%
8	5.534	430	433	437	rVB3	1367	2296	0.27%	0.035%
9	5.569	437	439	441	rBV3	1569	1592	0.19%	0.024%
10	6.328	564	568	570	rBV3	869	1040	0.12%	0.016%
11	7.004	677	683	691	rBV4	10039	27525	3.22%	0.415%
12	7.169	705	711	723	rBV	77707	149517	17.49%	2.253%
13	7.345	735	741	753	rBV	79538	150500	17.61%	2.268%
14	7.428	753	755	757	rVV3	2729	2431	0.28%	0.037%
15	7.457	759	760	762	rBV2	1238	881	0.10%	0.013%
16	7.822	816	822	834	rBV	86406	161465	18.89%	2.434%
17	8.004	851	853	858	rBV4	688	973	0.11%	0.015%
18	8.240	890	893	895	rBV4	1109	1153	0.13%	0.017%
19	8.398	917	920	923	rBV3	899	1274	0.15%	0.019%
20	8.551	941	946	958	rBV2	38392	90446	10.58%	1.363%
21	8.698	969	971	974	rVV4	1009	968	0.11%	0.015%
22	9.028	1020	1027	1040	rBV	92273	195370	22.86%	2.945%
23	9.169	1049	1051	1056	rVV4	1220	1439	0.17%	0.022%
24	9.334	1075	1079	1082	rBV4	688	1184	0.14%	0.018%
25	9.434	1092	1096	1098	rVB4	1018	1204	0.14%	0.018%
26	9.457	1098	1100	1104	rBV4	1224	1472	0.17%	0.022%
27	9.739	1141	1148	1163	rBV2	74812	157503	18.43%	2.374%
28	10.186	1222	1224	1226	rBV2	884	919	0.11%	0.014%
29	10.263	1230	1237	1248	rBV	84586	181332	21.21%	2.733%
30	10.557	1285	1287	1290	rVB3	1168	965	0.11%	0.015%
31	10.634	1293	1300	1306	rBV	121721	211874	24.79%	3.193%
32	10.681	1306	1308	1316	rVB5	9997	17873	2.09%	0.269%
33	10.816	1325	1331	1359	rBV2	77980	223497	26.15%	3.368%
34	11.357	1420	1423	1427	rVB2	946	1256	0.15%	0.019%
35	11.692	1477	1480	1485	rVV2	2250	3297	0.39%	0.050%
36	12.533	1620	1623	1626	rVB2	1562	1873	0.22%	0.028%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
 Data File : BM042823.D
 Acq On : 17 Nov 2023 01:45
 Operator : MA/JU
 Sample : 05268-14
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCKD6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

37	13.327	1754	1758	1761	rBV3	2278	3894	0.46%	0.059%
38	13.710	1820	1823	1825	rVV2	1009	959	0.11%	0.014%
39	13.898	1849	1855	1870	rBV	244589	376024	43.99%	5.667%
40	14.180	1896	1903	1916	rBV	270460	393407	46.03%	5.929%
41	14.392	1937	1939	1941	rBV2	952	1050	0.12%	0.016%
42	14.480	1948	1954	1961	rBV	180632	271157	31.72%	4.087%
43	14.539	1961	1964	1968	rVV4	4415	7198	0.84%	0.108%
44	14.604	1972	1975	1981	rVB4	953	2214	0.26%	0.033%
45	14.663	1981	1985	1986	rBV2	1143	1415	0.17%	0.021%
46	14.810	2005	2010	2015	rBV3	1239	2107	0.25%	0.032%
47	14.898	2022	2025	2028	rBV2	1559	1770	0.21%	0.027%
48	14.951	2031	2034	2037	rBV3	603	897	0.10%	0.014%
49	15.092	2056	2058	2064	rVB3	849	1482	0.17%	0.022%
50	15.216	2077	2079	2082	rBV2	1321	990	0.12%	0.015%
51	15.363	2102	2104	2108	rBV3	713	1011	0.12%	0.015%
52	15.474	2117	2123	2137	rBV	339988	519829	60.82%	7.835%
53	15.621	2143	2148	2163	rBV	71061	135058	15.80%	2.036%
54	15.780	2171	2175	2176	rVB2	651	855	0.10%	0.013%
55	16.357	2268	2273	2274	rVB4	970	923	0.11%	0.014%
56	16.410	2279	2282	2286	rVB3	855	969	0.11%	0.015%
57	16.739	2331	2338	2339	rVB2	924	1590	0.19%	0.024%
58	16.857	2355	2358	2360	rBV2	917	919	0.11%	0.014%
59	17.021	2383	2386	2389	rBV2	874	906	0.11%	0.014%
60	17.110	2399	2401	2406	rVB3	773	912	0.11%	0.014%
61	17.233	2416	2422	2433	rBV	201701	306434	35.85%	4.618%
62	17.333	2433	2439	2459	rVV	373788	595797	69.70%	8.980%
63	17.498	2466	2467	2471	rVB3	1474	1601	0.19%	0.024%
64	17.610	2485	2486	2490	rBV2	1200	922	0.11%	0.014%
65	18.051	2559	2561	2563	rVV2	1148	881	0.10%	0.013%
66	18.104	2563	2570	2575	rVV5	3662	9102	1.06%	0.137%
67	18.174	2578	2582	2583	rBV2	1491	1525	0.18%	0.023%
68	18.221	2587	2590	2591	rBV2	992	1084	0.13%	0.016%
69	18.504	2635	2638	2639	rBV2	1018	1035	0.12%	0.016%
70	18.709	2670	2673	2675	rBV3	815	882	0.10%	0.013%
71	19.004	2721	2723	2728	rVB3	943	1114	0.13%	0.017%
72	19.127	2741	2744	2745	rBV3	1174	1079	0.13%	0.016%
73	19.186	2752	2754	2757	rBV3	3102	3207	0.38%	0.048%
74	19.268	2762	2768	2773	rBV6	3264	6243	0.73%	0.094%
75	19.304	2773	2774	2778	rBV4	1132	1268	0.15%	0.019%
76	19.374	2784	2786	2792	rBV6	2218	3168	0.37%	0.048%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042823.D
Acq On : 17 Nov 2023 01:45
Operator : MA/JU
Sample : 05268-14
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCKD6

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Title : SVOA CALIBRATION

77	19.504	2806	2808	2810	rBV3	1723	1382	0.16%	0.021%
78	19.627	2823	2829	2841	rBV	582236	755050	88.33%	11.380%
79	20.151	2914	2918	2919	rBV3	3076	3628	0.42%	0.055%
80	21.415	3128	3133	3143	rBV	218415	331246	38.75%	4.992%
81	23.615	3500	3507	3521	rBV2	403063	854767	100.00%	12.883%
82	23.774	3528	3534	3543	rVB	182994	372176	43.54%	5.609%




Sum of corrected areas: 6635076

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042823.D
Acq On : 17 Nov 2023 01:45
Operator : MA/JU
Sample : 05268-14
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCKD6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

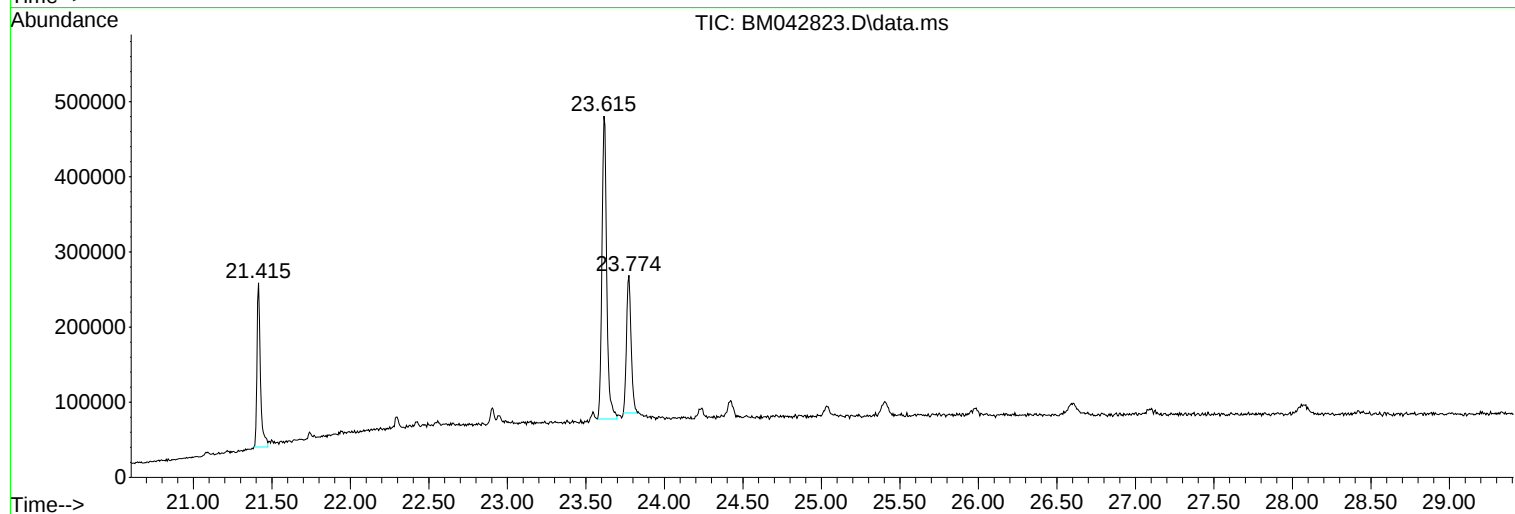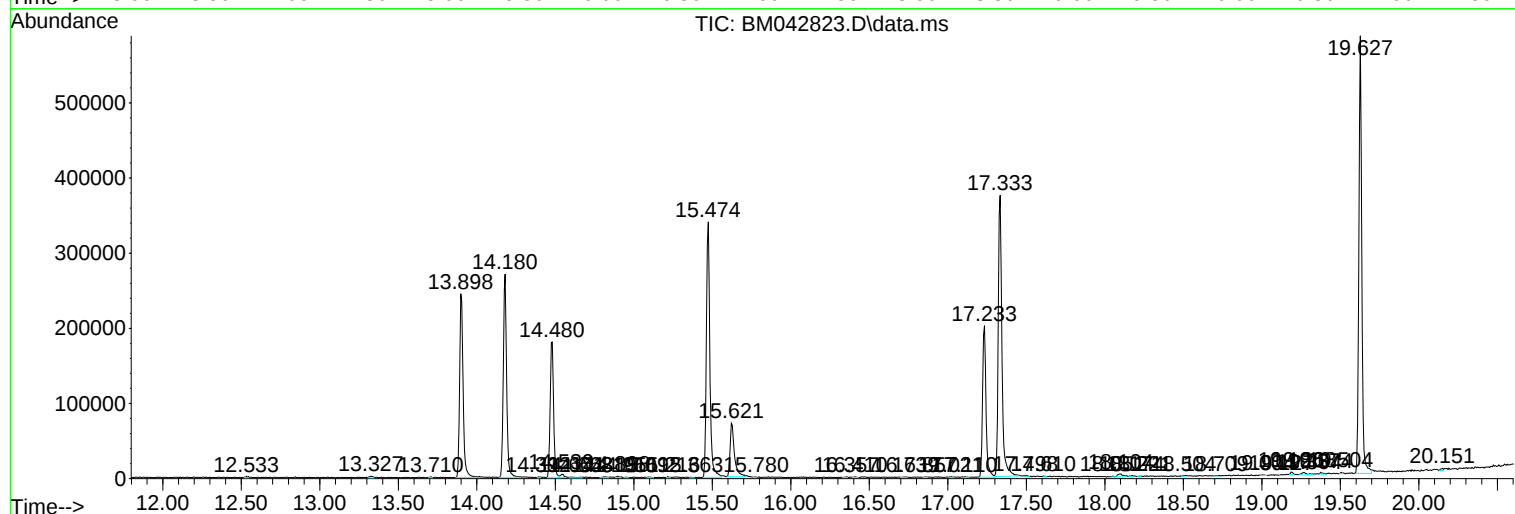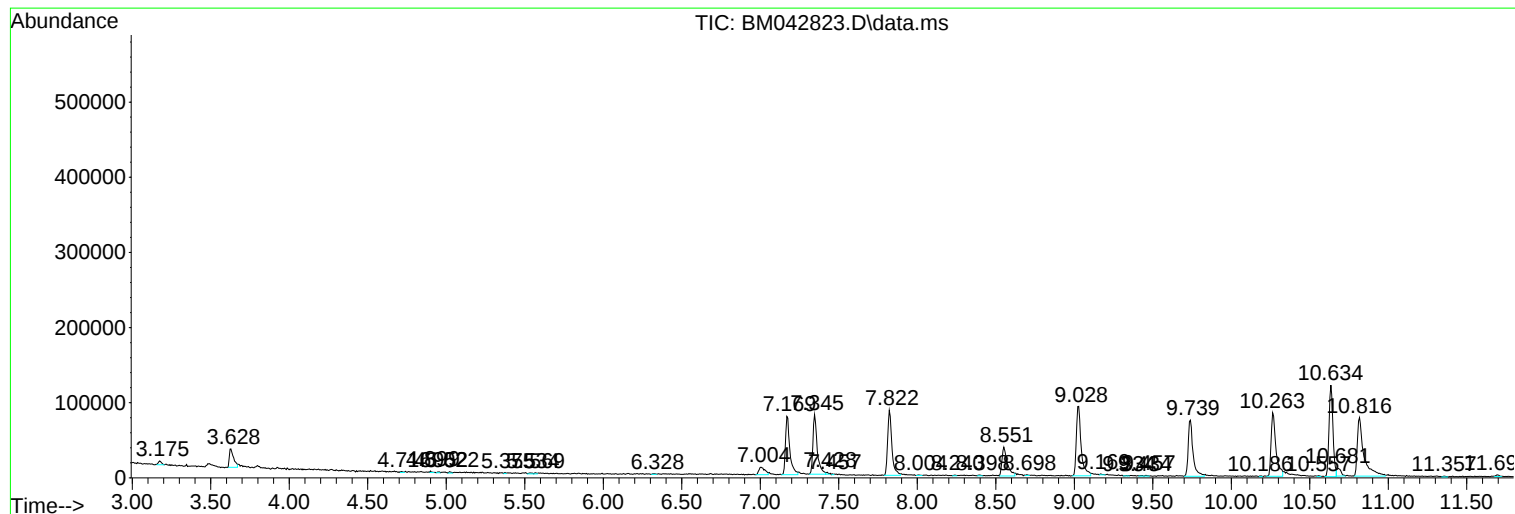

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042823.D
Acq On : 17 Nov 2023 01:45
Operator : MA/JU
Sample : 05268-14
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCKD6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042823.D
Acq On : 17 Nov 2023 01:45
Operator : MA/JU
Sample : 05268-14
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCKD6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc