

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
 Data File : BM042824.D
 Acq On : 17 Nov 2023 02:21
 Operator : MA/JU
 Sample : 05268-15
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCKD8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM042824.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	30	32	36	rVB3	5049	4853	0.39%	0.055%
2	3.481	82	84	85	rBV2	3639	3169	0.26%	0.036%
3	3.628	106	109	121	rBV	20836	38384	3.10%	0.433%
4	4.293	219	222	223	rBV3	2202	1903	0.15%	0.021%
5	4.693	288	290	297	rVB5	1684	2310	0.19%	0.026%
6	4.922	326	329	332	rBV4	2051	2264	0.18%	0.026%
7	5.510	427	429	431	rBV3	1172	1257	0.10%	0.014%
8	6.234	548	552	553	rBV4	1180	1294	0.10%	0.015%
9	6.634	616	620	621	rBV3	1091	1398	0.11%	0.016%
10	6.669	624	626	629	rVB4	1222	1366	0.11%	0.015%
11	6.998	677	682	695	rBV2	16886	43282	3.50%	0.488%
12	7.169	706	711	729	rBV	112276	205002	16.57%	2.313%
13	7.345	735	741	764	rVB	108646	213435	17.25%	2.409%
14	7.822	816	822	832	rBV	95115	172904	13.98%	1.951%
15	8.545	938	945	963	rBV	58677	129852	10.50%	1.465%
16	9.022	1020	1026	1044	rBV	136589	274960	22.22%	3.103%
17	9.151	1046	1048	1050	rVB2	1444	1333	0.11%	0.015%
18	9.734	1139	1147	1165	rBV2	115159	228901	18.50%	2.583%
19	10.263	1231	1237	1256	rBV	124553	274625	22.20%	3.099%
20	10.634	1294	1300	1310	rBV	135150	228857	18.50%	2.583%
21	10.816	1324	1331	1354	rBV2	74857	214394	17.33%	2.419%
22	11.698	1475	1481	1484	rVB3	1919	3295	0.27%	0.037%
23	13.333	1752	1759	1763	rBV5	1957	3424	0.28%	0.039%
24	13.898	1849	1855	1871	rBV	355980	530279	42.86%	5.984%
25	14.180	1896	1903	1912	rBV	370556	562212	45.44%	6.345%
26	14.480	1948	1954	1964	rBV	192456	291975	23.60%	3.295%
27	15.474	2116	2123	2135	rBV	494012	741035	59.90%	8.363%
28	15.621	2142	2148	2160	rBV	129520	225513	18.23%	2.545%
29	16.345	2267	2271	2275	rVB2	3309	3838	0.31%	0.043%
30	17.233	2416	2422	2433	rBV	230463	340730	27.54%	3.845%
31	17.333	2433	2439	2458	rVV	581815	862218	69.69%	9.730%
32	18.086	2564	2567	2570	rBV4	5554	8433	0.68%	0.095%
33	18.786	2684	2686	2688	rBV2	1785	1939	0.16%	0.022%
34	18.927	2707	2710	2713	rBV4	1520	2362	0.19%	0.027%
35	18.992	2720	2721	2725	rBV3	888	1312	0.11%	0.015%
36	19.192	2751	2755	2761	rBV5	4371	7596	0.61%	0.086%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042824.D
Acq On : 17 Nov 2023 02:21
Operator : MA/JU
Sample : 05268-15
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCKD8

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Title : SVOA CALIBRATION

37	19.262	2763	2767	2773	rBV2	4898	7764	0.63%	0.088%
38	19.368	2782	2785	2792	rBV6	3758	7472	0.60%	0.084%
39	19.445	2796	2798	2800	rBV3	1086	1322	0.11%	0.015%
40	19.627	2823	2829	2841	rBV	863207	1102763	89.13%	12.445%
41	19.874	2870	2871	2874	rBV3	1635	1691	0.14%	0.019%
42	20.256	2935	2936	2938	rBV2	2803	2098	0.17%	0.024%
43	20.333	2947	2949	2952	rBV4	2225	2802	0.23%	0.032%
44	21.415	3128	3133	3145	rBV	260907	391486	31.64%	4.418%
45	23.621	3501	3508	3524	rBV	626650	1237208	100.00%	13.962%
46	23.774	3527	3534	3546	rVB	220112	474676	38.37%	5.357%




Sum of corrected areas: 8861186

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042824.D
Acq On : 17 Nov 2023 02:21
Operator : MA/JU
Sample : 05268-15
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCKD8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

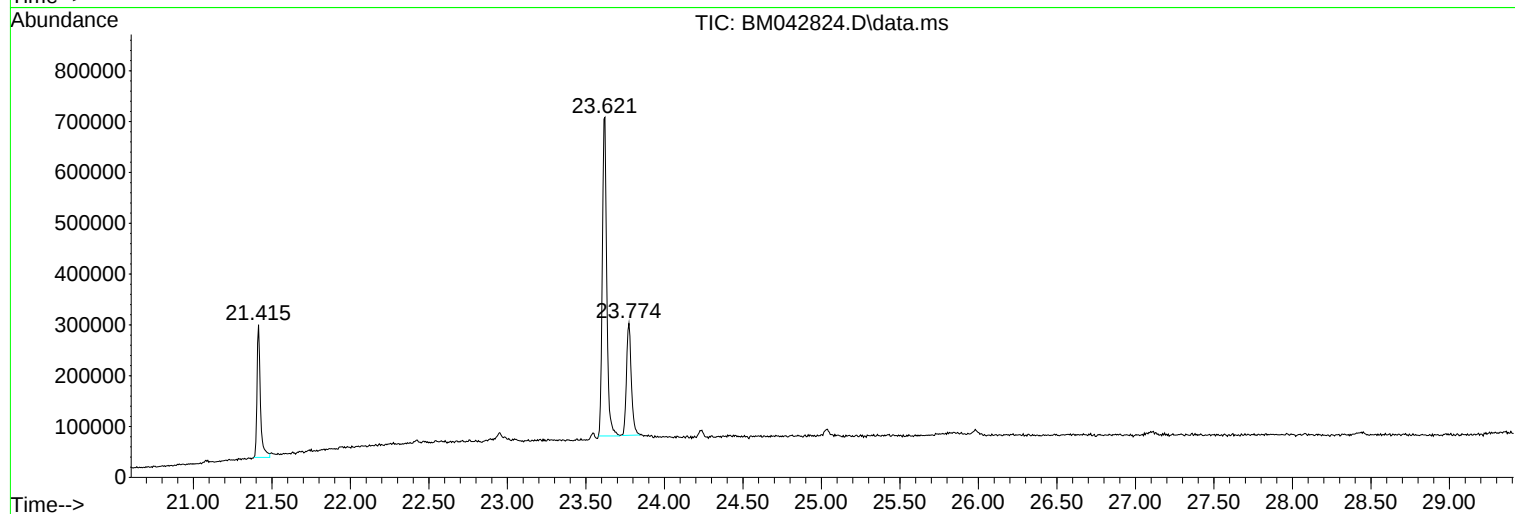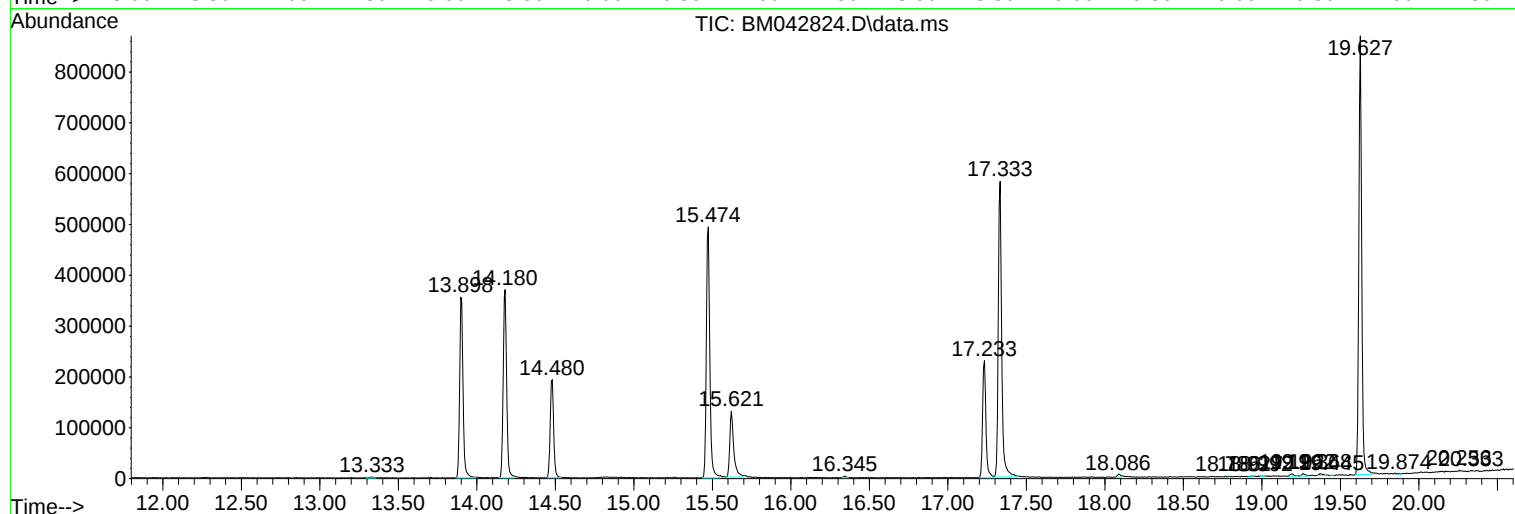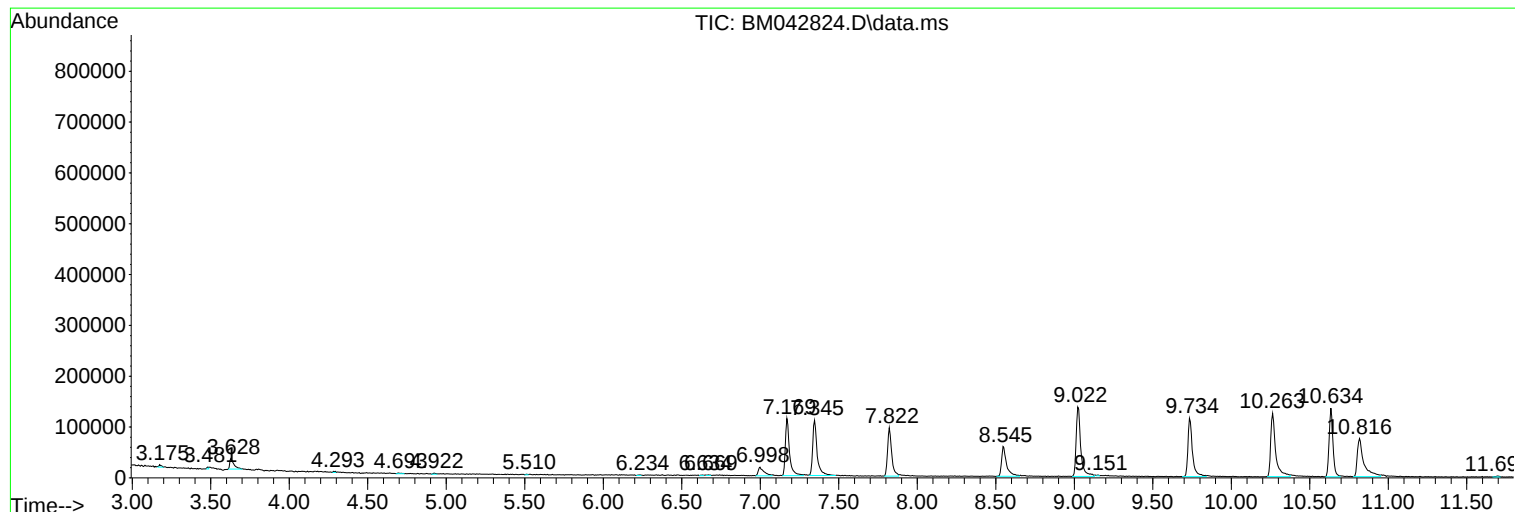

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042824.D
Acq On : 17 Nov 2023 02:21
Operator : MA/JU
Sample : 05268-15
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCKD8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042824.D
Acq On : 17 Nov 2023 02:21
Operator : MA/JU
Sample : 05268-15
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCKD8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc