

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
 Data File : BM042830.D
 Acq On : 17 Nov 2023 06:34
 Operator : MA/JU
 Sample : PB157053BL
 Misc :
 ALS Vial : 73 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK053

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM042830.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	29	32	41	rVB3	11926	20237	2.56%	0.252%
2	3.616	104	107	125	rBV	99056	173511	21.92%	2.165%
3	3.916	156	158	163	rVB5	2501	3724	0.47%	0.046%
4	4.610	274	276	280	rBV4	1587	1322	0.17%	0.016%
5	4.775	302	304	306	rVB3	1655	1255	0.16%	0.016%
6	4.869	318	320	321	rBV	1002	838	0.11%	0.010%
7	5.081	355	356	358	rBV2	1130	827	0.10%	0.010%
8	5.216	377	379	382	rVB4	1270	1288	0.16%	0.016%
9	5.281	388	390	393	rBV3	951	1095	0.14%	0.014%
10	5.551	434	436	438	rBV2	1239	1107	0.14%	0.014%
11	5.669	454	456	460	rVB3	892	1204	0.15%	0.015%
12	5.893	491	494	495	rBV3	976	1001	0.13%	0.012%
13	5.975	502	508	511	rBV5	1198	2682	0.34%	0.033%
14	6.063	522	523	525	rBV2	1600	884	0.11%	0.011%
15	6.263	555	557	562	rVB5	962	1428	0.18%	0.018%
16	6.393	578	579	580	rBV	1305	803	0.10%	0.010%
17	6.451	587	589	596	rVB6	1040	1365	0.17%	0.017%
18	6.634	615	620	621	rBV4	1525	1474	0.19%	0.018%
19	6.745	637	639	642	rBV3	1369	1177	0.15%	0.015%
20	6.793	645	647	649	rBV3	871	964	0.12%	0.012%
21	6.845	654	656	659	rBV4	1395	1833	0.23%	0.023%
22	6.987	675	680	700	rBV	116837	244295	30.86%	3.048%
23	7.169	706	711	724	rBV	104668	180417	22.79%	2.251%
24	7.340	734	740	760	rVB	137121	257422	32.51%	3.211%
25	7.751	807	810	813	rBV5	803	1033	0.13%	0.013%
26	7.822	816	822	833	rBV	109533	198991	25.13%	2.482%
27	7.922	838	839	843	rVB3	1633	1024	0.13%	0.013%
28	8.545	939	945	963	rBV	126411	264177	33.37%	3.296%
29	8.875	999	1001	1004	rVB3	1013	844	0.11%	0.011%
30	9.022	1020	1026	1044	rBV	120986	246182	31.09%	3.071%
31	9.186	1052	1054	1058	rVB4	780	854	0.11%	0.011%
32	9.292	1071	1072	1077	rVB2	987	1306	0.16%	0.016%
33	9.404	1088	1091	1092	rBV3	1063	1022	0.13%	0.013%
34	9.734	1140	1147	1159	rBV	100606	200252	25.29%	2.498%
35	10.263	1231	1237	1250	rBV	118634	250660	31.66%	3.127%
36	10.522	1279	1281	1283	rVB3	1158	933	0.12%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
 Data File : BM042830.D
 Acq On : 17 Nov 2023 06:34
 Operator : MA/JU
 Sample : PB157053BL
 Misc :
 ALS Vial : 73 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK053

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

37	10.633	1292	1300	1313	rBV	151747	263797	33.32%	3.291%
38	10.816	1325	1331	1356	rBV2	71359	205748	25.99%	2.567%
39	10.969	1356	1357	1361	rVV4	3059	2921	0.37%	0.036%
40	11.004	1361	1363	1368	rVB4	1188	1384	0.17%	0.017%
41	11.198	1395	1396	1400	rVB4	908	917	0.12%	0.011%
42	11.304	1412	1414	1417	rVB3	863	904	0.11%	0.011%
43	11.463	1439	1441	1443	rBV2	921	854	0.11%	0.011%
44	11.575	1458	1460	1463	rBV	627	810	0.10%	0.010%
45	11.686	1474	1479	1482	rBV	800	1197	0.15%	0.015%
46	11.769	1491	1493	1496	rVB2	1043	1084	0.14%	0.014%
47	11.804	1496	1499	1502	rBV4	849	1177	0.15%	0.015%
48	12.075	1542	1545	1549	rBV3	637	995	0.13%	0.012%
49	12.163	1559	1560	1563	rBV2	1162	1040	0.13%	0.013%
50	12.545	1621	1625	1626	rBV3	775	859	0.11%	0.011%
51	12.633	1637	1640	1643	rBV2	638	1007	0.13%	0.013%
52	13.327	1754	1758	1760	rBV2	1711	2088	0.26%	0.026%
53	13.398	1768	1770	1772	rBV2	728	873	0.11%	0.011%
54	13.539	1790	1794	1796	rVB4	891	1069	0.14%	0.013%
55	13.710	1817	1823	1826	rBV4	1008	1702	0.21%	0.021%
56	13.774	1832	1834	1837	rBV2	673	815	0.10%	0.010%
57	13.898	1850	1855	1872	rBV	279403	428581	54.13%	5.347%
58	14.063	1880	1883	1887	rBV3	680	980	0.12%	0.012%
59	14.092	1887	1888	1894	rVB4	1055	1343	0.17%	0.017%
60	14.180	1894	1903	1920	rBV	299416	464476	58.67%	5.794%
61	14.286	1920	1921	1927	rVV5	1071	1611	0.20%	0.020%
62	14.474	1947	1953	1966	rBV	216644	329283	41.59%	4.108%
63	14.568	1966	1969	1974	rVB7	1168	2149	0.27%	0.027%
64	14.757	1994	2001	2026	rBV6	19528	102216	12.91%	1.275%
65	15.039	2048	2049	2054	rVB3	1264	1246	0.16%	0.016%
66	15.157	2066	2069	2072	rVB2	896	1198	0.15%	0.015%
67	15.474	2116	2123	2135	rBV	376578	571473	72.18%	7.129%
68	15.621	2143	2148	2165	rBV2	76970	144504	18.25%	1.803%
69	15.933	2200	2201	2205	rVB3	869	970	0.12%	0.012%
70	16.004	2209	2213	2214	rBV3	852	847	0.11%	0.011%
71	16.368	2271	2275	2276	rBV3	776	966	0.12%	0.012%
72	16.827	2349	2353	2355	rBV4	621	959	0.12%	0.012%
73	16.915	2365	2368	2371	rVB4	797	1055	0.13%	0.013%
74	17.068	2392	2394	2398	rVB3	1080	1253	0.16%	0.016%
75	17.233	2416	2422	2432	rBV	255091	376654	47.57%	4.699%
76	17.333	2433	2439	2452	rVV	374243	590223	74.55%	7.363%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
 Data File : BM042830.D
 Acq On : 17 Nov 2023 06:34
 Operator : MA/JU
 Sample : PB157053BL
 Misc :
 ALS Vial : 73 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK053

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

77	17.651	2490	2493	2495	rBV3	990	985	0.12%	0.012%
78	17.909	2533	2537	2540	rBV5	694	1183	0.15%	0.015%
79	17.974	2546	2548	2549	rBV2	1085	1031	0.13%	0.013%
80	18.086	2564	2567	2570	rBV3	798	822	0.10%	0.010%
81	18.198	2582	2586	2588	rBV4	869	1095	0.14%	0.014%
82	18.374	2613	2616	2618	rBV3	873	809	0.10%	0.010%
83	18.415	2620	2623	2627	rBV4	845	1107	0.14%	0.014%
84	18.509	2636	2639	2641	rBV4	732	824	0.10%	0.010%
85	18.639	2659	2661	2664	rBV3	791	853	0.11%	0.011%
86	18.980	2717	2719	2720	rBV2	924	809	0.10%	0.010%
87	19.021	2724	2726	2729	rVB2	1544	1409	0.18%	0.018%
88	19.092	2735	2738	2741	rVB2	1414	1700	0.21%	0.021%
89	19.192	2750	2755	2758	rBV7	4187	6130	0.77%	0.076%
90	19.262	2763	2767	2771	rVV4	2330	4242	0.54%	0.053%
91	19.362	2782	2784	2787	rBV4	1139	911	0.12%	0.011%
92	19.409	2790	2792	2796	rBV5	938	1071	0.14%	0.013%
93	19.533	2812	2813	2814	rBV	1945	972	0.12%	0.012%
94	19.627	2824	2829	2843	rBV	545123	737279	93.12%	9.198%
95	19.739	2846	2848	2852	rVB5	2285	2432	0.31%	0.030%
96	21.415	3128	3133	3145	rBV	267948	417176	52.69%	5.204%
97	23.621	3501	3508	3526	rBV2	371538	791729	100.00%	9.877%
98	23.774	3528	3534	3545	rVB	217253	458623	57.93%	5.721%




Sum of corrected areas: 8015851

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042830.D
Acq On : 17 Nov 2023 06:34
Operator : MA/JU
Sample : PB157053BL
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK053

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

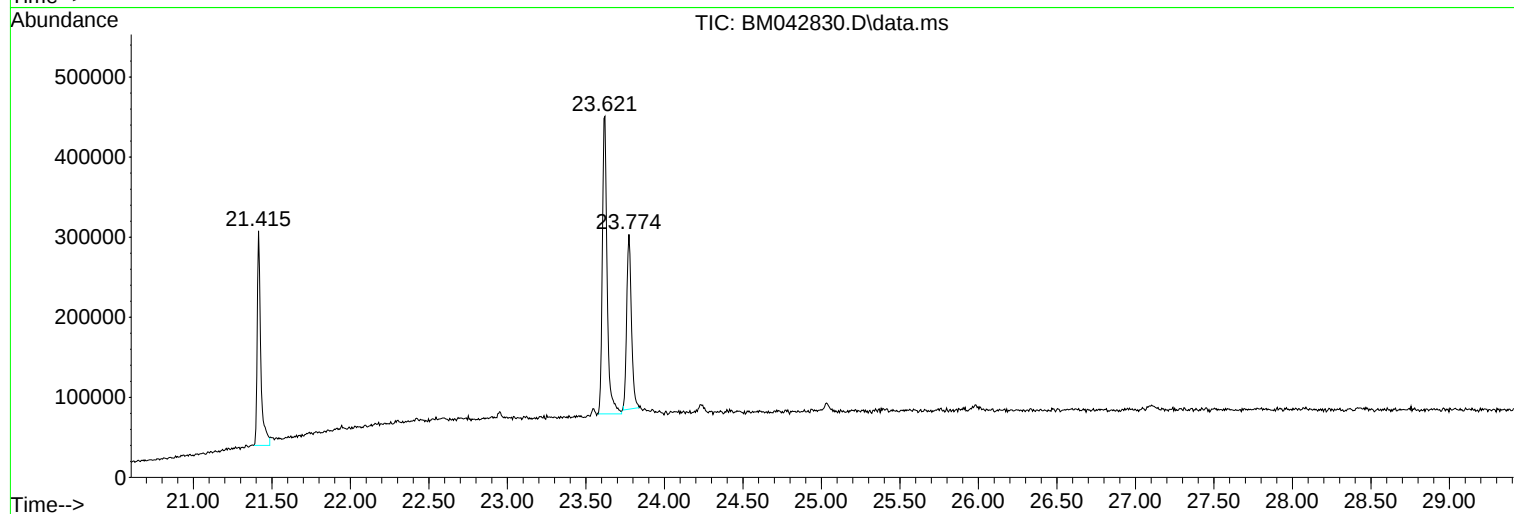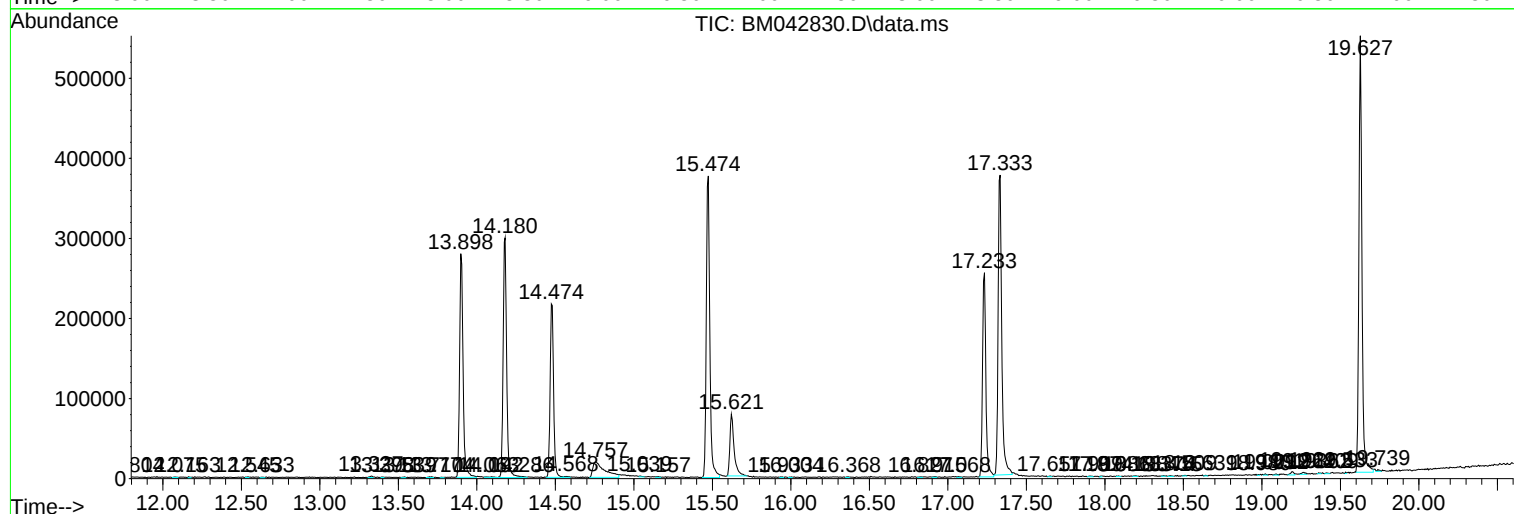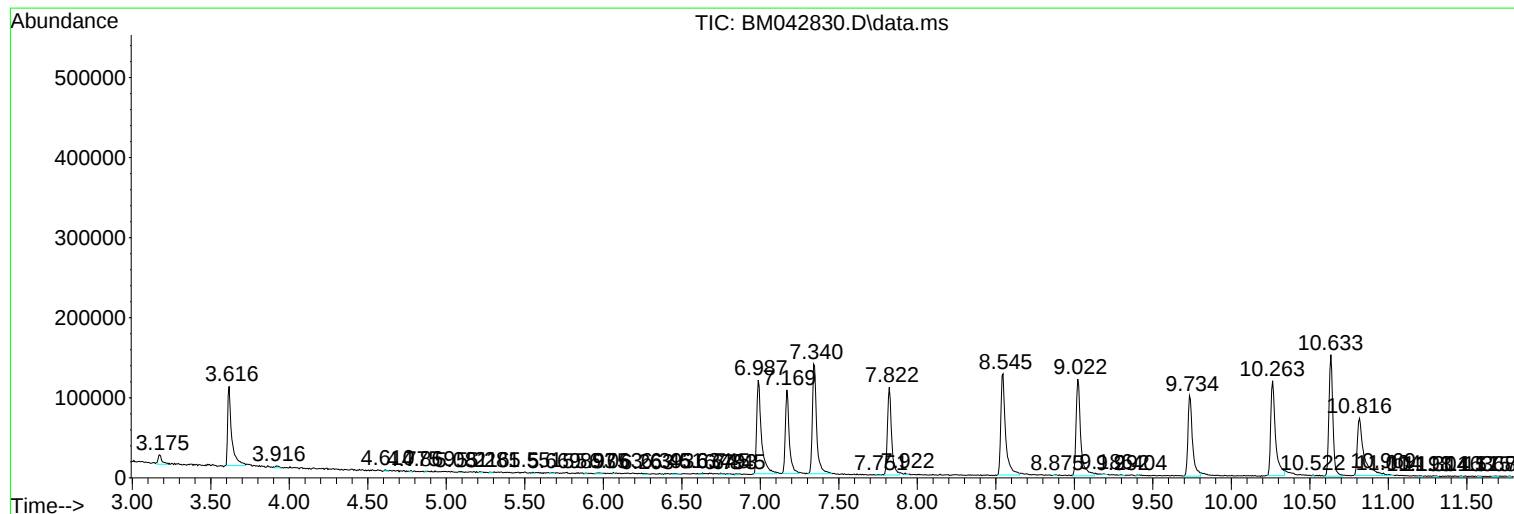

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042830.D
Acq On : 17 Nov 2023 06:34
Operator : MA/JU
Sample : PB157053BL
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK053

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042830.D
Acq On : 17 Nov 2023 06:34
Operator : MA/JU
Sample : PB157053BL
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK053

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------