

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
 Data File : BM042834.D
 Acq On : 17 Nov 2023 08:58
 Operator : MA/JU
 Sample : 05268-20
 Misc :
 ALS Vial : 77 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCKB5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM042834.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.169	29	31	37	rVB3	6209	8257	0.66%	0.084%
2	3.634	108	110	121	rBV5	8740	18798	1.49%	0.191%
3	3.799	134	138	141	rVB5	3256	5167	0.41%	0.053%
4	4.004	172	173	175	rBV	1904	1416	0.11%	0.014%
5	4.516	258	260	263	rVB3	1900	1664	0.13%	0.017%
6	6.998	677	682	694	rBV3	20816	53187	4.23%	0.541%
7	7.075	694	695	700	rVB4	1757	2329	0.19%	0.024%
8	7.169	705	711	729	rBV	133355	238458	18.95%	2.427%
9	7.345	735	741	751	rBV	131697	241411	19.19%	2.457%
10	7.734	803	807	811	rBV4	731	1439	0.11%	0.015%
11	7.822	816	822	833	rBV	108827	200675	15.95%	2.043%
12	8.545	940	945	957	rBV	77132	156535	12.44%	1.593%
13	9.022	1020	1026	1041	rBV	169506	323720	25.73%	3.295%
14	9.210	1056	1058	1063	rVB4	1978	2468	0.20%	0.025%
15	9.733	1140	1147	1163	rBV	138127	268067	21.31%	2.729%
16	10.257	1230	1236	1253	rBV	154715	324869	25.82%	3.307%
17	10.633	1293	1300	1314	rBV	149485	265341	21.09%	2.701%
18	10.810	1324	1330	1351	rBV2	89683	243787	19.38%	2.482%
19	11.480	1439	1444	1446	rVB2	970	1422	0.11%	0.014%
20	11.516	1446	1450	1453	rBV3	917	1300	0.10%	0.013%
21	11.692	1476	1480	1481	rBV4	1330	1383	0.11%	0.014%
22	12.269	1574	1578	1584	rVB3	919	1330	0.11%	0.014%
23	13.321	1753	1757	1761	rVB5	2181	3559	0.28%	0.036%
24	13.898	1849	1855	1868	rBV	428321	607294	48.27%	6.182%
25	13.986	1868	1870	1874	rVB3	1375	1964	0.16%	0.020%
26	14.174	1897	1902	1914	rBV	430586	651136	51.75%	6.628%
27	14.474	1946	1953	1964	rBV	229497	334470	26.58%	3.405%
28	14.786	2001	2006	2009	rBV3	1659	2650	0.21%	0.027%
29	14.968	2035	2037	2041	rBV3	832	1307	0.10%	0.013%
30	15.280	2088	2090	2098	rVB4	904	1785	0.14%	0.018%
31	15.474	2116	2123	2137	rBV	557230	841940	66.92%	8.571%
32	15.621	2143	2148	2172	rVV	150927	256349	20.37%	2.609%
33	17.104	2398	2400	2406	rBV3	696	1476	0.12%	0.015%
34	17.227	2416	2421	2432	rBV	259515	384843	30.59%	3.918%
35	17.327	2432	2438	2455	rVV	619453	932428	74.11%	9.492%
36	18.092	2564	2568	2570	rBV3	2999	4478	0.36%	0.046%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
 Data File : BM042834.D
 Acq On : 17 Nov 2023 08:58
 Operator : MA/JU
 Sample : 05268-20
 Misc :
 ALS Vial : 77 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCKB5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

37	18.345	2609	2611	2616	rVB4	921	1424	0.11%	0.014%
38	18.515	2638	2640	2645	rVV3	1573	1927	0.15%	0.020%
39	18.556	2645	2647	2652	rVB5	1181	1450	0.12%	0.015%
40	19.127	2740	2744	2749	rBV4	1726	3292	0.26%	0.034%
41	19.192	2749	2755	2759	rVV4	5585	8972	0.71%	0.091%
42	19.262	2764	2767	2771	rBV2	5724	8489	0.67%	0.086%
43	19.380	2784	2787	2792	rBV4	3050	5430	0.43%	0.055%
44	19.627	2823	2829	2842	rBV	923528	1186845	94.33%	12.081%
45	19.739	2846	2848	2849	rVB2	2264	1332	0.11%	0.014%
46	19.892	2872	2874	2875	rVB	2023	1346	0.11%	0.014%
47	19.909	2875	2877	2881	rBV3	1504	2282	0.18%	0.023%
48	20.127	2911	2914	2916	rBV4	1937	2532	0.20%	0.026%
49	20.639	2999	3001	3005	rBV5	3470	4065	0.32%	0.041%
50	21.415	3128	3133	3143	rBV	293284	439337	34.92%	4.472%
51	23.621	3501	3508	3524	rBV2	635948	1258219	100.00%	12.808%
52	23.774	3527	3534	3547	rVB	235327	508039	40.38%	5.172%




Sum of corrected areas: 9823683

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042834.D
Acq On : 17 Nov 2023 08:58
Operator : MA/JU
Sample : 05268-20
Misc :
ALS Vial : 77 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCKB5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

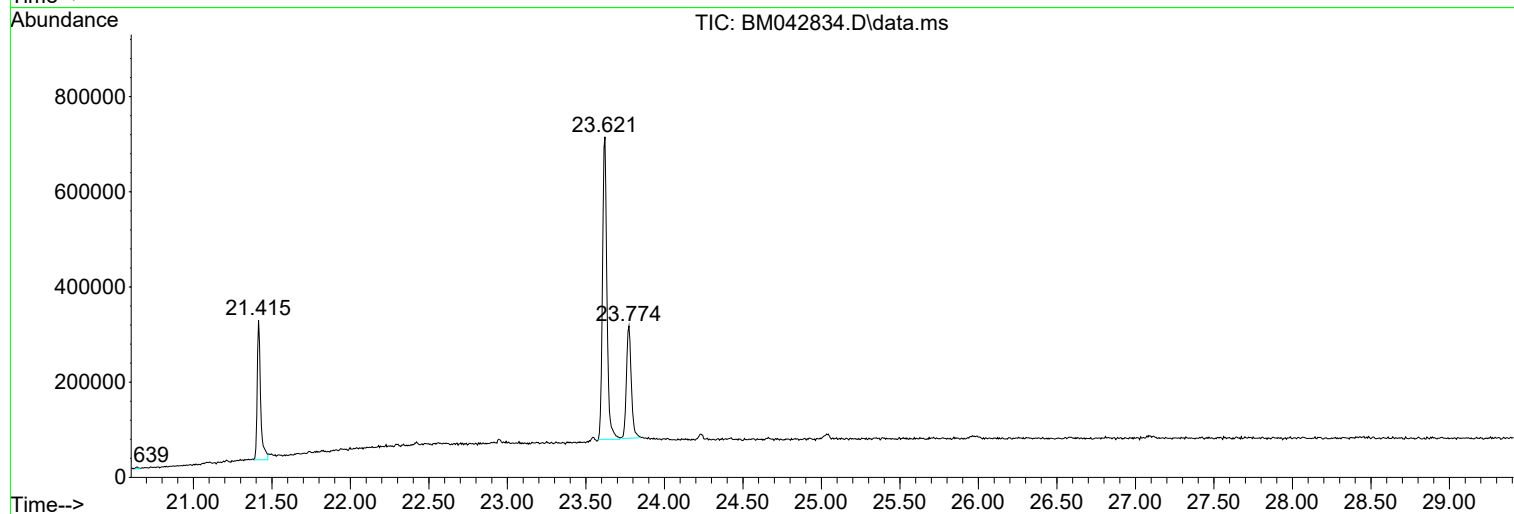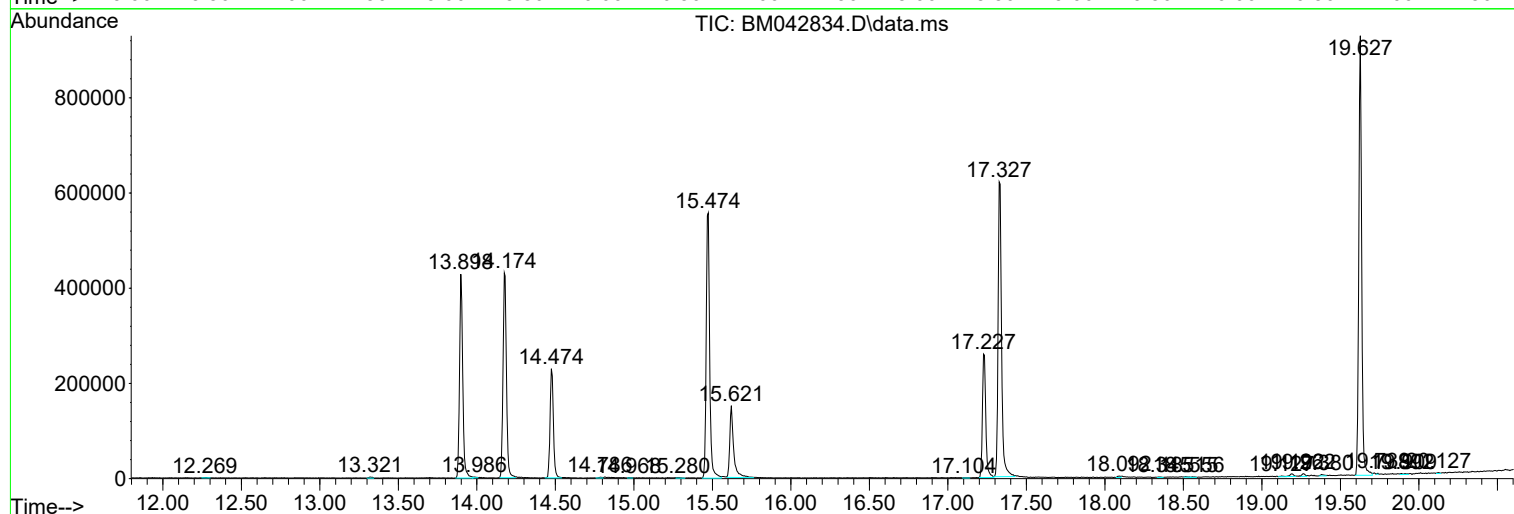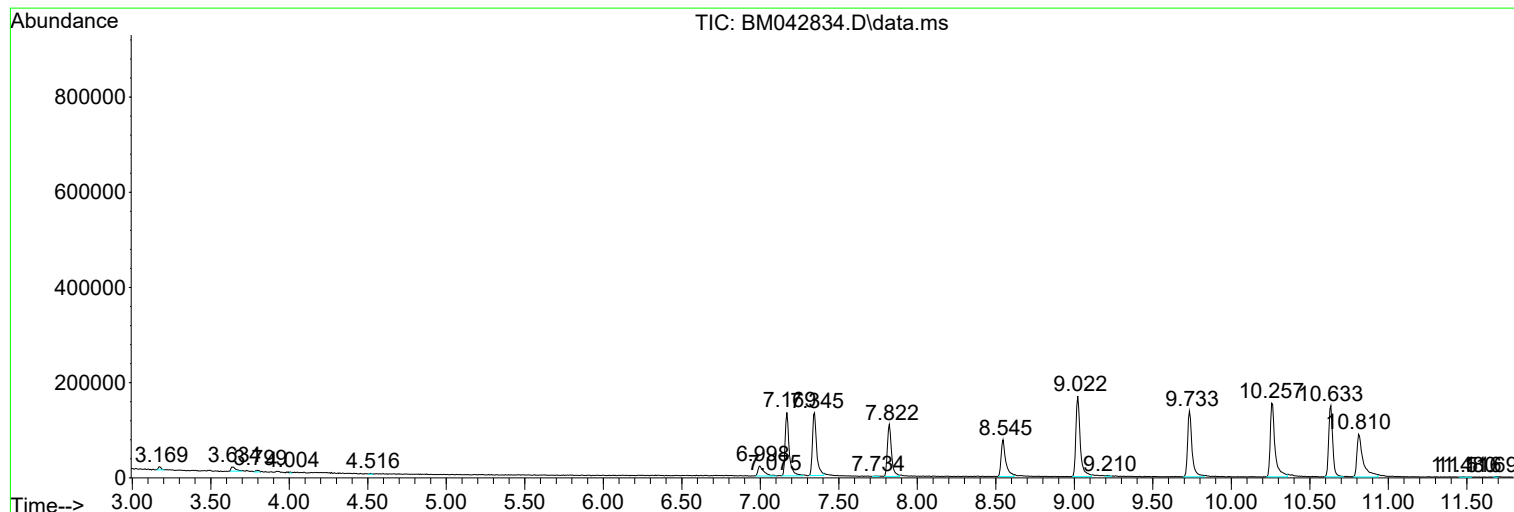

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042834.D
Acq On : 17 Nov 2023 08:58
Operator : MA/JU
Sample : 05268-20
Misc :
ALS Vial : 77 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCKB5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042834.D
Acq On : 17 Nov 2023 08:58
Operator : MA/JU
Sample : 05268-20
Misc :
ALS Vial : 77 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCKB5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc