

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
 Data File : BM042843.D
 Acq On : 17 Nov 2023 14:24
 Operator : MA/JU
 Sample : 05259-05
 Misc :
 ALS Vial : 91 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YCG93

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM042843.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	29	32	37	rVB4	7111	7951	0.94%	0.108%
2	3.622	105	108	118	rBV	32850	61776	7.29%	0.838%
3	3.798	136	138	142	rVB4	3675	4550	0.54%	0.062%
4	4.263	215	217	219	rBV3	1667	1027	0.12%	0.014%
5	4.287	219	221	226	rVB5	2083	2601	0.31%	0.035%
6	4.593	271	273	277	rVB5	1675	1429	0.17%	0.019%
7	5.298	392	393	396	rBV3	1379	1457	0.17%	0.020%
8	5.428	412	415	416	rBV2	1101	1199	0.14%	0.016%
9	5.816	479	481	484	rVB3	1266	1212	0.14%	0.016%
10	6.128	530	534	535	rBV4	769	958	0.11%	0.013%
11	6.328	566	568	570	rVB2	1375	925	0.11%	0.013%
12	6.522	600	601	605	rBV4	1459	1187	0.14%	0.016%
13	6.616	615	617	619	rBV2	918	980	0.12%	0.013%
14	6.998	678	682	693	rBV2	11555	30554	3.60%	0.415%
15	7.075	693	695	699	rVB4	1221	1239	0.15%	0.017%
16	7.169	705	711	720	rBV	90840	159942	18.86%	2.170%
17	7.345	735	741	761	rBV	89192	175630	20.71%	2.383%
18	7.469	761	762	766	rVB4	1955	1183	0.14%	0.016%
19	7.534	771	773	776	rVV3	1652	1475	0.17%	0.020%
20	7.634	786	790	791	rBV3	833	1230	0.15%	0.017%
21	7.675	795	797	799	rVB3	1273	1084	0.13%	0.015%
22	7.822	816	822	836	rBV	106587	195478	23.05%	2.652%
23	8.545	939	945	957	rBV	44897	100173	11.81%	1.359%
24	8.639	960	961	964	rVB3	1518	1217	0.14%	0.017%
25	8.710	971	973	976	rVB4	1203	1241	0.15%	0.017%
26	8.804	987	989	994	rVB4	978	1133	0.13%	0.015%
27	9.022	1020	1026	1043	rBV	111052	220608	26.02%	2.993%
28	9.204	1053	1057	1064	rVB5	4585	7796	0.92%	0.106%
29	9.733	1141	1147	1162	rBV2	89812	180716	21.31%	2.452%
30	9.927	1178	1180	1184	rVB4	1170	1276	0.15%	0.017%
31	10.263	1229	1237	1255	rBV2	98524	222821	26.28%	3.023%
32	10.375	1255	1256	1260	rVB4	2378	2261	0.27%	0.031%
33	10.475	1271	1273	1274	rBV	1311	895	0.11%	0.012%
34	10.633	1293	1300	1312	rBV	156301	261391	30.83%	3.546%
35	10.816	1324	1331	1358	rBV	71430	208682	24.61%	2.831%
36	11.398	1427	1430	1434	rBV5	883	1224	0.14%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
 Data File : BM042843.D
 Acq On : 17 Nov 2023 14:24
 Operator : MA/JU
 Sample : 05259-05
 Misc :
 ALS Vial : 91 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YCG93

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

37	11.698	1476	1481	1484	rVV4	1869	3149	0.37%	0.043%
38	11.880	1509	1512	1514	rBV3	1043	1153	0.14%	0.016%
39	12.063	1541	1543	1546	rVB2	1145	967	0.11%	0.013%
40	12.180	1560	1563	1566	rBV2	718	1008	0.12%	0.014%

41	12.310	1581	1585	1588	rVB3	786	1243	0.15%	0.017%
42	13.321	1754	1757	1763	rVB5	2526	3669	0.43%	0.050%
43	13.545	1792	1795	1798	rVB4	606	863	0.10%	0.012%
44	13.698	1817	1821	1825	rBV4	1432	2564	0.30%	0.035%
45	13.821	1841	1842	1845	rVB2	969	894	0.11%	0.012%

46	13.898	1850	1855	1873	rVV	274548	407062	48.01%	5.523%
47	14.015	1873	1875	1882	rVB5	944	1445	0.17%	0.020%
48	14.174	1896	1902	1916	rBV	282727	438430	51.71%	5.948%
49	14.474	1947	1953	1963	rBV	223698	330339	38.96%	4.482%
50	14.557	1965	1967	1973	rVB4	981	1365	0.16%	0.019%

51	14.833	2008	2014	2017	rBV4	1165	1624	0.19%	0.022%
52	14.904	2023	2026	2030	rVB4	911	1085	0.13%	0.015%
53	14.951	2032	2034	2036	rVB3	1080	937	0.11%	0.013%
54	15.192	2072	2075	2079	rBV3	1050	1144	0.13%	0.016%
55	15.268	2085	2088	2093	rVB4	920	1550	0.18%	0.021%

56	15.468	2117	2122	2136	rBV	359426	561211	66.19%	7.614%
57	15.621	2143	2148	2162	rBV2	76981	148879	17.56%	2.020%
58	15.745	2167	2169	2172	rVB2	1308	1337	0.16%	0.018%
59	15.998	2211	2212	2216	rBV2	878	908	0.11%	0.012%
60	16.039	2216	2219	2223	rVB4	850	1289	0.15%	0.017%

61	16.245	2251	2254	2257	rVB4	818	929	0.11%	0.013%
62	16.556	2303	2307	2309	rVB3	784	1118	0.13%	0.015%
63	17.068	2391	2394	2395	rBV2	1647	1004	0.12%	0.014%
64	17.227	2416	2421	2433	rBV	251337	373334	44.03%	5.065%
65	17.327	2433	2438	2453	rVV	401789	637327	75.17%	8.647%

66	17.445	2457	2458	2461	rVB4	1463	1142	0.13%	0.015%
67	17.674	2494	2497	2499	rVB4	1081	1148	0.14%	0.016%
68	17.768	2512	2513	2516	rVB3	1003	942	0.11%	0.013%
69	17.792	2516	2517	2520	rBV3	1228	1163	0.14%	0.016%
70	17.862	2524	2529	2532	rVV4	915	1643	0.19%	0.022%

71	17.915	2536	2538	2542	rVB3	936	1103	0.13%	0.015%
72	18.098	2565	2569	2570	rBV3	3897	4601	0.54%	0.062%
73	18.350	2610	2612	2615	rBV3	1556	1153	0.14%	0.016%
74	18.374	2615	2616	2619	rBV3	1164	1124	0.13%	0.015%
75	18.509	2636	2639	2643	rBV6	1542	1717	0.20%	0.023%

76	18.550	2643	2646	2650	rVB5	1124	1607	0.19%	0.022%
----	--------	------	------	------	------	------	------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
 Data File : BM042843.D
 Acq On : 17 Nov 2023 14:24
 Operator : MA/JU
 Sample : 05259-05
 Misc :
 ALS Vial : 91 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YCG93

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

77	18.692	2667	2670	2671	rBV2	1315	1027	0.12%	0.014%
78	18.733	2673	2677	2679	rVV3	1194	1615	0.19%	0.022%
79	18.774	2683	2684	2688	rVB2	1557	1333	0.16%	0.018%
80	18.815	2688	2691	2692	rBV3	1120	1193	0.14%	0.016%
81	18.909	2706	2707	2711	rVB4	1343	1276	0.15%	0.017%
82	18.945	2711	2713	2715	rBV3	949	1112	0.13%	0.015%
83	18.980	2718	2719	2723	rBV4	1042	1222	0.14%	0.017%
84	19.080	2732	2736	2738	rBV4	1620	1906	0.22%	0.026%
85	19.139	2745	2746	2750	rBV3	826	919	0.11%	0.012%
86	19.192	2752	2755	2758	rVB4	4136	4881	0.58%	0.066%
87	19.262	2763	2767	2768	rBV4	2764	3659	0.43%	0.050%
88	19.380	2782	2787	2789	rBV4	2899	4497	0.53%	0.061%
89	19.445	2796	2798	2801	rVB3	1939	1877	0.22%	0.025%
90	19.468	2801	2802	2805	rBV3	1684	1988	0.23%	0.027%
91	19.627	2822	2829	2839	rBV	601524	787095	92.83%	10.678%
92	19.950	2882	2884	2886	rBV2	1693	1690	0.20%	0.023%
93	21.415	3128	3133	3143	rBV	274092	422481	49.83%	5.732%
94	23.615	3501	3507	3525	rBV	403102	847902	100.00%	11.503%
95	23.774	3528	3534	3544	rVV	230839	471565	55.62%	6.398%




Sum of corrected areas: 7370909

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042843.D
Acq On : 17 Nov 2023 14:24
Operator : MA/JU
Sample : 05259-05
Misc :
ALS Vial : 91 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YCG93

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

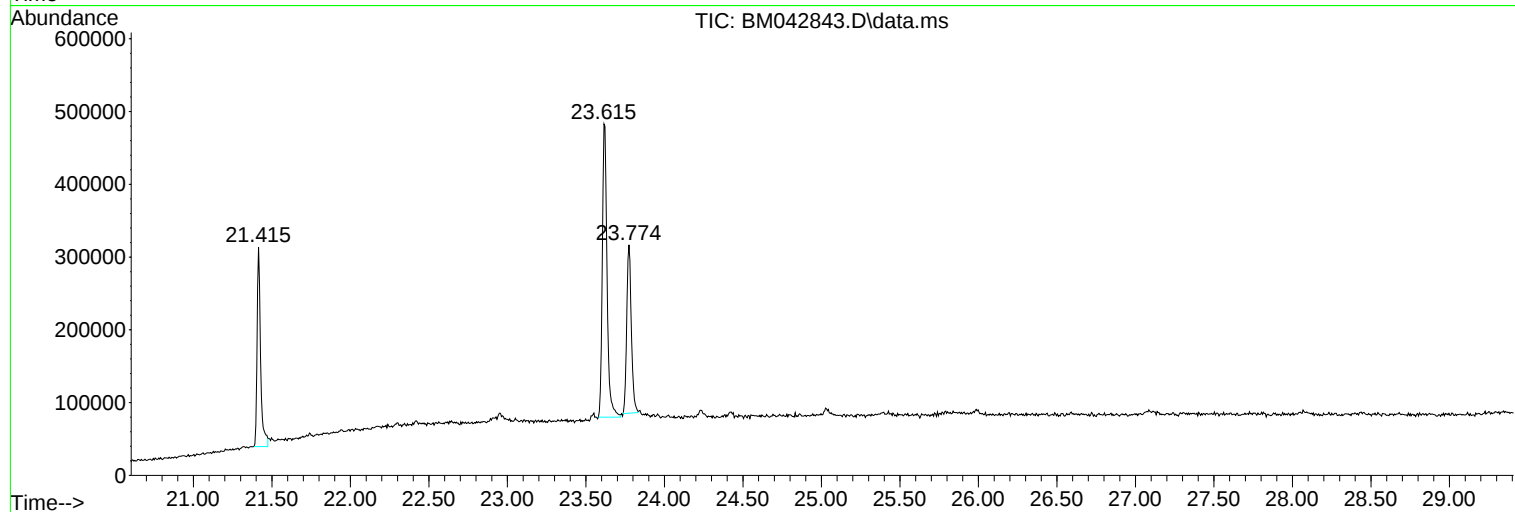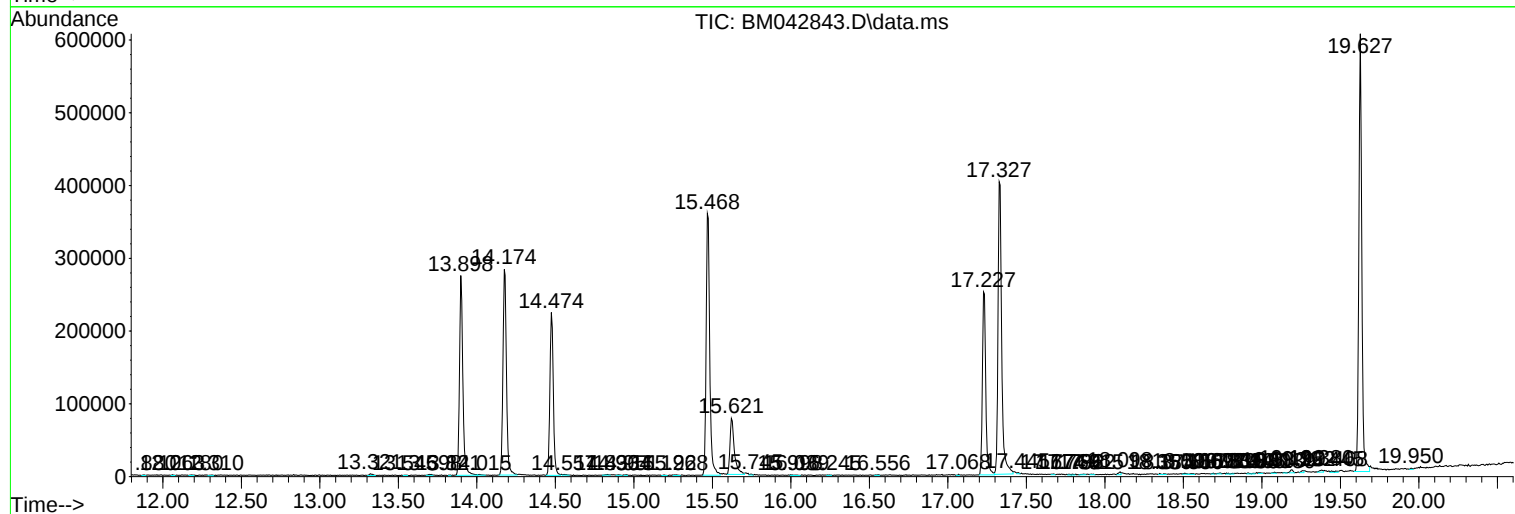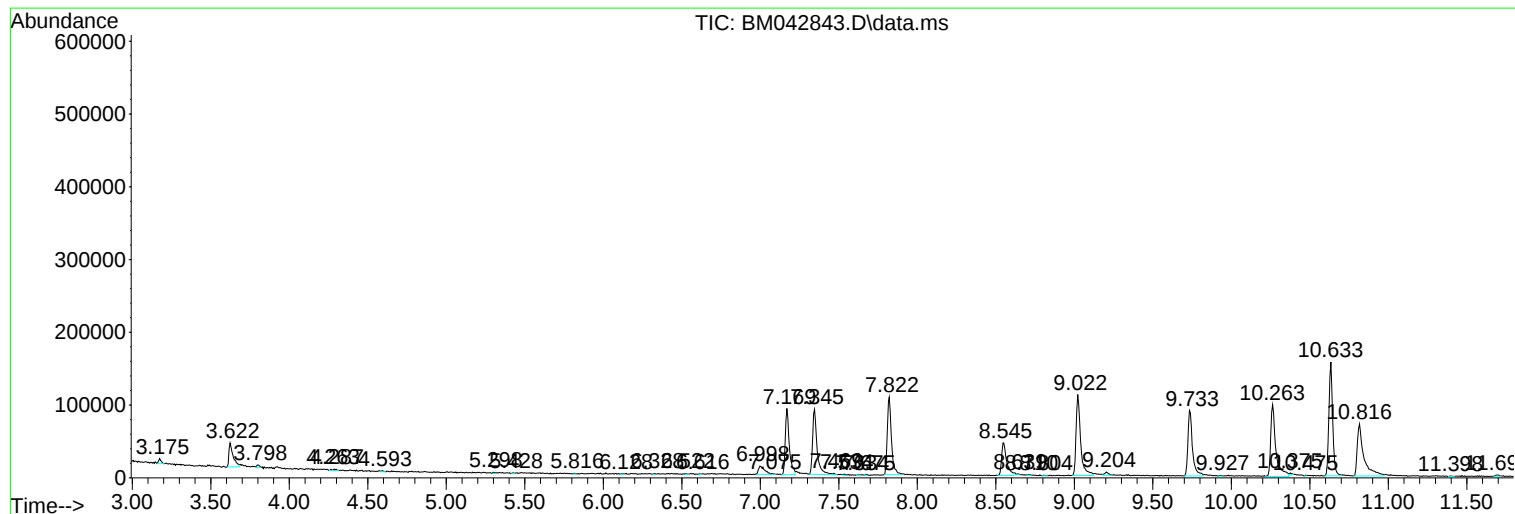

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042843.D
Acq On : 17 Nov 2023 14:24
Operator : MA/JU
Sample : 05259-05
Misc :
ALS Vial : 91 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YCG93

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042843.D
Acq On : 17 Nov 2023 14:24
Operator : MA/JU
Sample : 05259-05
Misc :
ALS Vial : 91 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YCG93

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc