

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
 Data File : BM042846.D
 Acq On : 17 Nov 2023 16:13
 Operator : MA/JU
 Sample : PB157005BL
 Misc :
 ALS Vial : 87 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK005

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM042846.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	29	32	36	rBV	11572	13209	1.46%	0.156%
2	3.610	103	106	119	rBV	144954	244038	26.92%	2.883%
3	4.863	317	319	321	rBV2	1666	1676	0.18%	0.020%
4	5.093	356	358	360	rBV3	1270	1094	0.12%	0.013%
5	5.257	384	386	389	rBV5	1046	1354	0.15%	0.016%
6	5.440	415	417	419	rBV2	933	927	0.10%	0.011%
7	5.610	445	446	448	rVB2	1547	982	0.11%	0.012%
8	6.440	585	587	589	rVB3	1406	1011	0.11%	0.012%
9	6.475	589	593	595	rBV4	1200	1653	0.18%	0.020%
10	6.622	616	618	621	rVV4	1225	994	0.11%	0.012%
11	6.651	621	623	626	rVB3	1008	1120	0.12%	0.013%
12	6.716	632	634	637	rBV4	876	1095	0.12%	0.013%
13	6.846	652	656	659	rBV4	870	1493	0.16%	0.018%
14	6.987	674	680	695	rBV	151502	295052	32.55%	3.486%
15	7.169	705	711	723	rBV	129766	221454	24.43%	2.617%
16	7.340	734	740	753	rBV	172926	303013	33.43%	3.580%
17	7.822	816	822	838	rBV	81073	154905	17.09%	1.830%
18	8.263	896	897	905	rVB6	623	983	0.11%	0.012%
19	8.375	913	916	917	rBV2	885	1041	0.11%	0.012%
20	8.445	926	928	931	rVB3	1020	1006	0.11%	0.012%
21	8.540	937	944	959	rBV	159484	316948	34.97%	3.745%
22	8.692	968	970	975	rVB6	1835	1887	0.21%	0.022%
23	9.022	1018	1026	1043	rBV	152345	292653	32.29%	3.458%
24	9.734	1140	1147	1164	rBV	127140	245897	27.13%	2.905%
25	10.257	1231	1236	1254	rBV	146572	318059	35.09%	3.758%
26	10.439	1265	1267	1270	rVB3	1479	1461	0.16%	0.017%
27	10.634	1293	1300	1310	rBV	110934	194579	21.47%	2.299%
28	10.810	1324	1330	1347	rBV	118129	287037	31.67%	3.392%
29	10.998	1361	1362	1367	rVB3	1784	1615	0.18%	0.019%
30	11.075	1373	1375	1378	rBV4	1021	1081	0.12%	0.013%
31	11.157	1386	1389	1392	rVB3	940	1165	0.13%	0.014%
32	11.469	1438	1442	1444	rBV2	957	1159	0.13%	0.014%
33	12.222	1567	1570	1573	rBV2	893	989	0.11%	0.012%
34	12.704	1649	1652	1654	rVV3	816	1094	0.12%	0.013%
35	13.327	1753	1758	1762	rBV6	1539	2581	0.28%	0.030%
36	13.898	1850	1855	1866	rVV	330650	472826	52.16%	5.587%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
 Data File : BM042846.D
 Acq On : 17 Nov 2023 16:13
 Operator : MA/JU
 Sample : PB157005BL
 Misc :
 ALS Vial : 87 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK005

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
 Title : SVOA CALIBRATION

37	14.174	1896	1902	1912	rBV	356015	531089	58.59%	6.275%
38	14.327	1926	1928	1935	rVB4	818	1430	0.16%	0.017%
39	14.474	1947	1953	1963	rVV2	166220	241955	26.69%	2.859%
40	14.539	1963	1964	1969	rVB3	1272	1829	0.20%	0.022%
41	14.745	1993	1999	2012	rBV5	25703	100532	11.09%	1.188%
42	14.892	2023	2024	2027	rVB2	1516	1175	0.13%	0.014%
43	14.998	2039	2042	2044	rVB3	1025	1062	0.12%	0.013%
44	15.057	2050	2052	2056	rVB4	1064	1103	0.12%	0.013%
45	15.257	2082	2086	2087	rBV2	1088	949	0.10%	0.011%
46	15.469	2116	2122	2137	rBV	440735	656123	72.39%	7.753%
47	15.621	2143	2148	2160	rBV	94747	172680	19.05%	2.040%
48	15.704	2160	2162	2168	rVB5	3065	4573	0.50%	0.054%
49	16.345	2267	2271	2273	rBV3	969	1232	0.14%	0.015%
50	16.392	2276	2279	2281	rVV2	848	1186	0.13%	0.014%
51	16.945	2371	2373	2375	rVB2	1388	942	0.10%	0.011%
52	16.992	2380	2381	2384	rBV2	1181	1061	0.12%	0.013%
53	17.045	2386	2390	2392	rVB3	922	1292	0.14%	0.015%
54	17.227	2416	2421	2433	rBV	185008	272854	30.10%	3.224%
55	17.327	2433	2438	2455	rVV	439131	673688	74.32%	7.960%
56	17.615	2485	2487	2489	rVB3	1103	973	0.11%	0.011%
57	17.792	2514	2517	2519	rVB2	944	1117	0.12%	0.013%
58	18.127	2569	2574	2575	rBV3	937	1486	0.16%	0.018%
59	18.168	2578	2581	2583	rVB3	713	953	0.11%	0.011%
60	18.333	2606	2609	2612	rVB3	908	1121	0.12%	0.013%
61	18.621	2654	2658	2661	rVB6	917	1242	0.14%	0.015%
62	18.645	2661	2662	2666	rBV4	841	1178	0.13%	0.014%
63	19.080	2735	2736	2738	rBV2	1450	1202	0.13%	0.014%
64	19.192	2752	2755	2758	rBV5	3783	5046	0.56%	0.060%
65	19.257	2763	2766	2771	rVV4	2334	4018	0.44%	0.047%
66	19.321	2775	2777	2779	rVB3	1352	998	0.11%	0.012%
67	19.627	2823	2829	2841	rBV	606473	825944	91.12%	9.759%
68	21.415	3129	3133	3148	rBV	167297	300441	33.15%	3.550%
69	23.621	3501	3508	3520	rBV2	435144	906414	100.00%	10.710%
70	23.774	3528	3534	3550	rVB	155070	355349	39.20%	4.199%




Sum of corrected areas: 8463368

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042846.D
Acq On : 17 Nov 2023 16:13
Operator : MA/JU
Sample : PB157005BL
Misc :
ALS Vial : 87 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK005

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

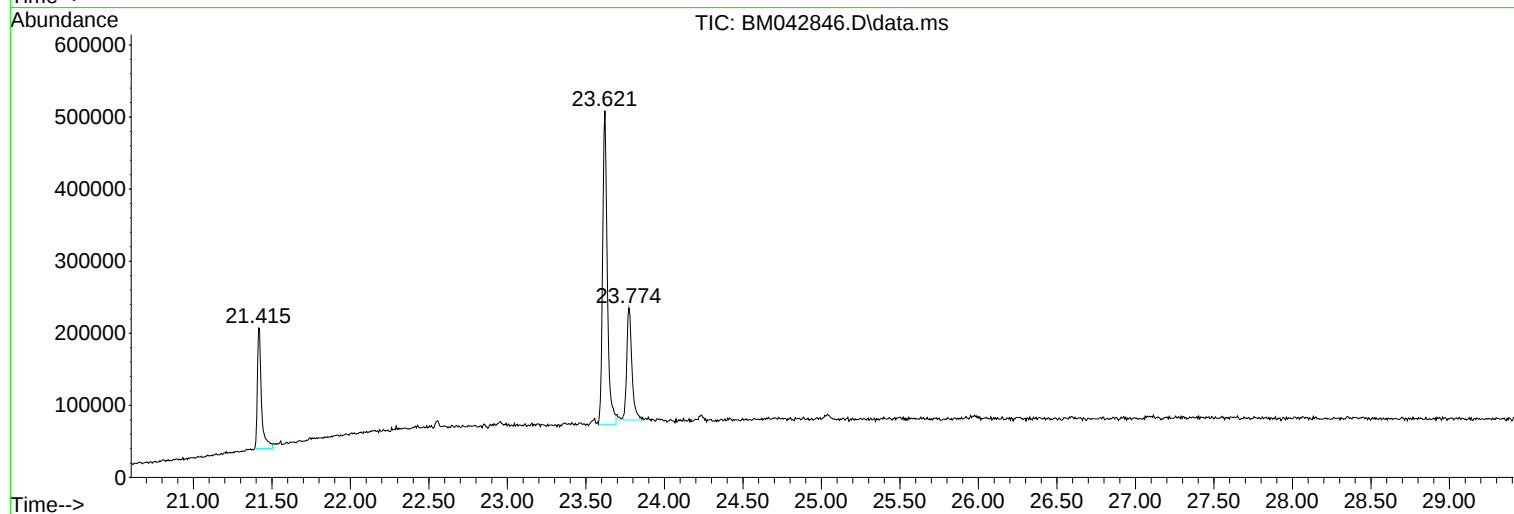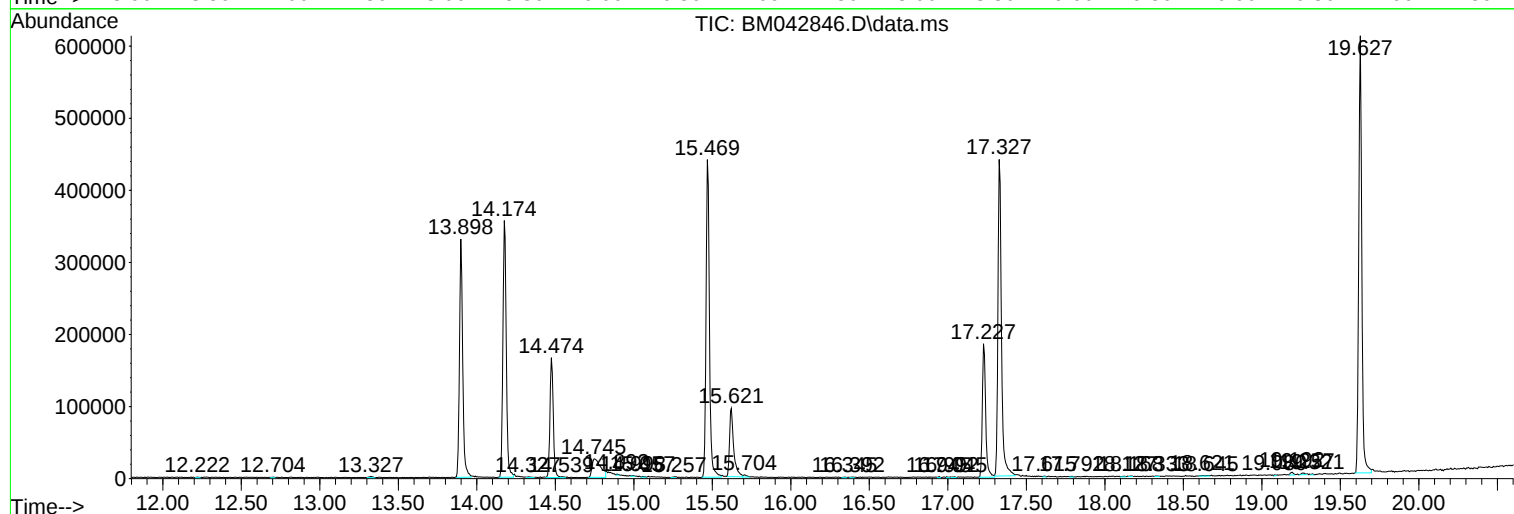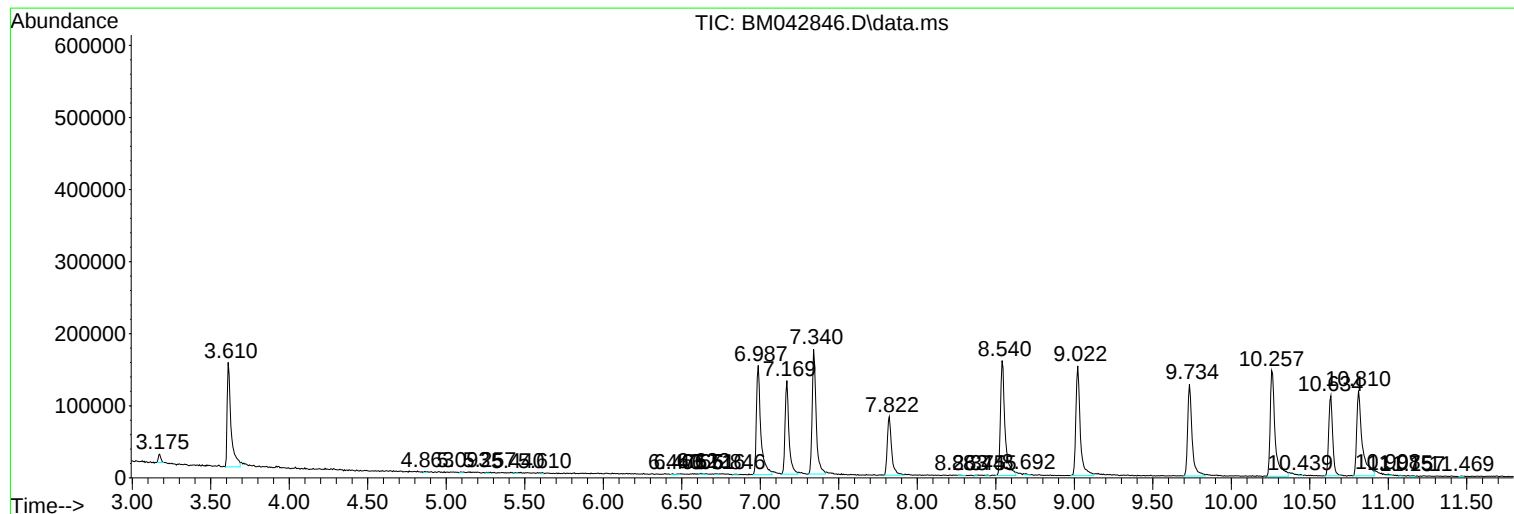

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042846.D
Acq On : 17 Nov 2023 16:13
Operator : MA/JU
Sample : PB157005BL
Misc :
ALS Vial : 87 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK005

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111323\
Data File : BM042846.D
Acq On : 17 Nov 2023 16:13
Operator : MA/JU
Sample : PB157005BL
Misc :
ALS Vial : 87 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK005

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM111323.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc