




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111324\
Data File : BM048672.D
Acq On : 14 Nov 2024 14:56
Operator : RC/JU
Sample : P4802-16
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GCPD6

Manual IntegrationsAPPROVED

Quant Time: Nov 14 15:41:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 13 11:38:55 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/15/2024
Supervised By :mohammad ahmed 11/15/2024

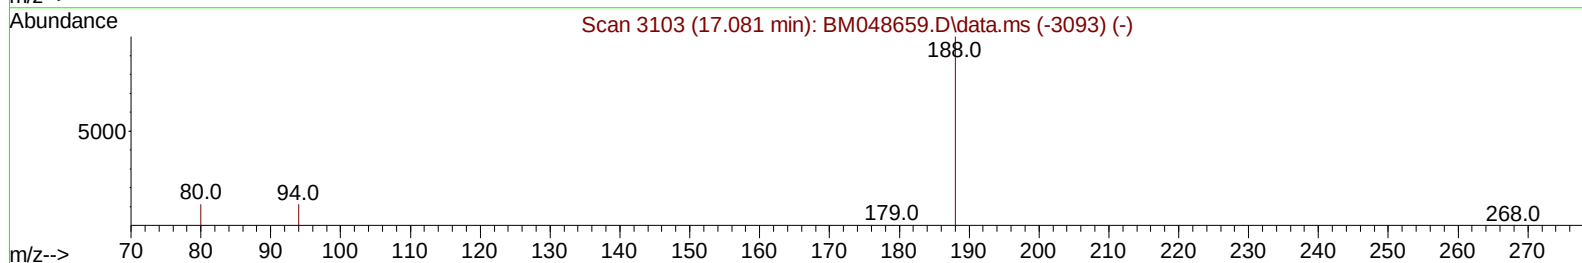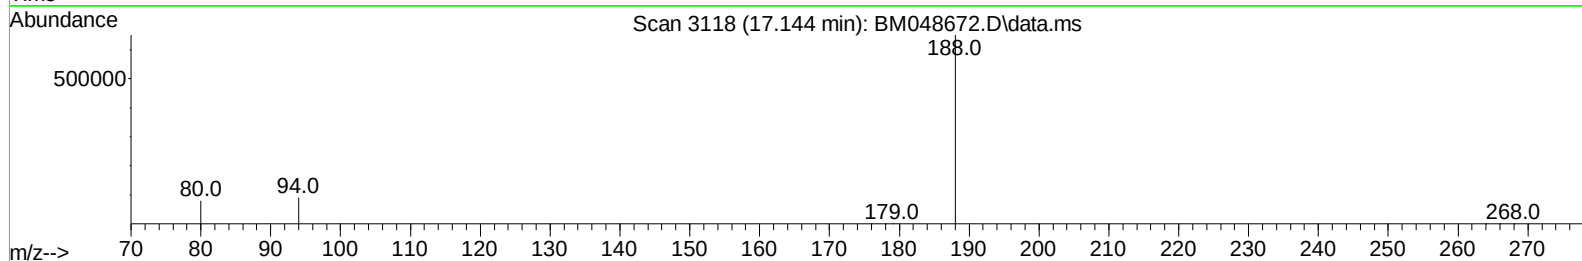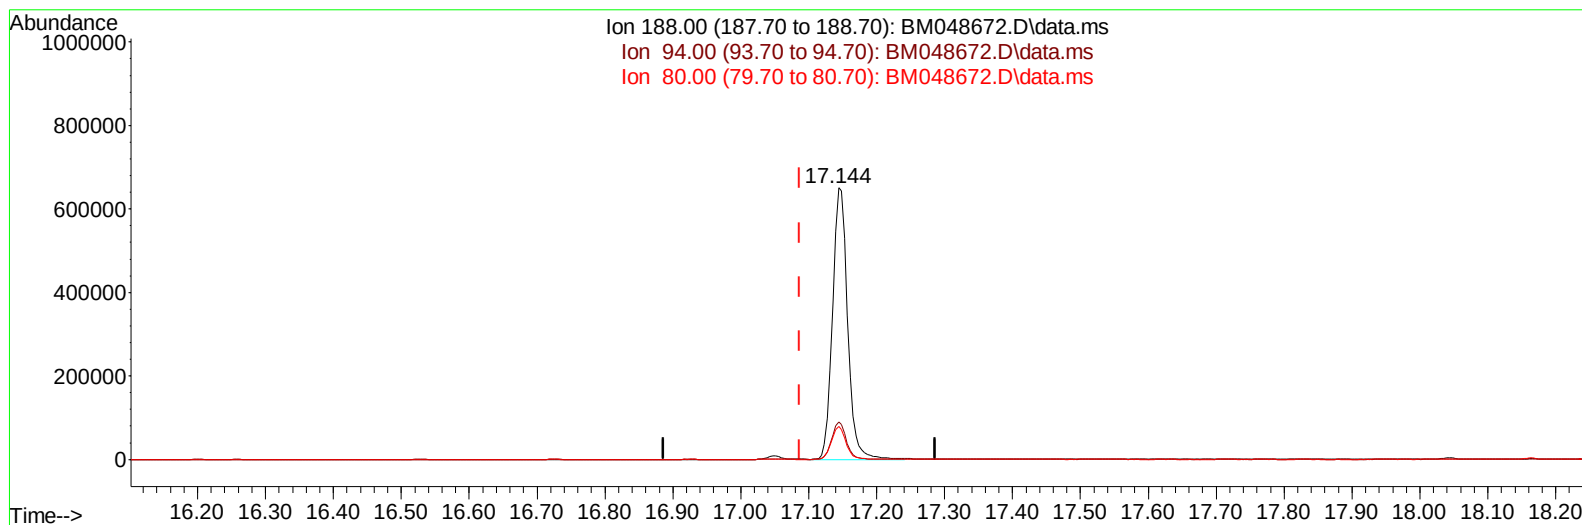

TIC: BM048672.D\data.ms

(13) Phenanthrene-d10 (I)

17.144min (+ 0.058) 0.40 ng/u1

response 1000896

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	12.00	13.87
80.00	12.60	12.14
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111324\
Data File : BM048672.D
Acq On : 14 Nov 2024 14:56
Operator : RC/JU
Sample : P4802-16
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GCPD6

Manual IntegrationsAPPROVED

Quant Time: Nov 14 15:41:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 13 11:38:55 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/15/2024
Supervised By :mohammad ahmed 11/15/2024

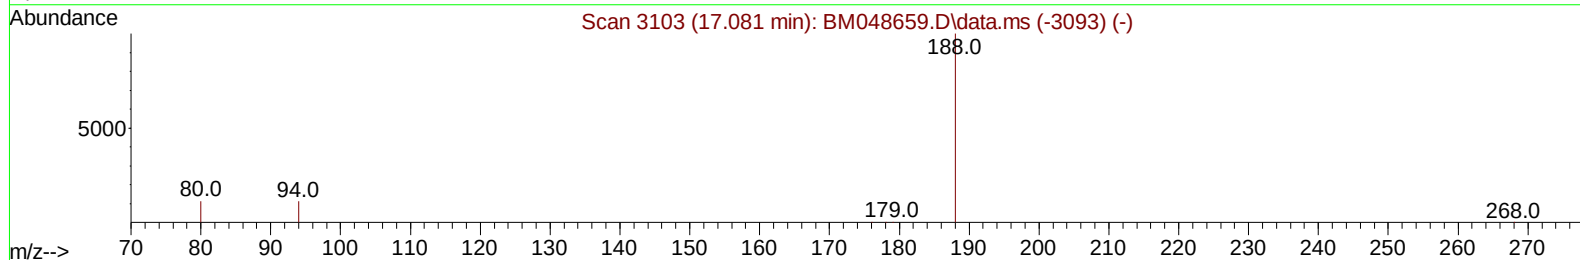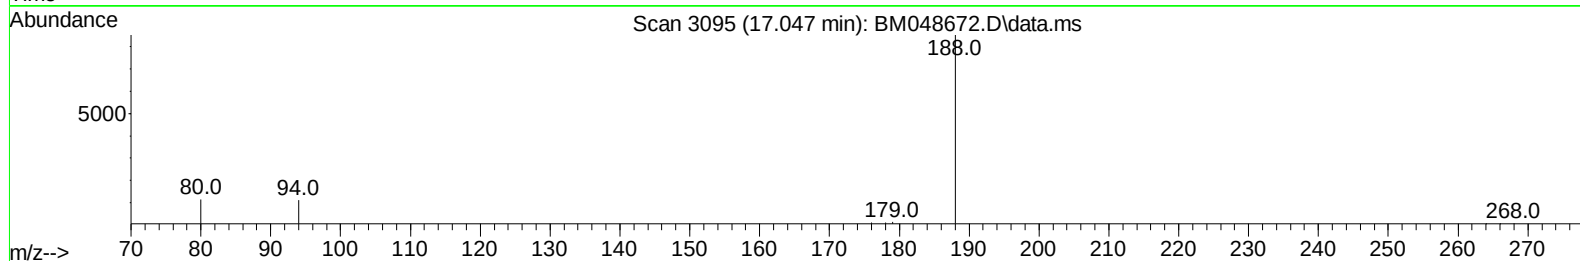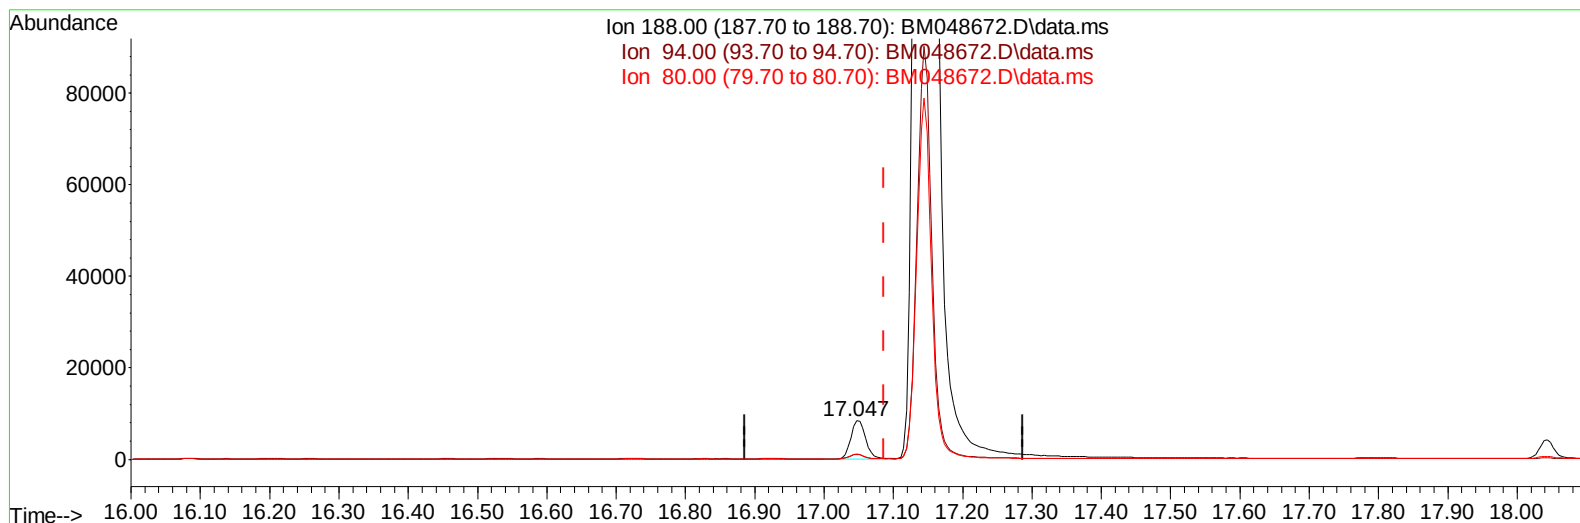

TIC: BM048672.D\data.ms

(13) Phenanthrene-d10 (I)

17.047min (-0.039) 0.40 ng/ul m

response 12627

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	12.00	13.26
80.00	12.60	13.49
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111324\
Data File : BM048672.D
Acq On : 14 Nov 2024 14:56
Operator : RC/JU
Sample : P4802-16
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GCPD6

Manual IntegrationsAPPROVED

Quant Time: Nov 14 15:41:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 13 11:38:55 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/15/2024
Supervised By :mohammad ahmed 11/15/2024

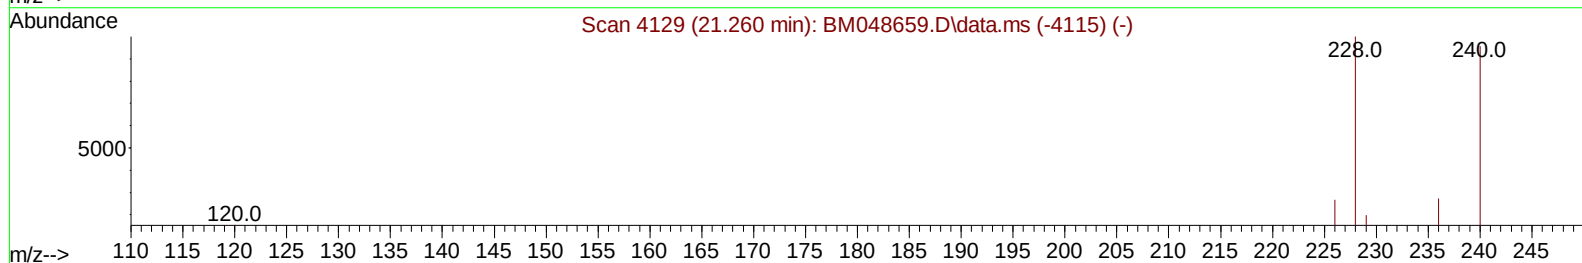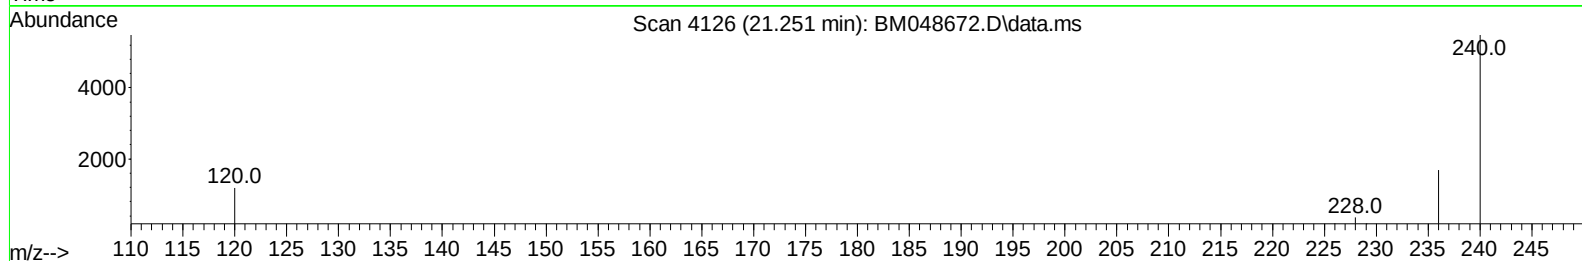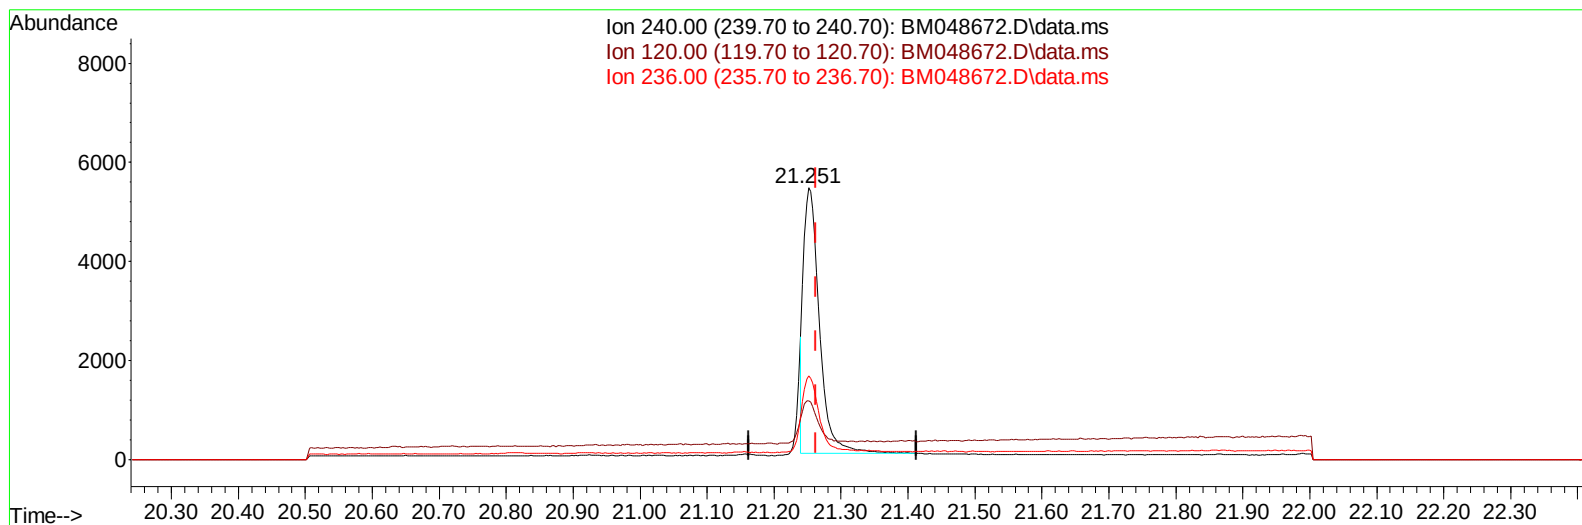

TIC: BM048672.D\data.ms

(17) Chrysene-d12

21.251min (-0.011) 0.40 ng/u1

response 8837

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	20.50	21.50
236.00	29.90	30.69
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111324\
Data File : BM048672.D
Acq On : 14 Nov 2024 14:56
Operator : RC/JU
Sample : P4802-16
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GCPD6

Manual IntegrationsAPPROVED

Quant Time: Nov 14 15:41:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 13 11:38:55 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/15/2024
Supervised By :mohammad ahmed 11/15/2024

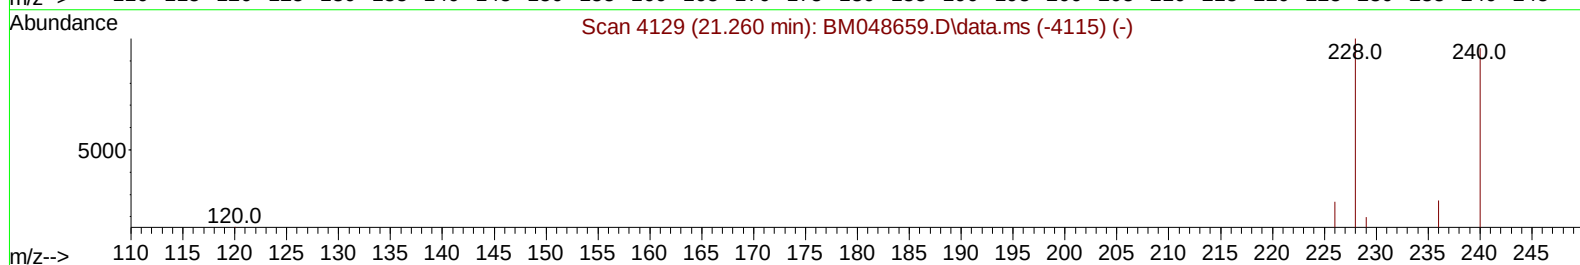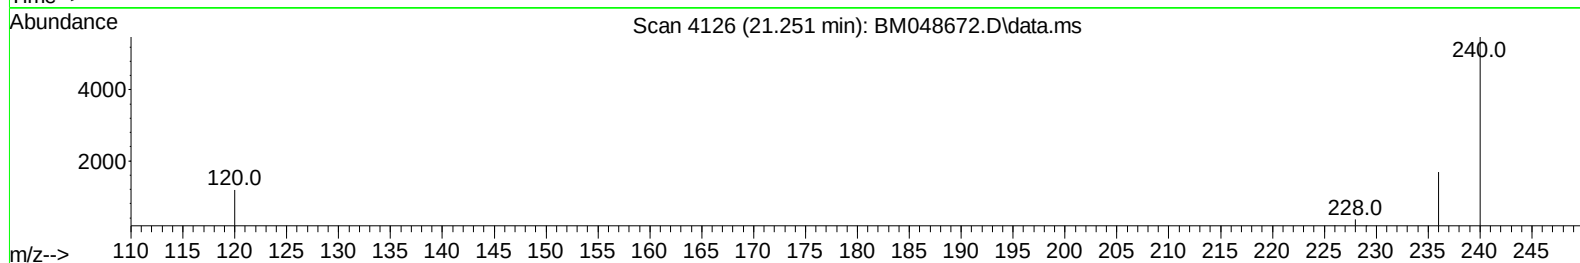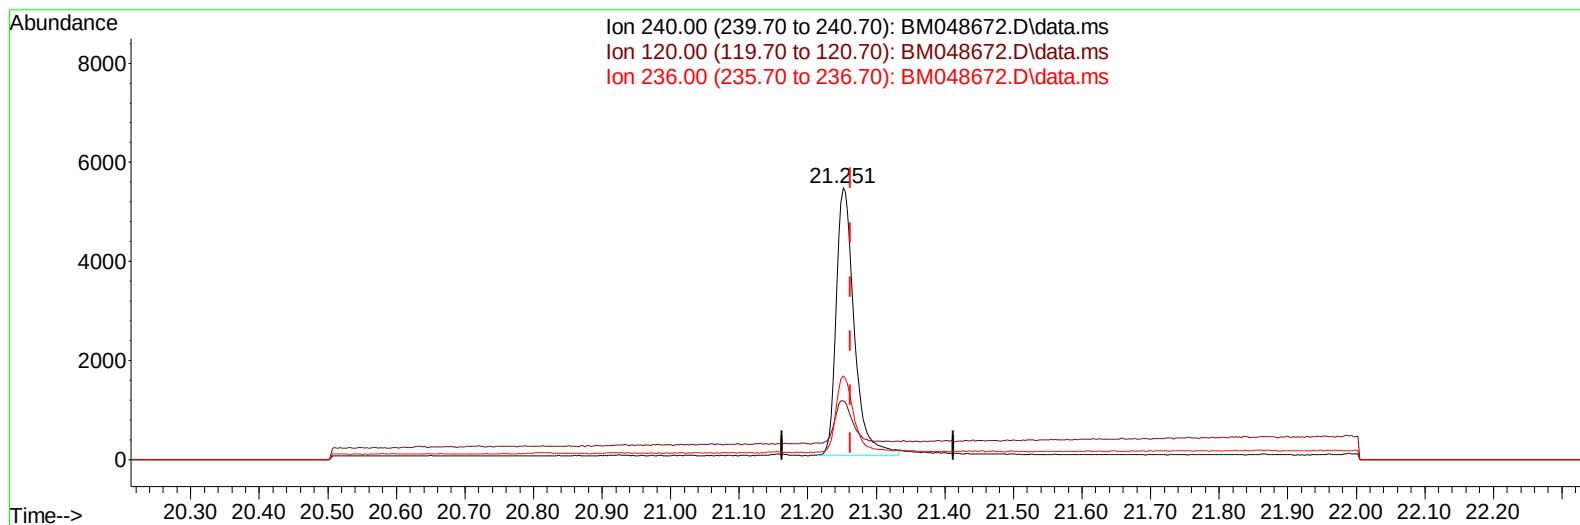

TIC: BM048672.D\data.ms

(17) Chrysene-d12

21.251min (-0.011) 0.40 ng/ul m

response 9836

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	20.50	21.50
236.00	29.90	30.69
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111324\
Data File : BM048672.D
Acq On : 14 Nov 2024 14:56
Operator : RC/JU
Sample : P4802-16
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GCPD6

Manual IntegrationsAPPROVED

Quant Time: Nov 14 15:41:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 13 11:38:55 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/15/2024
Supervised By :mohammad ahmed 11/15/2024

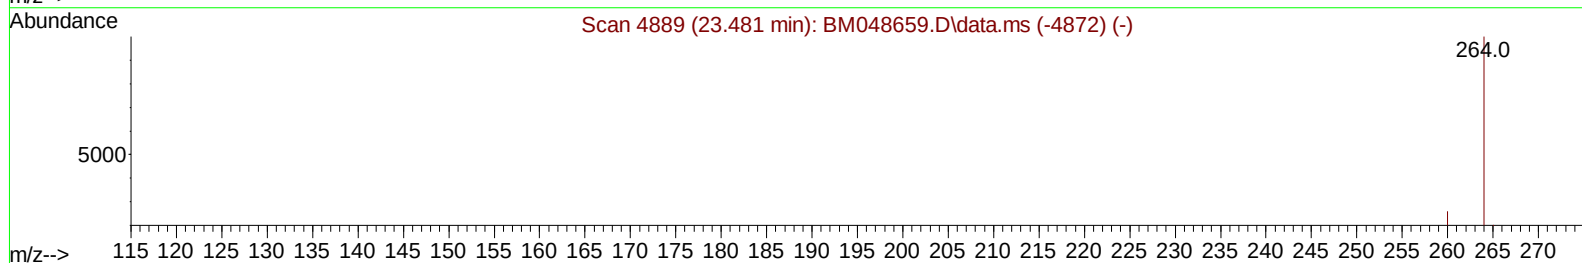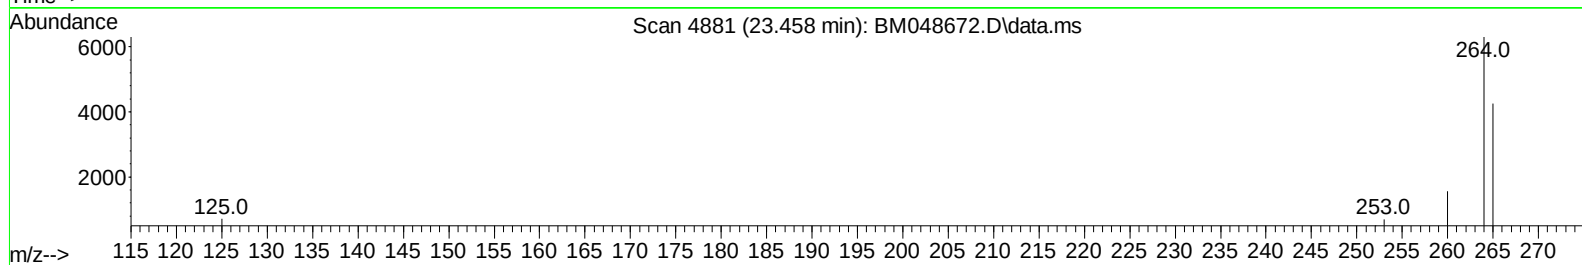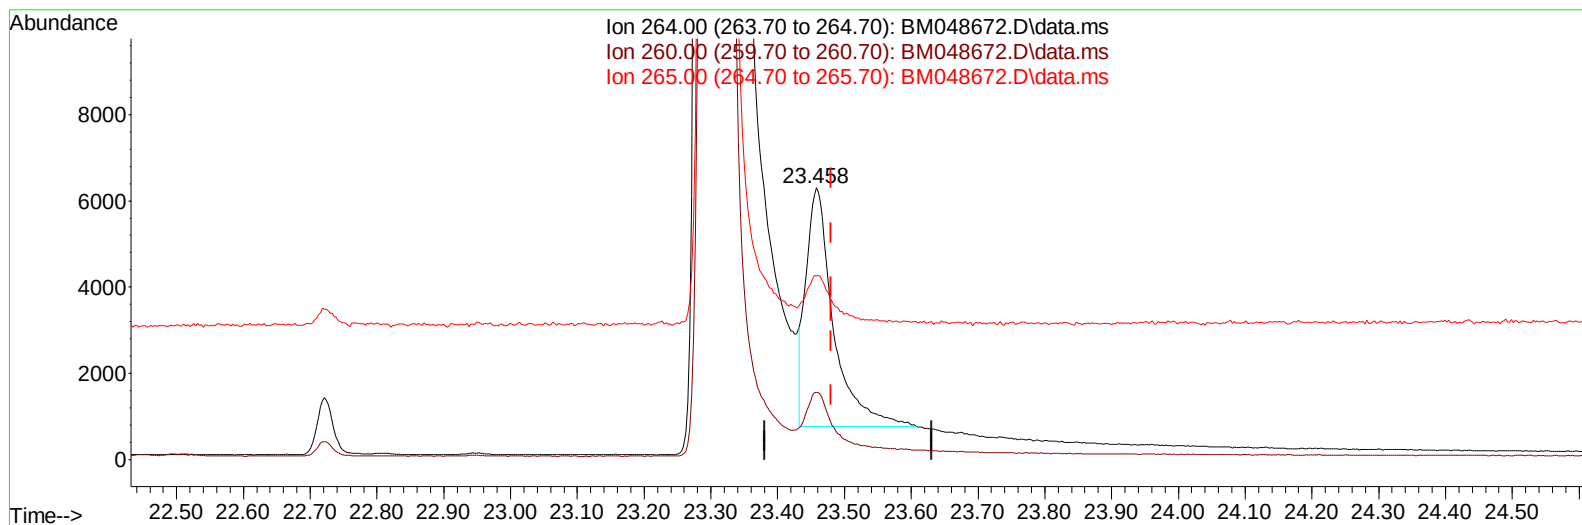

TIC: BM048672.D\data.ms

(23) Perylene-d12 (I)

23.458min (-0.023) 0.40 ng/u1

response 15989

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.30	24.67
265.00	119.80	67.57#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111324\
Data File : BM048672.D
Acq On : 14 Nov 2024 14:56
Operator : RC/JU
Sample : P4802-16
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GCPD6

Manual IntegrationsAPPROVED

Quant Time: Nov 14 15:41:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 13 11:38:55 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/15/2024
Supervised By :mohammad ahmed 11/15/2024

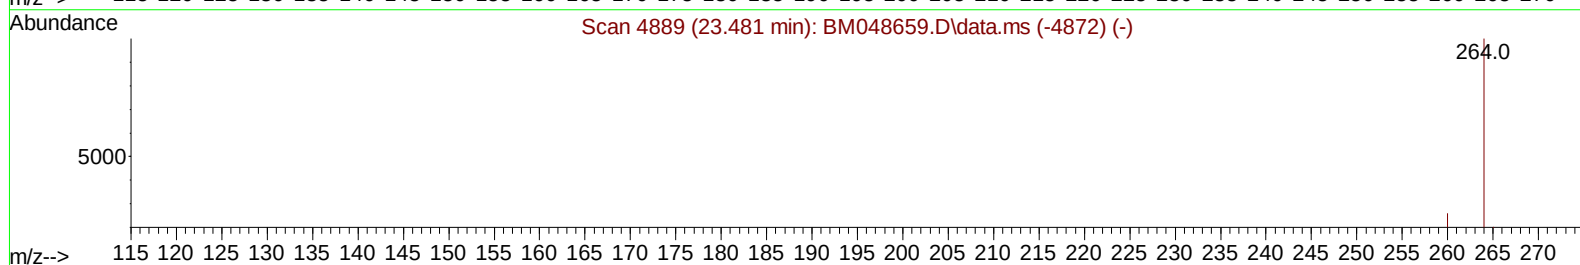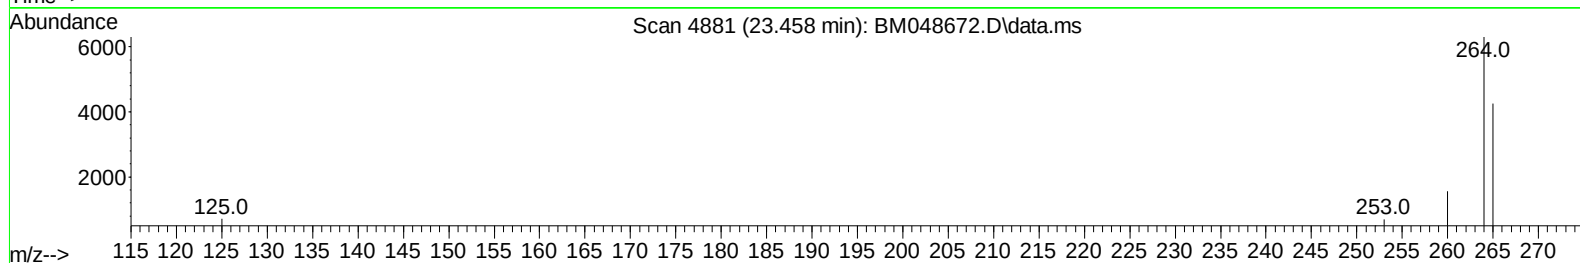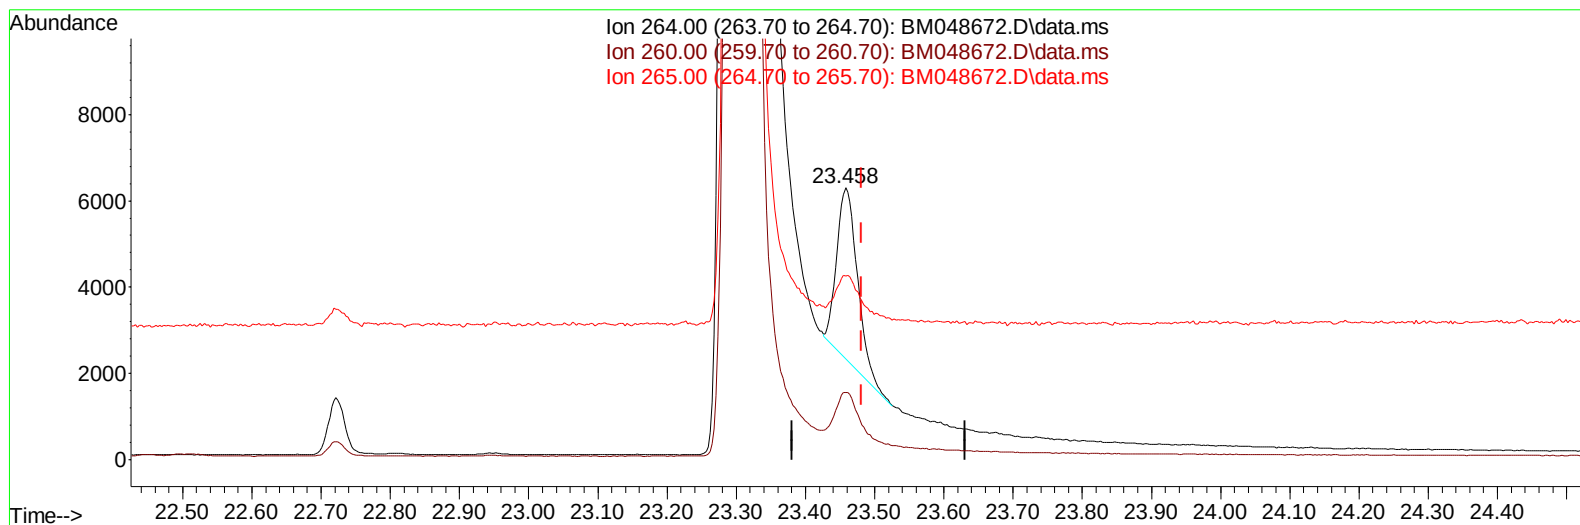

TIC: BM048672.D\data.ms

(23) Perylene-d12 (I)

23.458min (-0.023) 0.40 ng/ul m

response 8204

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.30	24.67
265.00	119.80	67.57#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111324\
 Data File : BM048672.D
 Acq On : 14 Nov 2024 14:56
 Operator : RC/JU
 Sample : P4802-16
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GCPD6

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/15/2024
 Supervised By :mohammad ahmed 11/15/2024

Quant Time: Nov 14 15:41:08 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 13 11:38:55 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.662	152	3534	0.400	ng/ul	-0.08
4) Naphthalene-d8	10.440	136	11430	0.400	ng/ul	-0.06
9) Acenaphthene-d10	14.302	164	5987	0.400	ng/ul	-0.02
13) Phenanthrene-d10	17.047	188	12627m	0.400	ng/ul	-0.04
17) Chrysene-d12	21.251	240	9836m	0.400	ng/ul	-0.01
23) Perylene-d12	23.458	264	8204m	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.122	96	24506	5.748	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.063	152	4567	0.309	ng/ul	-0.04
18) Fluoranthene-d10	19.080	212	12557	0.455	ng/ul	-0.03

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111324\
Data File : BM048672.D
Acq On : 14 Nov 2024 14:56
Operator : RC/JU
Sample : P4802-16
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GCPD6

Manual IntegrationsAPPROVED

Quant Time: Nov 14 15:41:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 13 11:38:55 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/15/2024
Supervised By :mohammad ahmed 11/15/2024

