

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111324\
 Data File : BM048663.D
 Acq On : 14 Nov 2024 09:32
 Operator : RC/JU
 Sample : P4777-01
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH7N7

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/15/2024
 Supervised By :mohammad ahmed 11/15/2024

Quant Time: Nov 14 10:07:33 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 13 11:38:55 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.661	152	3880	0.400	ng/ul	-0.08
4) Naphthalene-d8	10.440	136	11894	0.400	ng/ul	-0.06
9) Acenaphthene-d10	14.306	164	6127	0.400	ng/ul	-0.02
13) Phenanthrene-d10	17.051	188	12473m	0.400	ng/ul	-0.04
17) Chrysene-d12	21.266	240	9166m	0.400	ng/ul	0.00
23) Perylene-d12	23.461	264	6466m	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.122	96	20783	4.440	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.068	152	4562	0.297	ng/ul	-0.03
18) Fluoranthene-d10	19.084	212	11332	0.440	ng/ul	-0.02
Target Compounds					Qvalue	
2) 1,4-Dioxane	3.155	88	3472	0.645	ng/ul#	70

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111324\
Data File : BM048663.D
Acq On : 14 Nov 2024 09:32
Operator : RC/JU
Sample : P4777-01
Misc :
ALS Vial : 43 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
BH7N7

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/15/2024
Supervised By :mohammad ahmed 11/15/2024


Quant Time: Nov 14 10:07:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 13 11:38:55 2024
Response via : Initial Calibration

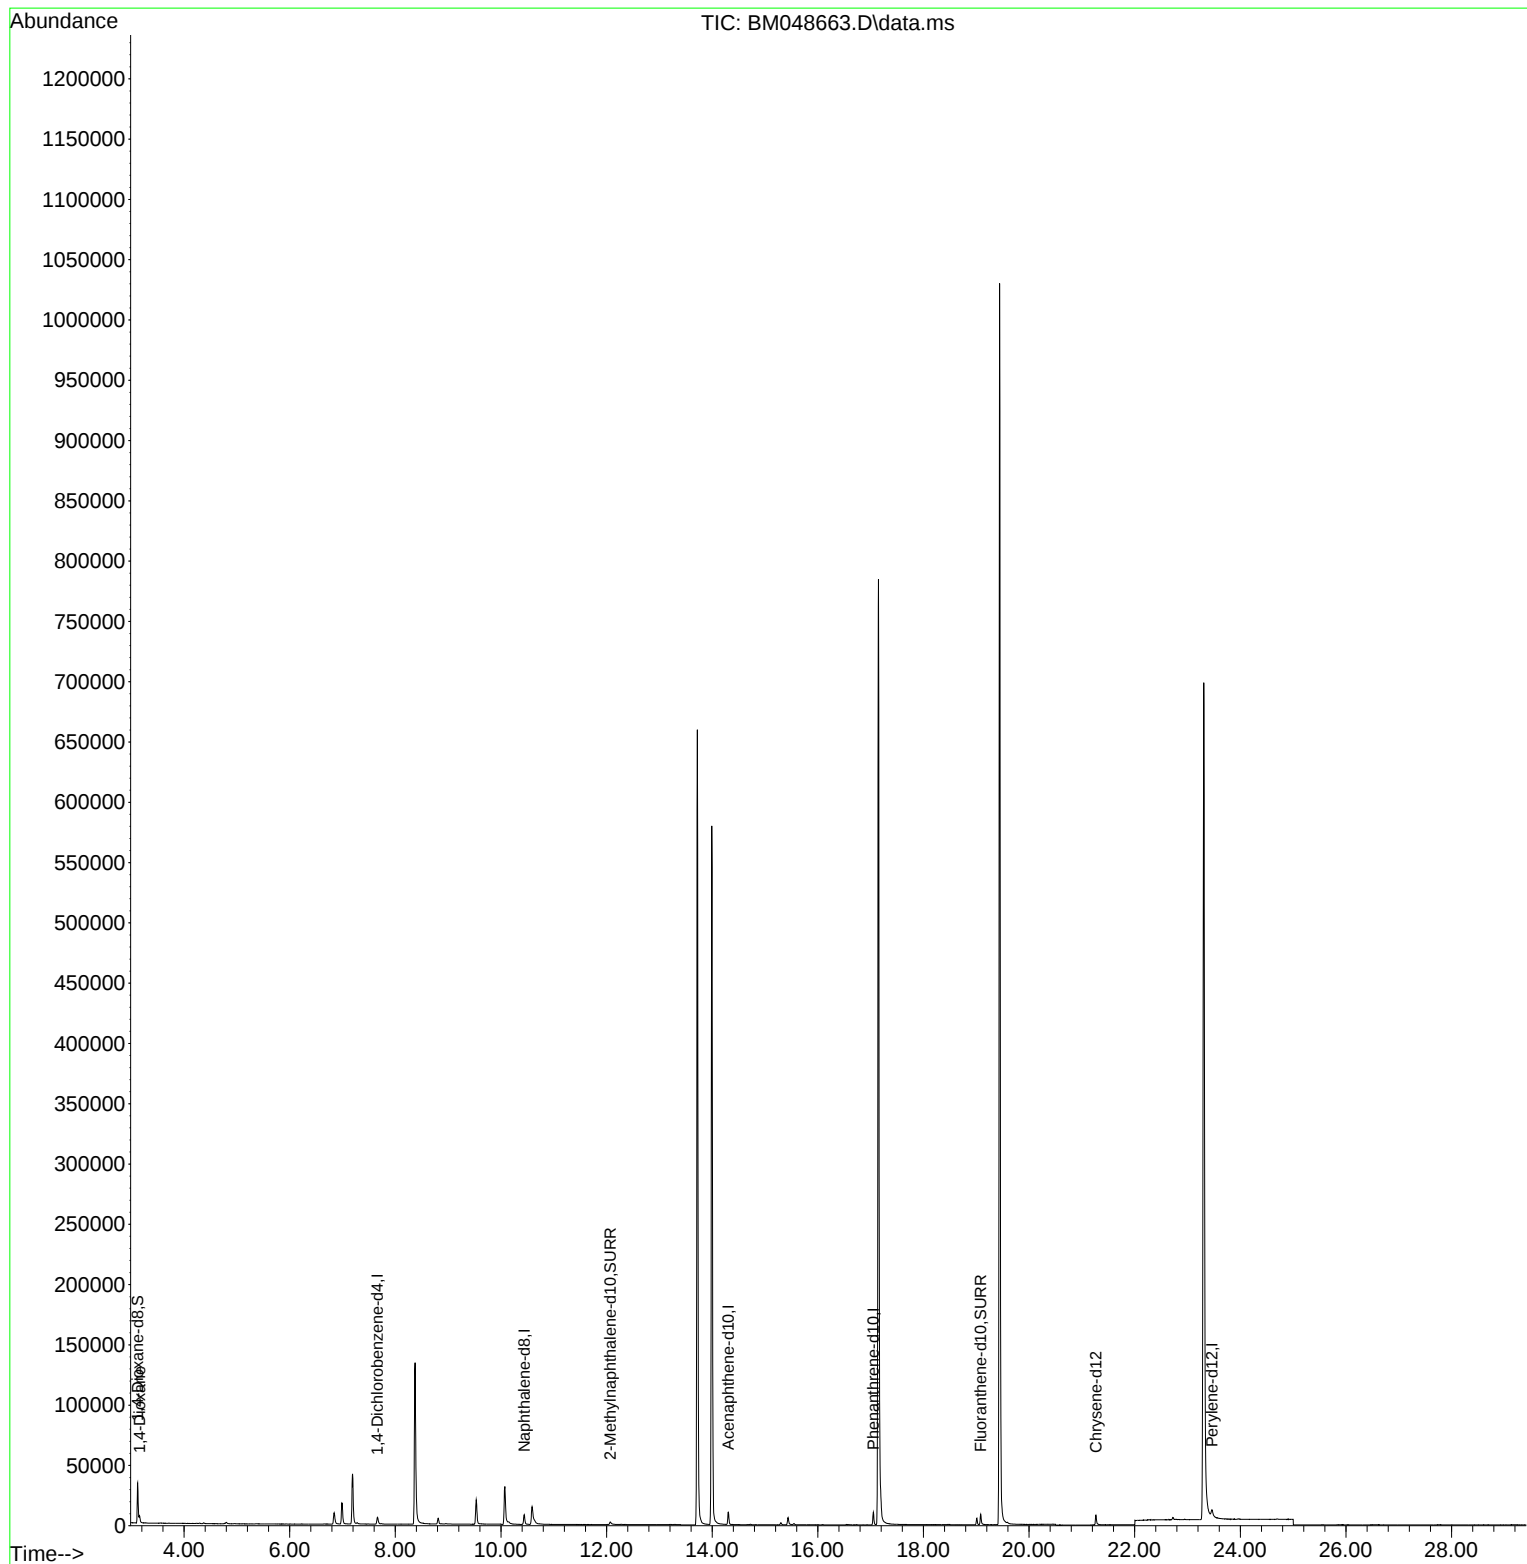

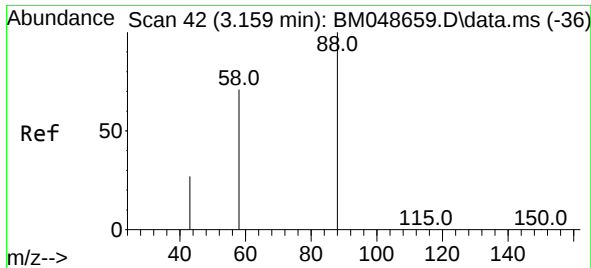

#2
 1,4-Dioxane
 Concen: 0.645 ng/ul
 RT: 3.155 min Scan# 41
 Delta R.T. -0.009 min
 Lab File: BM048663.D
 Acq: 14 Nov 2024 09:32

Instrument :
 BNA_M
 ClientSampleId :
 BH7N7

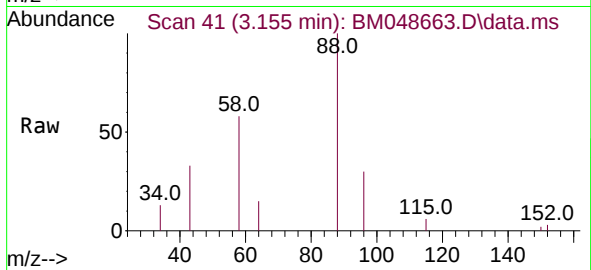

Tgt Ion: 88 Resp: 3472
 Ion Ratio Lower Upper
 88 100
 43 33.2 60.2 90.4
 58 58.5 44.2 66.2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/15/2024
 Supervised By :mohammad ahmed 11/15/2024

