

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111324\
 Data File : BM048680.D
 Acq On : 14 Nov 2024 19:45
 Operator : RC/JU
 Sample : P4777-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH7N7

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/15/2024
 Supervised By :mohammad ahmed 11/15/2024

Quant Time: Nov 14 22:23:08 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 13 11:38:55 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.661	152	3965	0.400	ng/ul	-0.08
4) Naphthalene-d8	10.436	136	12456	0.400	ng/ul	-0.06
9) Acenaphthene-d10	14.303	164	6572	0.400	ng/ul	#-0.02
13) Phenanthrene-d10	17.048	188	13780m	0.400	ng/ul	-0.04
17) Chrysene-d12	21.265	240	10789m	0.400	ng/ul	0.00
23) Perylene-d12	23.463	264	8203m	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.122	96	20867	4.362	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.069	152	4869	0.302	ng/ul	-0.03
18) Fluoranthene-d10	19.086	212	12718	0.420	ng/ul	-0.02
Target Compounds					Qvalue	
2) 1,4-Dioxane	3.155	88	3492	0.635	ng/ul#	72

(#) = qualifier out of range (m) = manual integration (+) = signals summed


```
Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111324\
Data File : BM048680.D
Acq On    : 14 Nov 2024   19:45
Operator  : RC/JU
Sample    : P4777-01
Misc      :
ALS Vial  : 5   Sample Multiplier: 1
```


Instrument :
BNA_M
ClientSampleId :
BH7N7

Manual Integrations

Reviewed By :Yogesh Patel 11/15/2024
Supervised By :mohammad ahmed 11/15/2024


Quant Time: Nov 14 22:23:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 13 11:38:55 2024
Response via : Initial Calibration

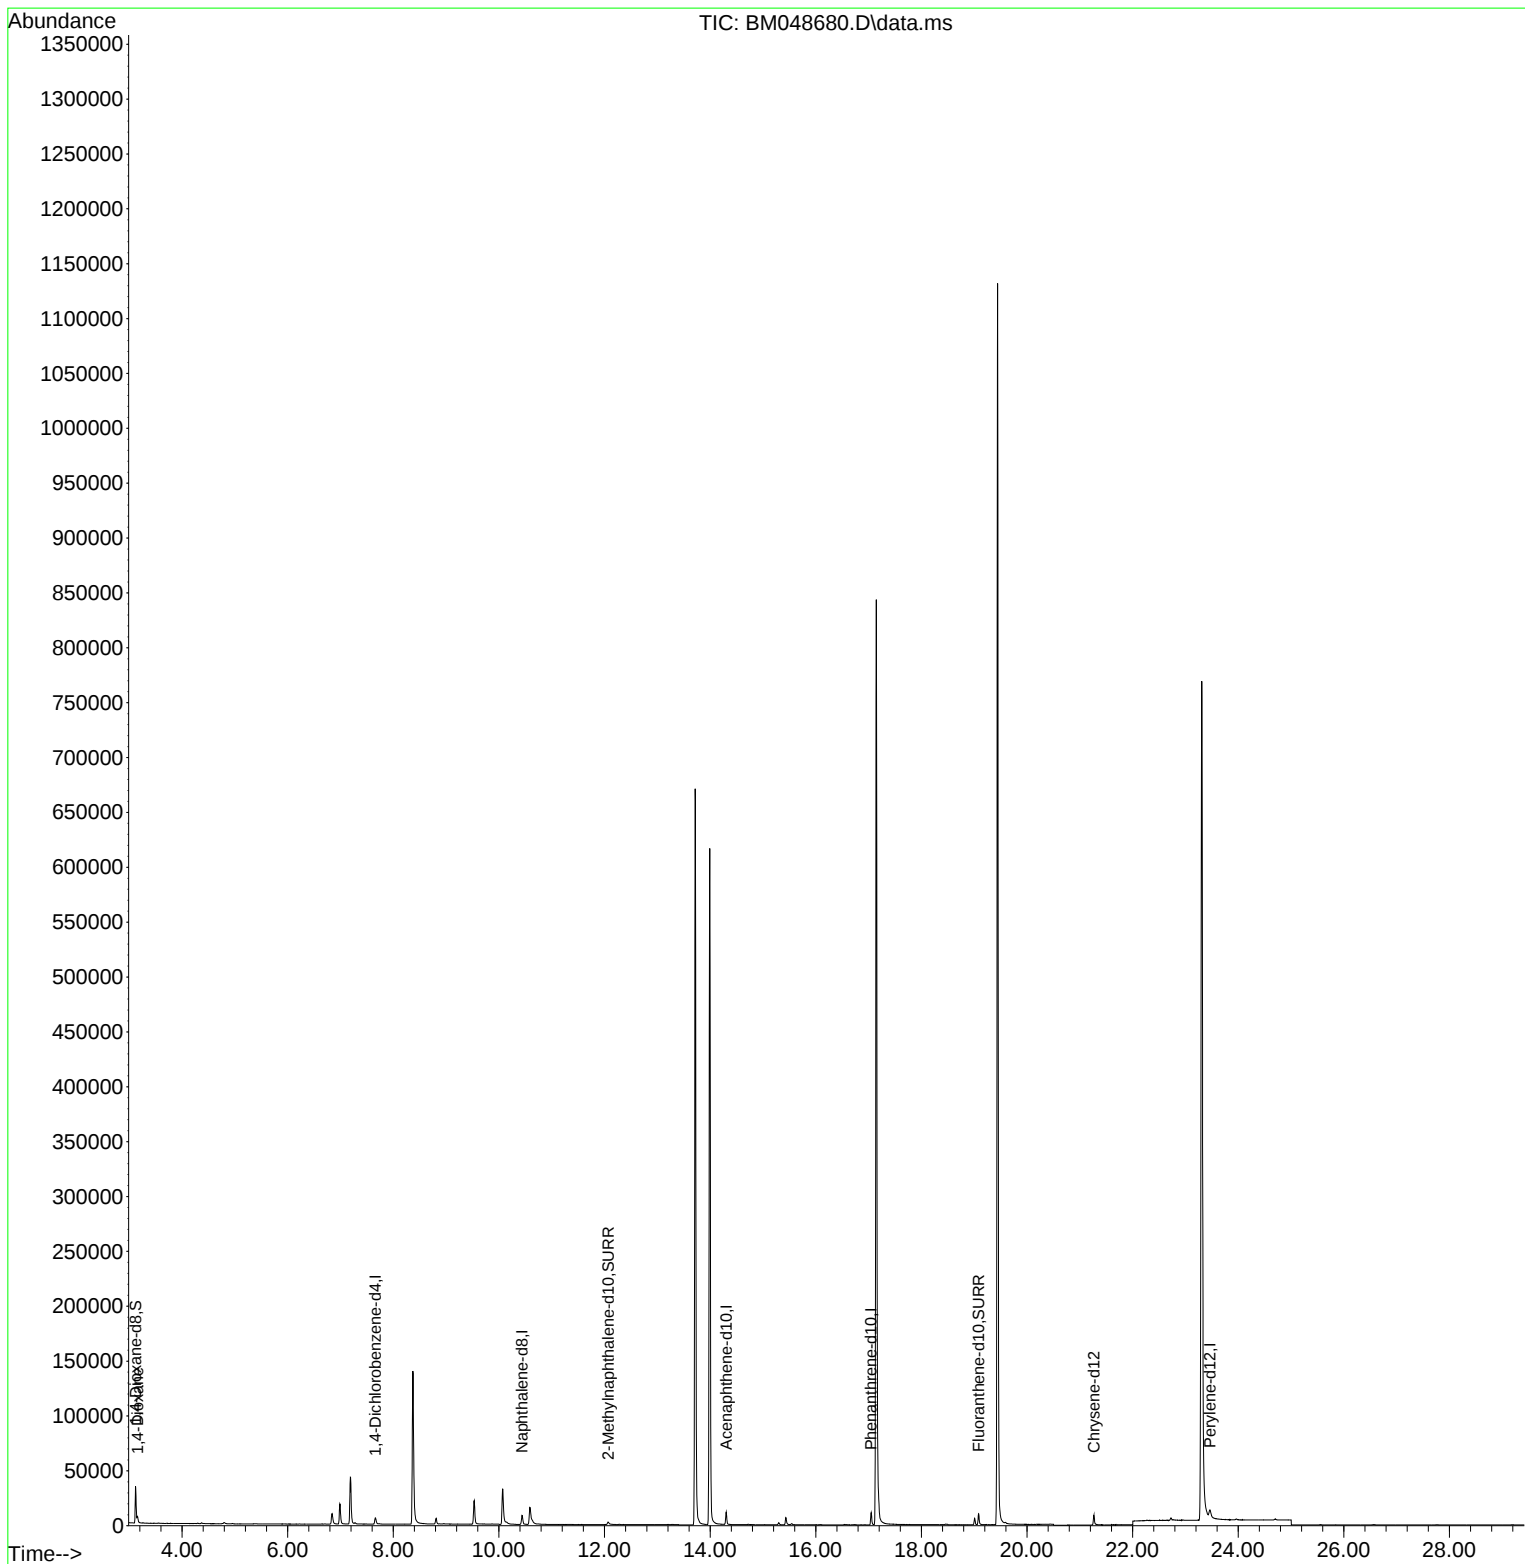

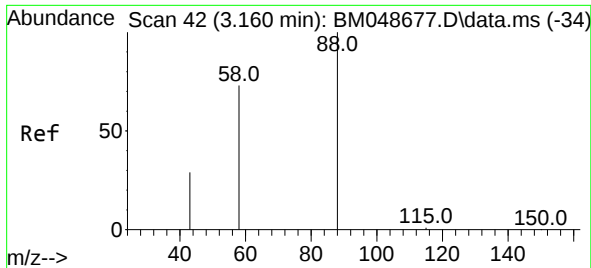

#2
 1,4-Dioxane
 Concen: 0.635 ng/ul
 RT: 3.155 min Scan# 41
 Delta R.T. -0.009 min
 Lab File: BM048680.D
 Acq: 14 Nov 2024 19:45

Instrument :
 BNA_M
 ClientSampleId :
 BH7N7

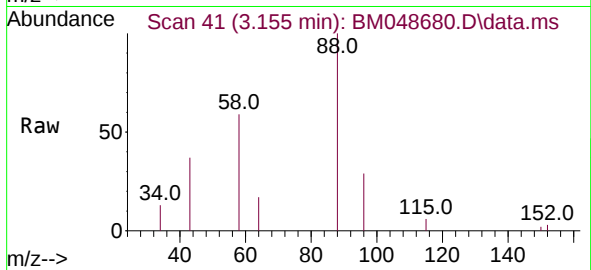

Tgt Ion: 88 Resp: 3492
 Ion Ratio Lower Upper
 88 100
 43 37.3 60.2 90.4
 58 58.6 44.2 66.2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/15/2024
 Supervised By :mohammad ahmed 11/15/2024

