

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111324\
 Data File : BM048684.D
 Acq On : 14 Nov 2024 22:09
 Operator : RC/JU
 Sample : P4802-04
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GCPC6

Manual Integrations
 APPROVED

Reviewed By :Yogesh
 Patel

Quant Time: Nov 14 22:38:27 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 13 11:38:55 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)	
Internal Standards							11/15/2024
1) 1,4-Dichlorobenzene-d4	7.662	152	3285	0.400	ng/ul	-0.08	Supervised By :mohammad
4) Naphthalene-d8	10.436	136	10464	0.400	ng/ul	-0.06	Summed
9) Acenaphthene-d10	14.303	164	5556	0.400	ng/ul	#-0.02	
13) Phenanthrene-d10	17.048	188	11674m	0.400	ng/ul	-0.04	
17) Chrysene-d12	21.266	240	9328m	0.400	ng/ul	0.00	
23) Perylene-d12	23.463	264	6391m	0.400	ng/ul	-0.02	11/15/2024
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.118	96	19273	4.863	ng/ul	-0.01	
6) 2-Methylnaphthalene-d10	12.069	152	4223	0.312	ng/ul	-0.03	
18) Fluoranthene-d10	19.086	212	10642	0.406	ng/ul	-0.02	
Target Compounds							Qvalue
2) 1,4-Dioxane	3.155	88	4686	1.029	ng/ul#	67	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111324\
Data File : BM048684.D
Acq On : 14 Nov 2024 22:09
Operator : RC/JU
Sample : P4802-04
Misc :
ALS Vial : 9 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
GCPC6

Manual Integrations
APPROVED

Reviewed By :Yogesh
Patel


Quant Time: Nov 14 22:38:27 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 13 11:38:55 2024
Response via : Initial Calibration

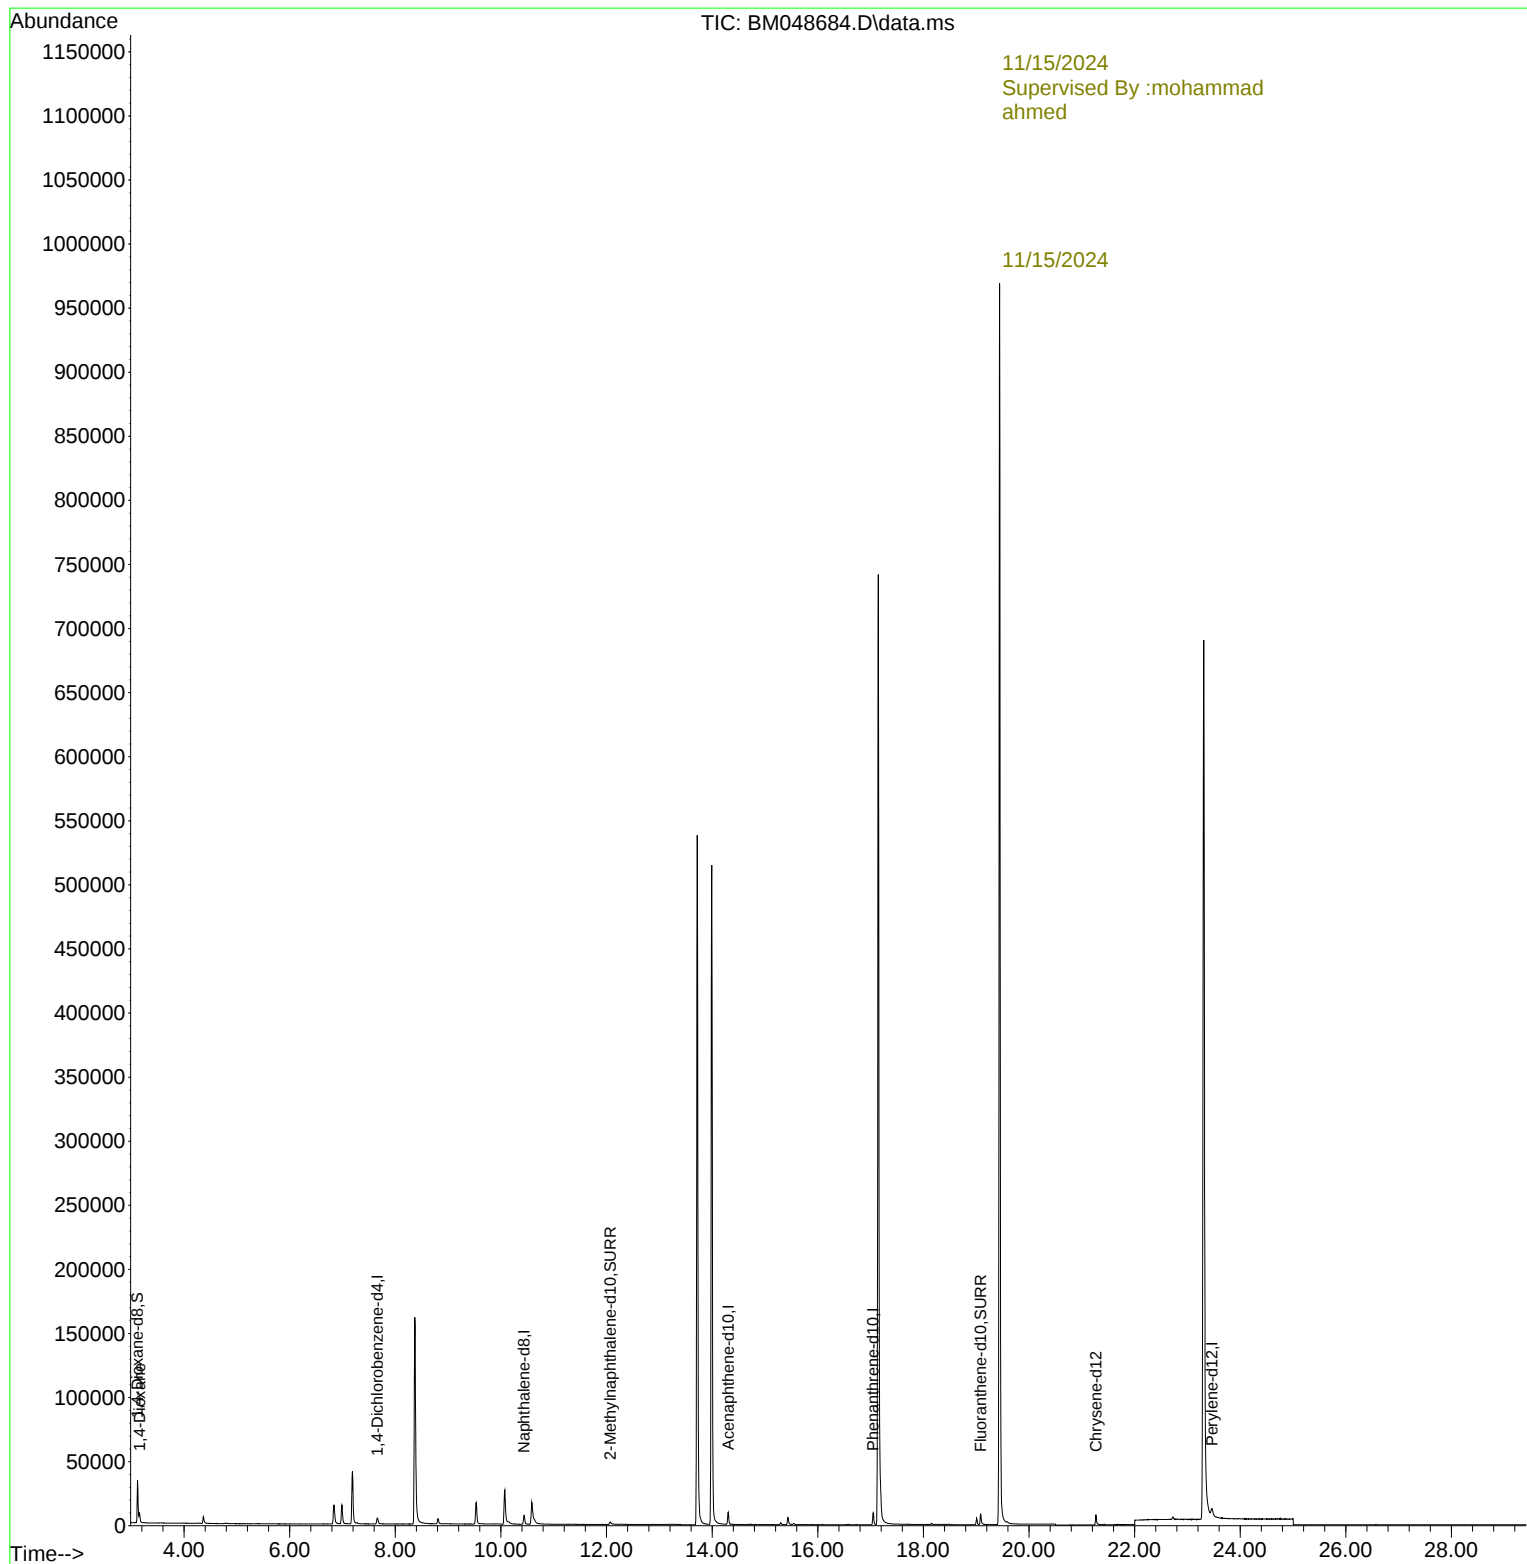

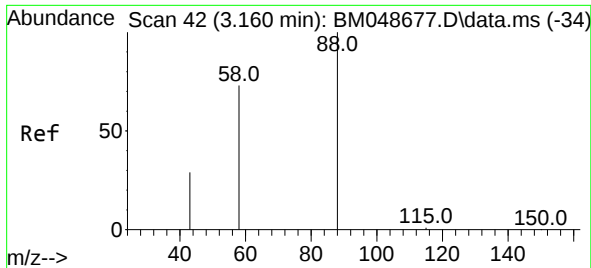

#2
 1,4-Dioxane
 Concen: 1.029 ng/ul
 RT: 3.155 min Scan# 41
 Delta R.T. -0.008 min
 Lab File: BM048684.D
 Acq: 14 Nov 2024 22:09

Instrument :
 BNA_M
 ClientSampleId :
 GCPC6

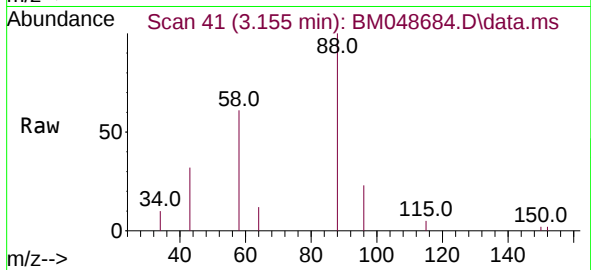

Tgt Ion: 88 Resp: 4680
 Ion Ratio Lower Upper
 88 100
 43 31.6 60.2 90.4
 58 60.8 44.2 66.2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/15/2024
 Supervised By :mohammad ahmed 11/15/2024

