
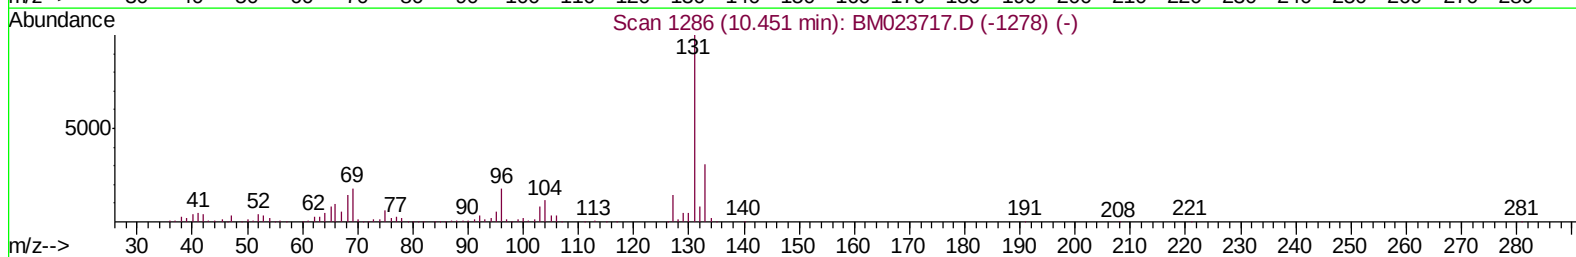
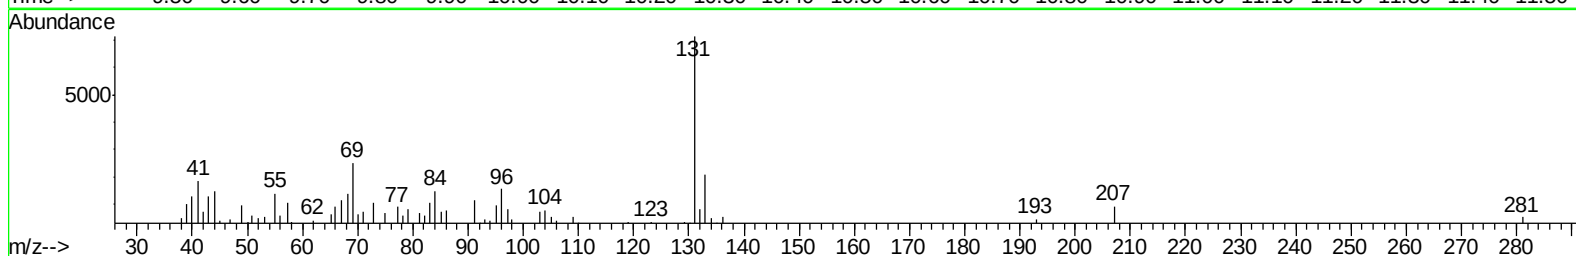


Data File : BM023720.D
Acq On : 14 Nov 2019 17:16
Operator : JU
Sample : K5678-08
Misc :
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Nov 15 06:33:00 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM11119MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 15 06:30:14 2019
Response via : Initial Calibration

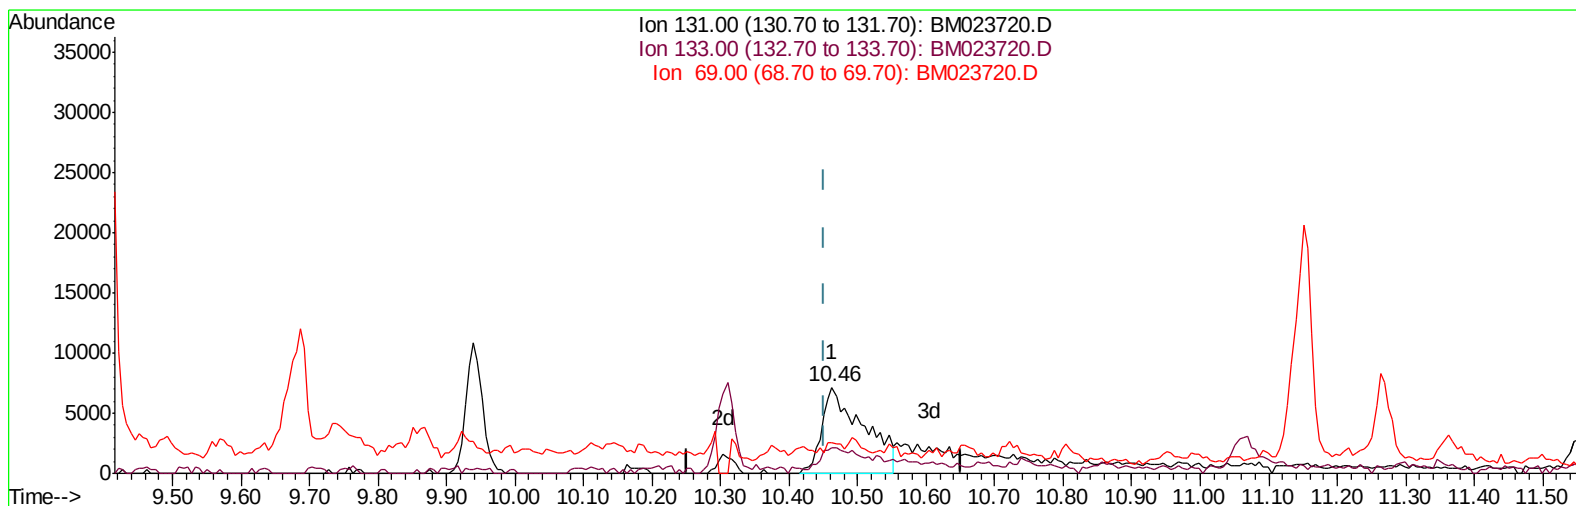

TIC: BM023720.D

(29) 4-Chloroaniline-d4 (S)

10.463min (+0.012) 1.01ng/ul m

response 29997

Ion	Exp%	Act%
131.00	100	100
133.00	32.50	29.25
69.00	19.60	35.15#
0.00	0.00	0.00