
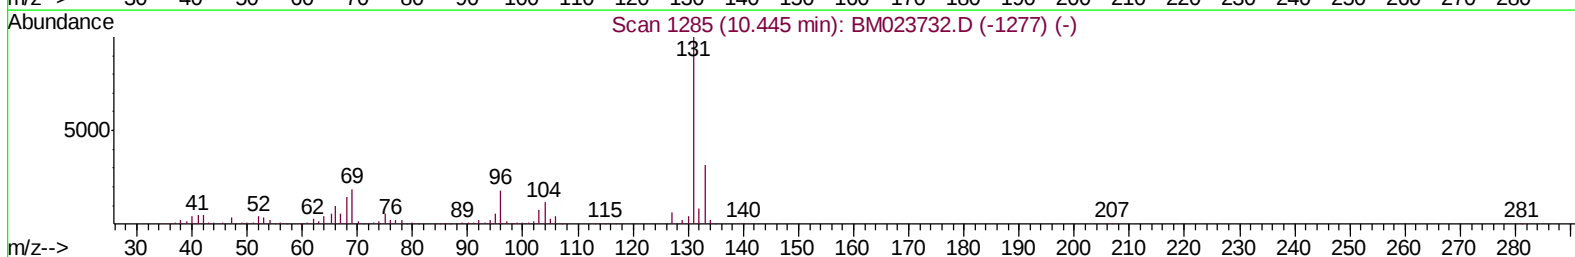
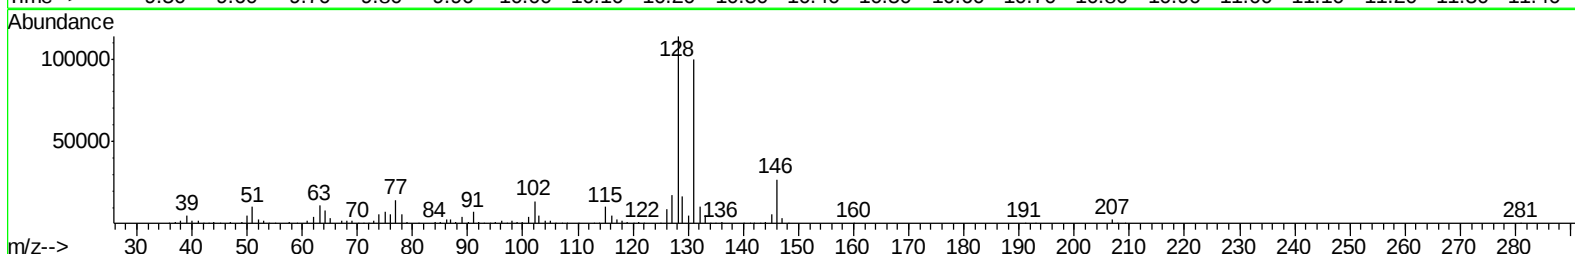


Data File : BM023737.D
Acq On : 15 Nov 2019 04:06
Operator : JU
Sample : K5700-15
Misc :
ALS Vial : 21 Sample Multiplier: 1

Quant Time: Nov 15 07:57:48 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM11119MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 15 07:53:56 2019
Response via : Initial Calibration

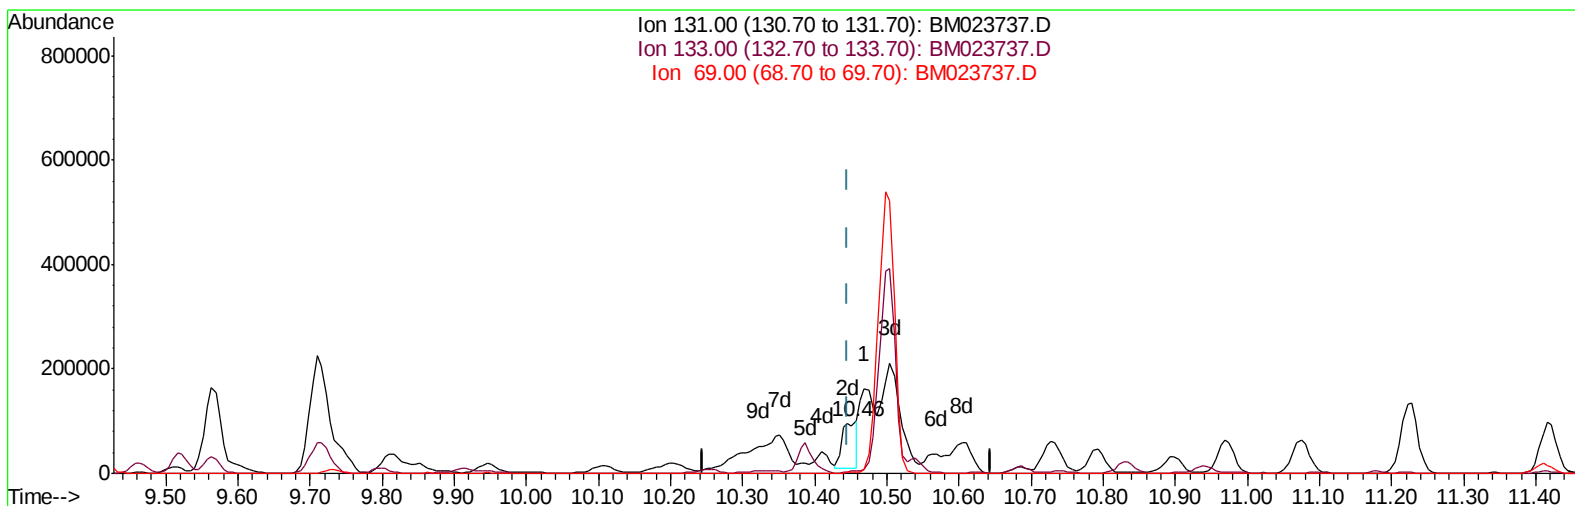

TIC: BM023737.D

(29) 4-Chloroaniline-d4 (S)

10.457min (+0.012) 4.64ng/ul m

response 124615

Ion	Exp%	Act%
131.00	100	100
133.00	32.50	4.77#
69.00	19.60	2.18#
0.00	0.00	0.00